

---

**User's  
Manual**

**AQ6370C/AQ6370D/AQ6373/  
AQ6373B/AQ6375  
Optical Spectrum Analyzer  
Remote Control**

---

---

## Foreword

Thank you for purchasing the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 Optical Spectrum Analyzer. This remote control user's manual covers the AQ6370C, AQ6370D, AQ6373, AQ6373B and AQ6375.

It describes the following.

- GP-IB Interface
- RS-232 Interface
- Ethernet Interface and Communication Commands
- Program Functions

To ensure correct use, please read this manual thoroughly before beginning operation.

After reading this manual, keep it in a convenient location for quick reference in the event a question arises during operation. In addition to this manual, there is one individual manual each for the AQ6370C, AQ6370D, AQ6373, AQ6373B and AQ6375. Read them along with this manual.

### AQ6370C

Manual Title	Manual No.	Description
AQ6370C Optical Spectrum Analyzer User's Manual	IM AQ6370C-01EN	The manual is located on the CD included in your package (pdf format). Explains all functions and operating procedures of the AQ6370C except remote control and program functions.
AQ6370C Optical Spectrum Analyzer Getting Started Guide	IM AQ6370C-02EN	Explains the handling precautions, installation procedure, component names, and specifications of the AQ6370C.

### AQ6370D

Manual Title	Manual No.	Description
AQ6370D Optical Spectrum Analyzer User's Manual	IM AQ6370D-01EN	The manual is located on the CD included in your package (pdf format). Explains all functions and operating procedures of the AQ6370D except remote control and program functions.
AQ6370D Optical Spectrum Analyzer Getting Started Guide	IM AQ6370D-02EN	Explains the handling precautions, installation procedure, component names, and specifications of the AQ6370D.

### AQ6373

Manual Title	Manual No.	Description
AQ6373 Optical Spectrum Analyzer User's Manual	IM AQ6373-01EN	The manual is located on the CD included in your package (pdf format). Explains all functions and operating procedures of the AQ6373 except remote control and program functions.
AQ6373 Optical Spectrum Analyzer Getting Started Guide	IM AQ6373-02EN	Explains the handling precautions, installation procedure, component names, and specifications of the AQ6373.

### AQ6373B

Manual Title	Manual No.	Description
AQ6373B Optical Spectrum Analyzer User's Manual	IM AQ6373B-01EN	The manual is located on the CD included in your package (pdf format). Explains all functions and operating procedures of the AQ6373B except remote control and program functions.
AQ6373B Optical Spectrum Analyzer Getting Started Guide	IM AQ6373B-02EN	Explains the handling precautions, installation procedure, component names, and specifications of the AQ6373B.

### AQ6375

Manual Title	Manual No.	Description
AQ6375 Optical Spectrum Analyzer User's Manual	IM AQ6375-01EN	The manual is located on the CD included in your package (pdf format). Explains all functions and operating procedures of the AQ6375 except remote control and program functions.
AQ6375 Optical Spectrum Analyzer Getting Started Guide	IM AQ6375-02EN	Explains the handling precautions, installation procedure, component names, and specifications of the AQ6375.

## Notes

- The contents of this manual are subject to change without prior notice as a result of improvements in the instrument's performance and functions. Display contents illustrated in this manual may differ slightly from what actually appears on your screen.
- Every effort has been made in the preparation of this manual to ensure the accuracy of its contents. However, should you have any questions or find any errors, please contact your nearest YOKOGAWA dealer.
- Copying or reproducing all or any part of the contents of this manual without the permission of Yokogawa Meters&Instruments Corporation is strictly prohibited.

## Trademarks

- Microsoft and Windows are registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.
- Adobe and Acrobat are registered trademarks or trademarks of Adobe Systems incorporated.
- The company and product names used in this manual are not accompanied by the registered trademark or trademark symbols (® and TM).
- Other company and product names are registered trademarks or trademarks of their respective companies.

## Revisions

- 1st Edition September, 2010
- 2nd Edition January, 2011
- 3rd Edition October, 2011
- 4th Edition April, 2014
- 5th Edition March, 2015
- 6th Edition July, 2015

# Safety Precautions

This instrument is an IEC protection class I instrument (provided with terminal for protective earth grounding).

The general safety precautions described herein must be observed during all phases of operation. If the instrument is used in a manner not specified in this manual, the protection provided by the instrument may be impaired. Yokogawa Electric Corporation assumes no liability for the customer's failure to comply with these requirements.

## The following safety symbols and wording is used in this manual.



Warning: Handle with care. Refer to the user's manual or service manual.

This symbol appears on dangerous locations on the instrument which require special instructions for proper handling or use. The same symbol appears in the corresponding place in the manual to identify those instructions.



Alternating current



ON (power)



OFF (power)

## French



Avertissement : À manipuler délicatement.

Toujours se reporter aux manuels d'utilisation et d'entretien. Ce symbole a été apposé aux endroits dangereux de l'instrument pour lesquels des consignes spéciales d'utilisation ou de manipulation ont été émises. Le même symbole apparaît à l'endroit correspondant du manuel pour identifier les consignes qui s'y rapportent.



Courant alternatif



Marche (alimentation)



Arrêt (alimentation)

# Conventions Used in This Manual

## Safety Markings

The following markings are used in this manual.



Improper handling or use can lead to injury to the user or damage to the instrument. This symbol appears on the instrument to indicate that the user must refer to the user's manual for special instructions. The same symbol appears in the corresponding place in the user's manual to identify those instructions. In the manual, the symbol is used in conjunction with the word "WARNING" or "CAUTION."

### **WARNING**

Calls attention to actions or conditions that could cause serious or fatal injury to the user, and precautions that can be taken to prevent such occurrences.

### **CAUTION**

Calls attention to actions or conditions that could cause light injury to the user or damage to the instrument or user's data, and precautions that can be taken to prevent such occurrences.

## French

### **AVERTISSEMENT**

Attire l'attention sur des gestes ou des conditions susceptibles de provoquer des blessures graves (voire mortelles), et sur les précautions de sécurité pouvant prévenir de tels accidents.

### **ATTENTION**

Attire l'attention sur des gestes ou des conditions susceptibles de provoquer des blessures légères ou d'endommager l'instrument ou les données de l'utilisateur, et sur les précautions de sécurité susceptibles de prévenir de tels accidents.

### **Note**

Calls attention to inf

## Notations Used in the Procedural Explanations

On pages that describe the operating procedures in each chapter, the following notations are used to distinguish the procedure from their explanations.

### Procedure

This subsection contains the operating procedure used to carry out the function described in the current section. The procedures are written with inexperienced users in mind; experienced users may not need to carry out all the steps.

### Explanation

This subsection describes the setup parameters and the limitations on the procedures.

## Terms Used in Explanations of Procedures

---

### Panel Keys and Soft Keys

Bold characters used in the procedural explanations indicate characters that are marked on the panel keys or the characters of the soft keys displayed on the screen menu.

### SHIFT+Panel Key

SHIFT+key means you will press the SHIFT key to turn it ON and then press the panel key. The setup menu marked in purple below the panel key that you pressed appears on screen.

---

## Units

---

k Denotes 1000. Example: 12 kg, 100 kHz

K Denotes 1024. Example: 459 KB (file size)

---

# How To Use This Manual

## Structure of This Manual

This user's manual consists of the following eight chapters, an appendix, and an index.

### **Chapter 1 Remote Control Functions**

This section describes the various types of communication interfaces and program functions.

### **Chapter 2 GP-IB Interface (GP-IB1 Port)**

Describes the functions and lists the specifications of the GP-IB1 port.

### **Chapter 3 Ethernet Interface**

Describes the functions and lists the specifications of the Ethernet interface.

### **Chapter 4 Serial (RS-232) Interface**

Describes the functions and lists the specifications of the RS-232 interface.

### **Chapter 5 GP-IB Interface (GP-IB2 Port)**

Describes the functions and lists the specifications of the GP-IB2 port.

### **Chapter 6 Status Registers**

Explains the status byte and describes the various kinds of registers, cues, and other items.

### **Chapter 7 Remote Commands**

Describes each individual command that can be used.

### **Chapter 8 Program Function**

Explains the program function for controlling another instrument using the AQ6370C/AQ6370D/AQ6373/AQ6375 as the controller.

### **Appendix**

Lists commands that are compatible with the AQ6317.

### **Index**

An alphabetical index.

# Contents

Safety Precautions.....	iii
Conventions Used in This Manual .....	iv
How To Use This Manual .....	vi
<b>Chapter 1 Remote Control Functions</b>	
1.1    Remote Interfaces .....	1-1
1.2    Switching between Local and Remote .....	1-2
1.3    Sending/Receiving Remote Commands .....	1-3
<b>Chapter 2 GP-IB Interface (GP-IB1 Port)</b>	
2.1    Connecting via GP-IB .....	2-1
2.2    GP-IB Interface Function.....	2-3
2.3    GP-IB Interface Specifications .....	2-4
2.4    Setting the GP-IB Address .....	2-5
2.5    Responses to Interface Messages .....	2-7
2.6    Sample Program .....	2-9
<b>Chapter 3 Ethernet Interface</b>	
3.1    Connecting via Ethernet .....	3-1
3.2    Setting Up Ethernet .....	3-2
3.3    Sample Program .....	3-8
<b>Chapter 4 Serial (RS-232) Interface</b>	
4.1    Connecting via the Serial (RS-232) Interface .....	4-1
4.2    Remote Control Using Commands.....	4-4
4.3    Setting Up RS-232 .....	4-5
<b>Chapter 5 GP-IB Interface (GP-IB2 Port )</b>	
5.1    Connecting via GP-IB2 .....	5-1
5.2    GP-IB Interface Specifications .....	5-2
5.3    Setting the GP-IB Address .....	5-3
<b>Chapter 6 Status Registers</b>	
6.1    Status Registers .....	6-1
6.2    Status Byte Registers .....	6-3
6.3    Standard Event Status Registers .....	6-5
6.4    Operation Status Registers .....	6-7
6.5    Questionable Status Registers .....	6-10

**Chapter 7 Remote Commands**

7.1	Rules of Syntax and Command Types .....	7-1
7.2	Table of Correspondence between Soft Keys and Remote Commands .....	7-4
7.3	ANALYSIS Setting Parameters .....	7-20
7.4	Remote Command Tree .....	7-29
7.5	Common Commands .....	7-37
7.6	Instrument-Specific Commands .....	7-40
	ABORT Sub System Command .....	7-40
	APPLication Sub System Commands .....	7-40
	CALCulate Sub System Command .....	7-43
	CALibration Sub System Command.....	7-68
	DISPlay Sub System Command.....	7-70
	FORMAT Sub System Command.....	7-76
	HCOPY Sub System Command.....	7-76
	INITiate Sub System Command .....	7-77
	MEMory Sub System Command .....	7-77
	MMEMory Sub System Command .....	7-78
	PROGram Sub System Command.....	7-82
	SENSe Sub System Command.....	7-83
	STATus Sub System Command .....	7-86
	SYStem Sub System Command .....	7-87
	TRACe Sub System Command.....	7-91
	TRIGger Sub System Command.....	7-95
	UNIT Sub System Command .....	7-97
7.7	Output Format for Analysis Results.....	7-98

**Chapter 8 Program Function**

8.1	Editing a Program.....	8-1
8.2	Executing a Program.....	8-9
8.3	Program Function Commands .....	8-15
8.4	Controlling an External Instrument with the Program Function .....	8-57
8.5	Sample Program .....	8-59

**Appendix AQ6317-Compatible GP-IB Commands**

Switching Command Modes .....	App-1
AQ6317 Status Byte .....	App-3
List of the AQ6317-Compatible Commands.....	App-4
HIGH1, HIGH2, HIGH3 of Measurement Sensitivity .....	App-17

**Index**

## 1.1 Remote Interfaces

This instrument is equipped with the following remote interfaces.

### GP-IB1 (IEEE 488.2, See Chapter 2)

This port is used to connect a controller such as a PC to remote control this instrument.

Connect a controller or another device controlled by the controller to this port.

This instrument is controlled using remote commands.

Two types of remote commands are provided: the instrument's native commands complying with SCPI (Standard Commands for Programmable Instruments), and commands compatible with the conventional model AQ6317 (see the appendix).

The GP-IB on the AQ6370D/AQ6373B corresponds to this function.

### GP-IB2 (IEEE 488.1, See Chapter 5)

The instrument acts as a controller for remote control of external instruments. Connect to the external device to be controlled using the instrument's program function. This function is not available on the AQ6370D/AQ6373B.

### RS-232 (See Chapter 3)

This port is used to connect a controller such as a PC to control the instrument remotely.

### Ethernet (See Chapter 4)

This port is used to connect a controller such as a PC to control the instrument remotely via network.

## GP-IB1 and GP-IB2 Ports

The GP-IB1 and GP-IB2 ports must be used differently for different purposes.

The GP-IB port on the AQ6370D corresponds to the GP-IB1 port. The GP-IB2 port is not available on the AQ6370D/AQ6373B.

The GP-IB1 port is used when controlling the instrument from a PC.

The GP-IB2 port is used when controlling an external instrument from the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.

Therefore, please note the following.

- A controller such as a PC that is connected to the GP-IB2 port cannot remotely control the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.
- Even if a turnable laser source or an external device to be controlled by the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 using program functions is connected to the GP-IB1 port, it cannot remote control the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.
- The GP-IB1 and GP-IB2 ports are independent of each other. Thus, a controller connected to the GP-IB1 port cannot directly send a message to an external device connected to the GP-IB2 port.
- When a PC or other controller is connected to the GP-IB1 port, connecting the GP-IB1 port with the GP-IB2 port results in improper operation.

Do not connect these ports together, or turn OFF the system controller function.

The default is ON.

## 1.2 Switching between Local and Remote

### Switching from Local to Remote

When in Local mode, if a listen address is sent from the controller that sets REN (remote enable) and ATN to “True,” the instrument enters Remote mode.

- When in Remote mode, the REMOTE indicator lights.
- Keys other than the LOCAL key are disabled.
- Settings entered in Local mode are held even if switching to Remote mode.
- When an LLO (Local Lock Out) message is received from the controller, the instrument enters local lockout status. In LLO status, the LOCAL key is disabled and does not return the instrument to Local mode even when pressed. After cancelling the local lockout status, press the LOCAL key. To cancel the local lockout status, set REN to “False” from the controller.

### Switching from Remote to Local

If you press the LOCAL key when in Remote mode the instrument enters Local mode.

However, it does not return to Local mode if in the local lockout state.

- The REMOTE indicator turns off.
- All keys are enabled.
- Settings entered in Remote mode are held even if switching to Local mode.
- When a GTL (Go to Local) message is received from the controller, the instrument enters Local mode even if REN is set to False.

## 1.3 Sending/Receiving Remote Commands

### Buffers

#### **Input Buffer**

The instrument's input buffer is a single stage 1 MB buffer. When receiving data that exceeds the buffer size, the data after the first megabyte is discarded. The remote command after the last command separator of the 1 MB of data is deleted.

#### **Output Buffer**

The instrument's output buffer is a single stage 1 MB buffer. Only the most recent data is held. (When a talker command is received while there is data in the buffer, the old data in the buffer is replaced with the incoming data.) When talker commands are combined and executed resulting in generation of talker data that exceeds the buffer size, the following process is carried out.

- The query error bit (QYE) of the standard event status register is set to 1.
- The talker output buffer is cleared.
- Commands received even after the buffer overflow are processed. Note, however, that talker data by talker commands is not stored at the output buffer.

#### **Error Buffer**

This instrument's error buffer is of a single stage and stores only the latest error information.

### Message Terminators

This instrument allows the following message terminators to be used.

#### **Program Message Terminators**

- Assertion of EOI (End-Of-Identify) signal
- LF (line feed) character
- LF+EOI

Here, LF is a line feed (0Ah) in ASCII. For CR + LF, because CR (0Dh) is recognized as "wsp," CR + LF can consequently also be used as a message terminator. Also, for waveform binary transfer, only EOI is used as a message terminator.

#### **Response Message Terminator**

LF+EOI is used as the response message terminator.

### Receiving Remote Commands

- When completing receipt of a remote command, the instrument releases the GP-IB bus.
- When receiving the next command while a command action is being executed, the instrument captures that command to store it in the receive buffer, and then releases the GP-IB bus.
- When there is a remote command in the receive buffer, the instrument does not capture a successive command even if there are commands on the GP-IB bus.
- When the action of the preceding command is complete, the instrument executes the command stored in the receive buffer and clears the buffer. Then it captures the next command into the receive buffer if there is one on the bus.
- When an output statement contains multiple remote commands, this instrument captures them all and services them in the order they were written. In this case, unless the last command in the statement has started to be executed, this instrument cannot capture the next command.

### Data Inquiry

- Inquiry of data by the external controller is made using a query command or a data output request from the controller.
- Query commands end with a question mark (?).
- For query commands with an argument, the argument is specified in the form of <wsp> + <argument> at the end of the “?”.
- When a query command is received, the instrument prepares a reply to the query command in the output buffer.
- Data in the output buffer will be retained until the instrument receives an input statement or a new query command from the controller.
- If multiple query commands are specified and written in succession using a semicolon “;”, the instrument prepares replies to all of them in the output buffer. In this case, the instrument will collectively output all of the prepared data when receiving the next data output request.

### Setting the timeout time

A timeout time setting of 30 seconds or more is recommended.

At approximately 10 minute intervals, the instrument performs an auto offset for approximately 30 seconds. The communication timeout of the external controller should be set to 30 seconds or more so that a timeout does not occur during the execution of the offset. See the user's manual of your remote interface card for instructions on how to set the communication timeout time.

The instrument's auto offset function is set to ON by default, and it performs offset of the analog circuits at approximately 10 minute intervals. The offset process takes about 30 seconds. On the AQ6373 and AQ6375, during this offset process, the receiving of remote commands, execution of remote commands, and talker data transmission processes are suspended. If an external controller sends a remote command or requests output of talker data while the suspension is in effect, the external controller may experience a communication timeout error because the instrument cannot perform the requested action until the offset process is complete.

#### If you do not want to set the communication timeout to 30 seconds or less

To avoid remote malfunctions due to communication timeouts, offset processing can be performed manually. Turn the auto offset function OFF in advance, and perform the offset manually during a gap in measurement sequences. Wait approximately 30 seconds until the offset process is finished. After the offset is complete, restart the measurement sequence.

The remote commands are as follows.

Turn OFF the auto offset function	:CALibration:ZERO off
Perform a manual offset	:CALibration:ZERO once

#### Note

---

- An offset interval of 10 minutes is recommended.
- If the AUTO OFFSET key is OFF, the offset can fluctuate over time, and the level axis performance can degrade. Always have it turned ON.
- When the AUTO OFFSET key is set to ON,  is displayed at the bottom of the screen.

### Device Trigger Function

When GET (Group Execute Trigger) is received, the instrument will perform a single sweep.

## 2.1 Connecting via GP-IB

### GP-IB Cable

This instrument is equipped with an IEEE standard 488-1978 24-pin GP-IB connector. Use a GP-IB cable that conforms to the IEEE standard 488-1978.

### Connections

The instrument has two ports, GP-IB1 and GP-IB2. The GP-IB port on the AQ6370D/AQ6373B corresponds to the GP-IB1 port. The GP-IB2 port is not available on the AQ6370D/AQ6373B.

GP-IB1 port: Can be connected to a PC for remote control of the instrument from the PC.

GP-IB2 port: Can be connected to another instrument for remote control of that instrument using the AQ6370C/AQ6373/AQ6375's program function.

For now, you will connect a PC to the GP-IB1 port.

Turn OFF all the power switches of the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 and any devices to be connected to it. Connect a cable to the GP-IB1 port on the rear panel of the instrument.


#### CAUTION

Always turn OFF the power to the instrument and the PC when connecting or disconnecting communication cables. Failure to turn OFF the power can result in malfunction or damage to internal circuitry.

#### French

#### ATTENTION

Veillez à mettre le PC et l'oscilloscope DLM4000 hors tension lorsque vous branchez ou débranchez les câbles de communication, car cela risquerait de provoquer des dysfonctionnements ou des courts-circuits internes.

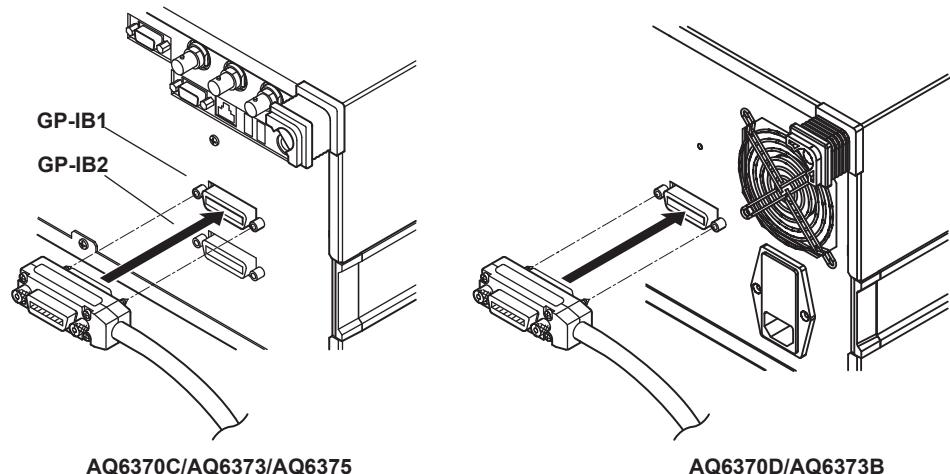


## 2.1 Connecting via GP-IB

---

### Precautions When Making Connections

- Securely fasten the screw that is attached to the GP-IB cable connector.
- You can connect several cables to connect to several devices. However, fifteen or more devices including the controller cannot be connected to a single bus.
- When connecting several devices, you cannot specify the same address for more than one.
- Use a cable of two meters or longer to connect between devices.
- Ensure that the total length in cables does not exceed twenty meters.
- When carrying out communications, make sure that at least two-thirds of all connected devices are turned ON.
- When connecting multiple devices, use a star or linear configuration as shown in the figure below. A loop or parallel configuration cannot be used.

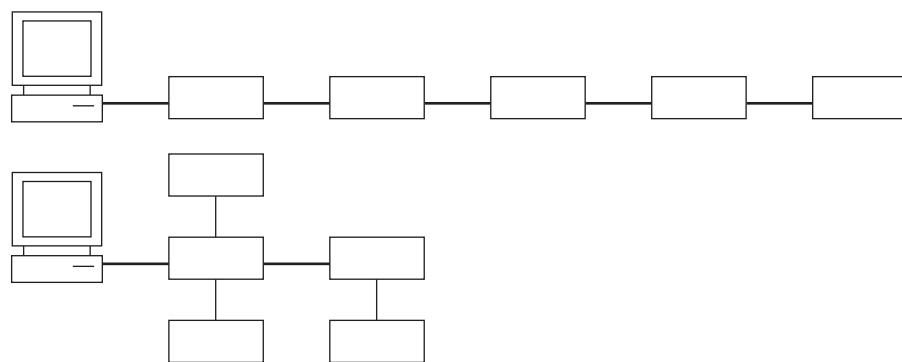

## 2.2 GP-IB Interface Function

### GP-IB Interface Function

#### Listener Function

- All of the same settings can be performed using the interface (except for power ON/OFF and communication settings) as when using the instrument's panel keys.
- Settings, waveforms, and other data can be received through output commands from the controller.
- Additionally, you can also receive commands regarding status reports and other data.

#### Talker Function

- Settings, waveforms, and other data can be output.

**Note**

Listen only, talk only, and controller functions are not available.

### Switching between Remote and Local

#### Switching from Local to Remote

When in Local mode, if the instrument received a listen address from the controller that sets REN (remote enable) and ATN to "True," the instrument enters Remote mode.

- When in Remote mode, the REMOTE indicator lights.
- Keys other than the LOCAL key are disabled.
- Settings entered in Local mode are held even if switching to Remote mode.
- When an LLO (Local Lock Out) message is received from the controller, the instrument enters local lockout status. In LLO status, the LOCAL key is disabled and does not return this instrument to Local mode even when pressed. After cancelling the local lockout status, press the LOCAL key. To cancel the local lockout status, set REN to "False" from the controller.

#### Switching from Remote to Local

If you press the LOCAL key when in Remote mode the instrument enters Local mode. However, it does not return to Local mode if in the local lockout state.

- The REMOTE indicator turns off.
- All keys are enabled.
- Settings entered in Remote mode are held even if switching to Local mode.
- When a GTL (Go to Local) message is received from the controller, the instrument enters Local mode even if REN is set to False.

**Note**

The GP-IB interface cannot be used simultaneously with other communication interfaces (RS-232, USB, or Ethernet).

## 2.3 GP-IB Interface Specifications

### GP-IB Interface Specifications

Electromechanical specifications:	Conforms to IEEE std. 488-1978
Functional specifications:	See table below
Protocols:	Conforms to IEEE std. 488.2-1992
Encoding:	ISO (ASCII)
Mode:	Addressable mode
Address setting:	Addresses 0-30 can be set in the GP-IB setting screen in the SYSTEM menu.
Remote mode cancel:	Press LOCAL to cancel Remote mode. Note that this is disabled when under Local Lockout by the controller.

### Functional Specifications


Function	Subset	Description
Source handshake	SH1	All capabilities of send handshake
Acceptor handshake	AH1	All capabilities of receive handshake
Talker	T6	Basic talker function, serial polling, and talker cancel function through MLA (my listen address). Talker only not provided.
Listener	L4	Basic listener function, serial polling, and listener cancel function through MLA (my listen address). Listener only not provided.
Service request	SR1	All service request functions
Remote local	RL1	All Remote/Local functions
Parallel port	PP0	Parallel polling function not provided
Device clear	DC1	All device clear functions Output buffer clear Input buffer clear (clearing of an unexecuted commands) Error buffer clear STB, ESR clear
Device trigger	DT0	Device trigger function
Controller	C0	Controller function not provided
Electrical characteristics	E1	Open collector

## 2.4 Setting the GP-IB Address

### Procedure


#### Selecting the Communication Interface

1. Press **SYSTEM**. The system setting menu is displayed.
2. Press the **MORE1/4** soft key. The communication interface setting menu is displayed.
3. Press the **REMOTE INTERFACE** soft key. The setting menu for the interface to be used is displayed.
4. Press the **GP-IB** soft key to specify GP-IB as the communication interface.

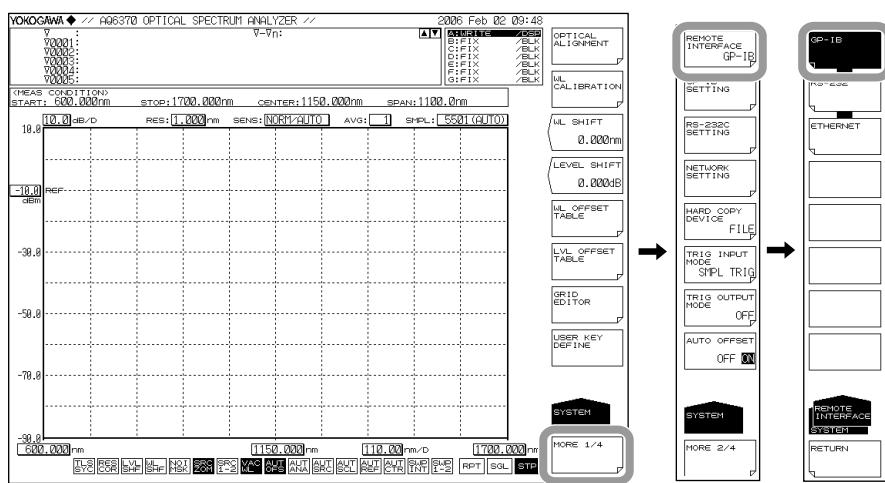

#### Setting the Address

5. Press the **GP-IB SETTING** soft key. The GP-IB setting menu is displayed.
6. Press the **MY ADDRESS** soft key. The GP-IB address setting screen is displayed.
7. Set the GP-IB address using the **rotary knob** or the **arrow keys**, and press **ENTER**.

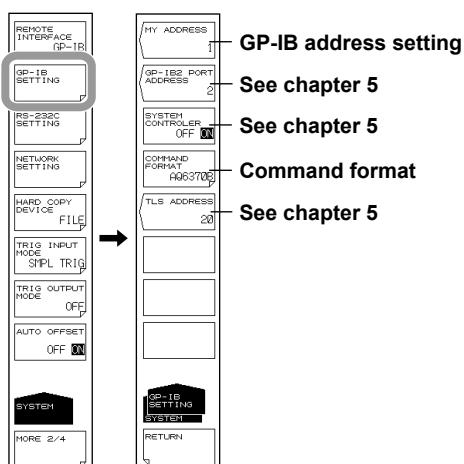

### Setting the Command Format

8. Perform these steps if you will use AQ6370C/AQ6370D/AQ6373/AQ6375 commands. Press the **COMMAND FORMAT** soft key. The command format setting menu is displayed.
9. Normally, you will enter AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375. If you wish to use AQ6317 commands, enter AQ6317.

### Explanation

The settings below are used when entering the settings that can be entered using the instrument's panel keys from a controller, or when outputting settings or waveform data to the controller.

#### GP-IB Address Settings

When in Addressable mode, set the instrument's address within the following range.  
0–30

Each device that can be connected via GP-IB has its own unique GP-IB address. This address allows each device to be distinguished from other devices. Therefore, when connecting the instrument to a PC or other device, make sure not to set the same address on the instrument as any of the other devices.

#### Note

- Do not change an address while the controller or other devices are using GP-IB.
- Set addresses other than those used by the GP-IB2 port.

#### Command Format Settings

Normally, you will enter AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375 mode. If you wish to use the commands of the AQ6317 (another product in the series), enter AQ6317. See the appendix for AQ6317 commands that are compatible with the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.

#### Note

Controller functions and TLS address settings are entered when controlling an external device using the GP-IB2 port. These settings are invalid for the GP-IB1 port.

## 2.5 Responses to Interface Messages

### Responses to Interface Messages

#### Responses to Uniline Messages

##### **IFC (Interface Clear)**

Clears talker and listener. Output is cancelled if outputting data.

##### **REN (Remote Enable)**

Switches between Local and Remote.

IDY (Identify) is not supported.

#### Responses to Multiline Messages (Address Commands)

##### **GTL (Go To Local)**

Switches to Local mode.

##### **SDC (Selected Device Clear)**

- Clears program messages (commands) being received, and the output queue.
- The \*OPC and \*OPC? commands are invalid during execution.
- The \*WAI command closes immediately.

PPC (parallel poll configure), GET (group execute trigger), and TCT (take control) are not supported.

#### Responses to Multiline Messages (Universal Commands)

##### **LLO (Local Lockout)**

Disables the front panel SHIFT+CLEAR operation, and prohibits switching to Local mode.

##### **DCL (Device Clear)**

Same operation as SDC.

##### **SPE (Serial Poll Enable)**

Places the talker function of all devices on the bus in Serial poll mode. The controller polls each device in order.

##### **SPD (Serial Poll Disable)**

Cancels Serial poll mode for the talker function of all devices on the bus.

PPU (Parallel Poll Unconfigure) is not supported.

### Definition of Interface Messages

*Interface messages* are also called *interface commands* or *bus commands*, and are commands that are issued from the controller. Interface messages come in the following categories.

#### Uniline Messages

A message is sent through a single command line. The following are the three types of uniline messages.

IFC (Interface Clear)

REN (Remote Enable)

IDY (Identify)

## 2.5 Responses to Interface Messages

### Multiline Messages

A message is sent through eight data lines. Multiline messages come in the following categories.

#### Address Commands

These commands are valid when the device is specified as the listener or the talker.

The following are the five types of address commands.

#### Commands valid for devices specified as listeners

- GTL (Go To Local)
- SDC (Selected Device Clear)
- PPC (Parallel Poll Configure)
- GET (Group Execute Trigger)

#### Commands valid for devices specified as talkers


- TCT (Take Control)

#### Universal Commands

These commands are valid for all devices regardless of whether they are specified as listeners, talkers, or neither. The following are the three types of universal commands.

- LLO (Local Lockout)
- DCL (Device Clear)
- PPU (Parallel Poll Unconfigure)

Additionally, an interface message can consist of a listener address, talker address, or secondary command.

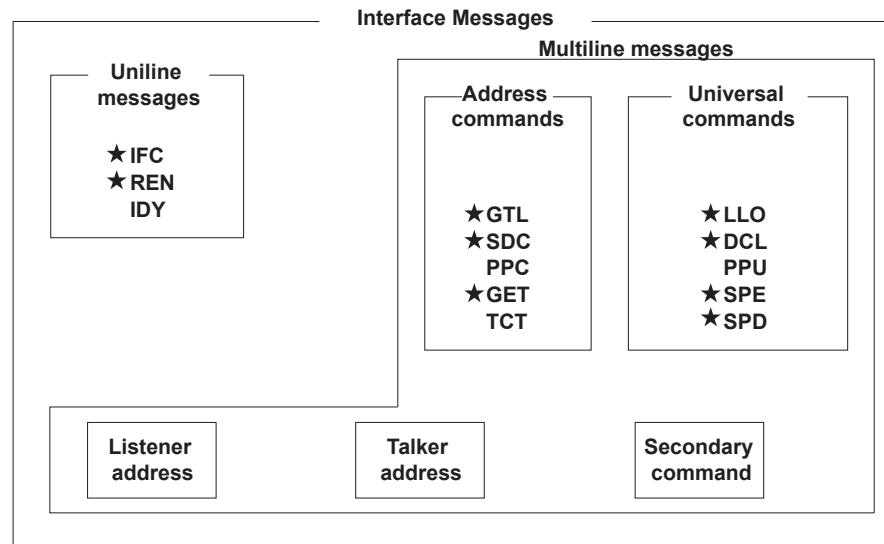

A star indicates an interface message supported by this instrument.

#### Note

##### Differences between SDC and DCL

Of the multiline messages, SDC is an address command requires specification of the talker or listener, and DCL is a universal command that does not require specification of the talker or listener. Therefore, SDC is applicable only to certain devices, but DCL is applicable to all devices on the bus.

## 2.6 Sample Program

The following shows an example of controlling the AQ6370C/AQ6370D/AQ6373/AQ6375 remotely using the GP-IB port. The sample program uses Visual Basic 6.0 as the programming language. Also, a GP-IB board by National Instruments (hereinafter, "NI") is used as the GP-IB controller and the NI-supplied driver is used as a library.

### Sample Program 1

The program sets the measurement conditions (center wavelength, span, sensitivity, and the sampling number) and then performs a sweep. After completing this sweep, the program executes a thresh-based spectrum width analysis and then outputs the results to the screen.

```

Const BOARD_ID = 0                                ' GP-IB Interface card
Address
Const osa = 1                                     ' OSA GP-IB Address

Private Sub AQ637XTEST()
    Dim intData As Integer
    Dim dblMeanWL As Double
    Dim dblSpecWd As Double
    Dim strData As String

    ' === GP-IB Interface setting ===
    ' send IFC
    Call SendIFC(BOARD_ID)

    ' assert th REN GPIB line
    intAddrList(0) = NOADDR
    Call EnableRemote(BOARD_ID, intAddrList())

    ' GPIB time out setting
    Call ibtmo(BOARD_ID, T30s)                      ' Time out = 30sec

    ' === Set the measurement parameter ===
    Call SendGPIB(osa, "*RST")                       ' Setting initialize
    Call SendGPIB(osa, "CFORM1")                      ' Command mode
    Call SendGPIB(osa, ":sens:wav:cent 1550nm")      ' set(AQ637X mode)
    Call SendGPIB(osa, ":sens:wav:span 10nm")         ' sweep center wl
    Call SendGPIB(osa, ":sens:sens mid")              ' sweep span
    Call SendGPIB(osa, ":sens:sweep:points:auto on")   ' sens mode = MID
    Call SendGPIB(osa, "")                            ' Sampling Point = AUTO

    ' === Sweep execute ===
    Call SendGPIB(osa, ":init:smode 1")               ' single sweep mode
    Call SendGPIB(osa, "*CLS")                        ' status clear
    Call SendGPIB(osa, ":init")                        ' sweep start

    ' === Wait for sweep complete ===
    Do
        Call SendGPIB(osa, ":stat:oper:even?")          ' get Operation Event
        strData = RecieveGPIB(osa)                      Register
        intData = Val(strData)
    Loop While ((intData And 1) <> 1)                  ' Bit0: Sweep status

    ' === Analysis ===
    Call SendGPIB(osa, ":calc:category swth")          ' Spectrum width
    Call SendGPIB(osa, ":calc")                         analysis(THRESH type)
    Call SendGPIB(osa, ":calc:data?")                  ' Analysis Execute
    strData = RecieveGPIB(osa)                          ' get data

```

## 2.6 Sample Program

---

```
' === Capture analytical results ===
dblMeanWL = Val(Left(strData, 16))                                ' get mean wavelegnth
dblSpecWd = Val(Mid(strData, 18, 16))                                ' get spectrum width

' === Output the result to the screen ===
MsgBox ("MEAN WL: " & dblMeanWL * 1000000000# & " nm" & vbCrLf &
        "SPEC WD: " & dblSpecWd * 1000000000# & " nm")

' === Disconnect ===
Call EnableLocal(BOARD_ID, intAddrList())
End Sub

'=====
' Sub routine
' Send Remote Command
'=====
Sub SendGPIB(intAddr As Integer, strData As String)
    Call Send(BOARD_ID, intAddr, strData, NLend)
    If (ibsta And EERR) Then
        MsgBox " GP-IB device can't write"
    End If
End Sub

'=====
' Sub routine
' Recieve query data
'=====
Function RecieveGPIB(intAddr As Integer) As String
    Const READSIZE = 10000
    Dim strBuffer As String

    strBuffer = Space(READSIZE)
    RecieveGPIB = ""
    Do
        DoEvents

        Call Receive(BOARD_ID, intAddr, strBuffer, STOPend)
        If (ibsta And EERR) Then
            MsgBox " GP-IB device can't read."
            RecieveGPIB = ""
            Exit Function
        Else
            RecieveGPIB = RecieveGPIB & Left(strBuffer, ibcntl)
        End If
    Loop Until ((ibsta And EEND) = EEND)
End Function
```

**Sample Program 2**

Save an image of the instrument's screen to a BMP file, then use a file transfer command to load the file onto the PC. Save the image on the PC under the file name, "C:\test.bmp".

```

Const BOARD_ID = 0                      'GP-IB Interface card Address
Const osa = 1                           'OSA GP-IB Address

Private Sub Command1_Click()
    Dim intAddrList(31) As Integer
    Dim intData As Integer
    Dim lngDataSize As Long
    Dim strData As String
    Dim intI As Integer
    Dim byteData() As Byte
    Dim byteSaveData() As Byte
    Dim lngL As Long

    '----- GPIB Interface setting
    ' send IFC
    Call SendIFC(BOARD_ID)

    ' assert th REN GPIB line
    intAddrList(0) = NOADDR
    Call EnableRemote(BOARD_ID, intAddrList())

    ' GPIB time out setting
    Call ibtmo(BOARD_ID, T30s)           'Time out = 30sec

    '----- send command to OSA
    Call SendGPIB(osa, "CFORM1")        ' Command mode set(AQ637X mode)

    Call SendGPIB(osa, ":mmem:stor:grap color,bmp,\""test"\",int")
                                         ' Save bmp file to internal memory
    Call SendGPIB(osa, ":mmem:data? \"test.bmp\"",int)
                                         ' get file data from OSA
    lngDataSize = RecieveBinaryGPIB(osa, byteData())
                                         ' Recieve binary block data

    If byteData(0) <> Asc("#") Then      ' check first data
        MsgBox "Data format error"
        Exit Sub
    End If

    '----- calculate data size
    intData = byteData(1) - Asc("0")
    strData = ""
    For intI = 1 To intData
        strData = strData + Chr(byteData(intI + 1))
    Next intI
    lngDataSize = Val(strData)           ' data size

    '----- make save data
    ReDim byteSaveData(lngDataSize)
    For lngL = 0 To lngDataSize - 1
        byteSaveData(lngL) = byteData(lngL + intData + 2)
    Next lngL

    '----- save data to file
    Open "c:\test.bmp" For Binary As #1
        Put #1, , byteSaveData
    Close #1

    '----- Disconnect
    Call EnableLocal(BOARD_ID, intAddrList())
    MsgBox "Complete"
End Sub

```

## 2.6 Sample Program

---

```
'=====
' Sub routine
' Send Remote Command
'=====

Sub SendGPIB(intAddr As Integer, strData As String)
    Call Send(BOARD_ID, intAddr, strData, NLend)
    If (ibsta And EERR) Then
        MsgBox " GP-IB device can't write"
    End If
End Sub

'=====
' Sub routine
' Recieve Binary query data
'=====

Function RecieveBinaryGPIB(intAddr As Integer, byteArray() As Byte) As Long
    Const READSIZE = 1200000          ' MAX 1.2MB
    Dim lngSize As Long
    Dim lngL As Long
    Dim lngPos As Long
    Dim ud As Integer
    Dim byteLow As Byte
    Dim byteHigh As Byte
    Dim strA As String

    Dim intDummy(READSIZE) As Integer
    lngSize = 0

    ----- open device
    ud = ildev(0, intAddr, 0, T30s, 1, 0)
    lngPos = 0

    ----- read data
    Do
        DoEvents
        Call ibrdi(ud, intDummy, READSIZE)
        If (ibsta And EERR) Then
            MsgBox "GP-IB device can't Read(GPIB:" & intAddr & ")"
            RecieveBinaryGPIB = 0
            Exit Function
        Else
            ReDim Preserve byteArray(lngPos + ibcntl + 2)
            For lngL = 0 To ibcntl / 2 - 1
                strA = Right("0000" & Hex(intDummy(lngL)), 4)
                byteHigh = Val("&H" + Left(strA, 2))
                byteLow = Val("&H" + Right(strA, 2))
                byteArray(lngPos) = byteLow
                byteArray(lngPos + 1) = byteHigh
                lngPos = lngPos + 2
            Next lngL
        End If
    Loop While (ibcntl = READSIZE)

    RecieveBinaryGPIB = lngPos
End Function
```

## 3.1 Connecting via Ethernet


You can connect to a LAN using the Ethernet interface for control of the instrument from a PC.

### Ethernet Interface Specifications

Communication ports:	1
Electromechanical specifications:	Conforms to IEEE802.3
Transmission method:	Ethernet (10BASE-T/100BASE-TX/ 1000BASE-T (AQ6370D/AQ6373B only))
Transmission speed:	10 Mbps/100 Mbps/1000 Mbps (AQ6370D/AQ6373B only)
Communication protocol:	TCP/IP
Connector type:	RJ45
Port number used:	10001/tcp (default)

### Connections

Connect a UTP (unshielded twisted-pair) cable or an STP (shielded twisted-pair) cable that is connected to another device to the ETHERNET port on the rear panel of the instrument.

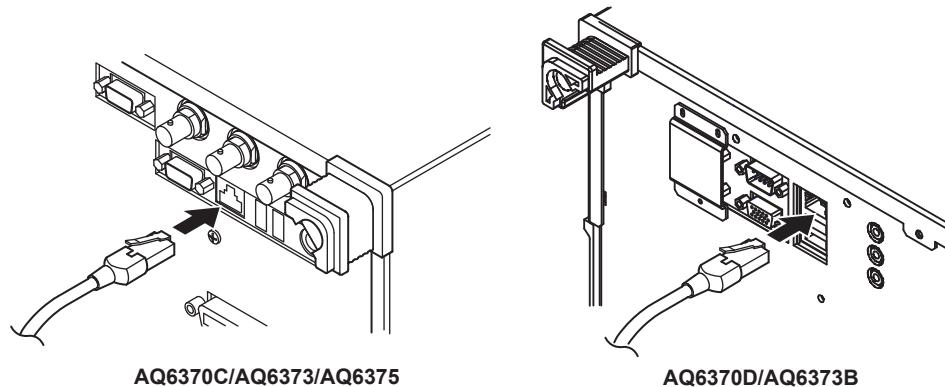

#### Precautions When Making Connections


- Be sure to use a straight cable through a hub when connecting a PC to the instrument. Performance cannot be guaranteed if a 1-to-1 connection is made with a cross cable.
- When using a UTP (straight) cable, make sure that it is a category 5 cable.

## 3.2 Setting Up Ethernet

### Procedure


#### Selecting the Communication Interface

1. Press **SYSTEM**. The system setting menu is displayed.
2. Press the **MORE1/4** soft key. The communication interface setting menu is displayed.
3. Press the **REMOTE INTERFACE** soft key. The setting menu for the interface to be used is displayed.
4. Press the **ETHERNET** soft key to specify Ethernet as the communication interface.

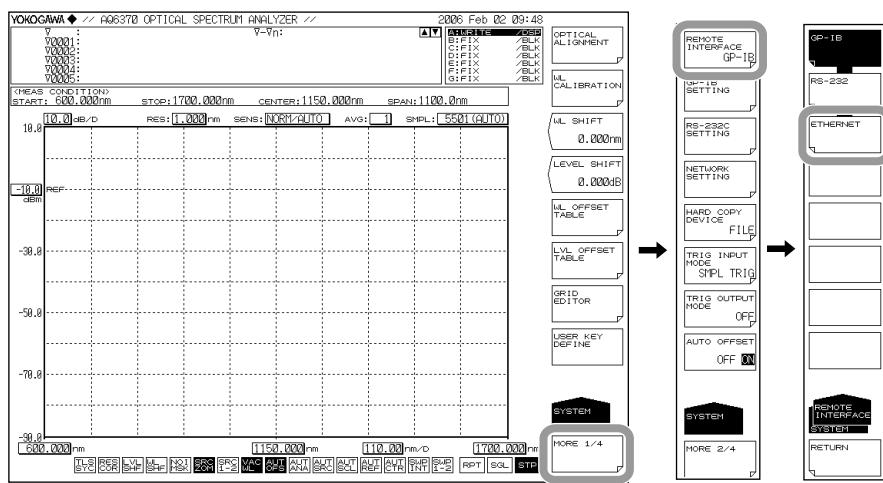

#### Setting Up TCP/IP


5. Press the **NETWORK SETTING** soft key. The ethernet setting menu is displayed.
6. Press the **TCP/IP SETTING** soft key. The TCP/IP setting menu is displayed.
7. Using the <, > soft keys, select AUTO (DHCP) or MANUAL.
8. Press the **SELECT** soft key. The item is selected.

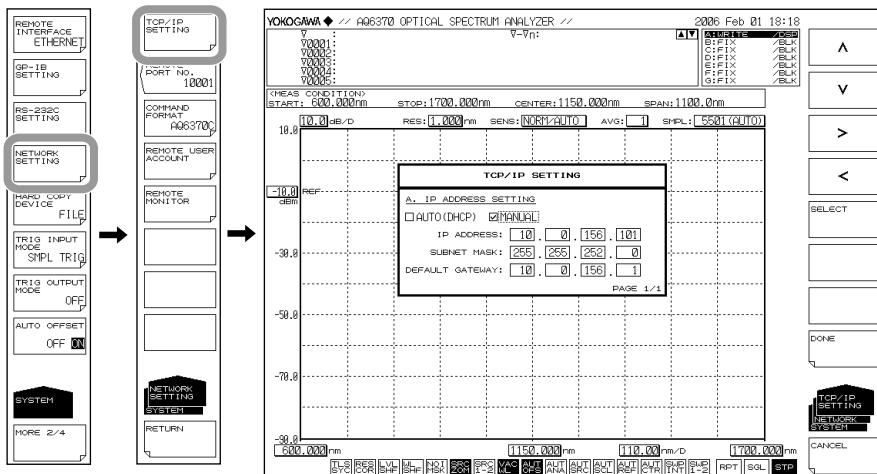

9. If you select MANUAL, enter the IP address, subnet mask, and default gateway. Using the arrow soft keys, select an input position, and press ENTER. If you selected AUTO, skip to step 10.
10. Enter a number using the **rotary knob** or the **<, >, ^, v keys**, and press **ENTER**.
11. When all settings are entered, press the **DONE** soft key.

### Setting the Remote Port Number

12. Press the **REMOTE PORT NO.** soft key. The port number setting screen is displayed.
13. Enter a port number using the **rotary knob** or the **arrow keys**, and press **ENTER**.

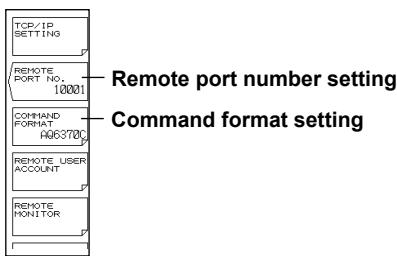


### Setting the Command Format

14. Perform these steps if you will use AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375 commands. Press the **COMMAND FORMAT** soft key. The command format setting menu is displayed.
15. Normally, you will enter AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375. If you wish to use AQ6317 commands, enter AQ6317.

### Setting the User Name and Password

16. Press the **REMOTE USER ACCOUNT** soft key. The user name and password setting menu is displayed.




17. Press the **USER NAME** soft key. The user name setting screen appears. The default is anonymous.
18. Specify a user name using 11 alphanumeric characters or fewer. If the user name is set to anonymous, the password setting is not required.
19. Press the **PASSWORD** soft key. The password setting screen is displayed.
20. Specify a password using 11 alphanumeric characters or fewer.

### 3.2 Setting Up Ethernet

#### Configuring the Remote Monitor Settings (On the AQ6370C/AQ6370D/AQ6373B)


21. Press the **REMOTE MONITOR** soft key. The remote monitor setup menu appears.
22. Press the **MONITOR PORT** soft key. Each time you press the soft key, the setting toggles between ON and OFF. Remote monitoring is possible when the setting is ON.

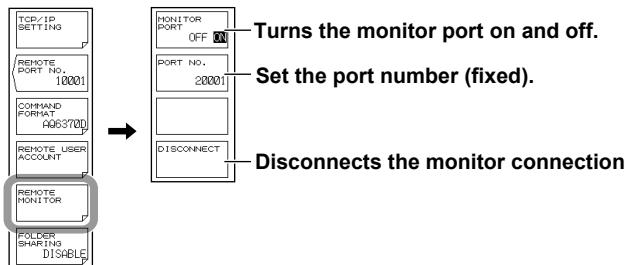

- **Disconnecting the Monitor Connection**
- 23. Press the **DISCONNECT** soft key. The monitor connection from the PC is disconnected.

#### Setting Directory Sharing (Only on the AQ6370D/AQ6373B)

24. Press the **FOLDER SHARING** soft key. A directory sharing setup menu appears.
25. Press the **READ ONLY** soft key. The user area directory of the AQ6370D/AQ6373B is shared (read only).

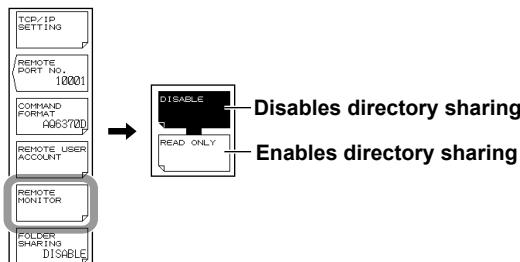

- **Disabling Directory Sharing**
- 26. Press the **DISABLE** soft key. The sharing of the user area directory is disabled.

### Explanation

#### TCP/IP Settings

It is necessary to set up the IP address for correct use of the instrument. If a DHCP server is provided on the network to which this instrument is connected, the IP address given to the instrument is automatically set. Thus, set the item IP ADDRESS SETTING under SYSTEM <NETWORK SETTING><TCP/IP SETTING> to "AUTO." Please ask your network administrator for details about network connections.

#### Note

- If you start the AQ6370C/AQ6373/AQ6375 when it is connected to a network, it may take a few minutes for the start procedure to finish. (The progress of initialization is indicated at the bottom of the screen with indications from "STEP 1/9" to "STEP 9/9.")
- When the start procedure is finished and the measurement screen appears, it may take a few more minutes before you can access the AQ6370C/AQ6373/AQ6375 from a PC over the network. In addition, the DONE key of TCP/IP settings may be unavailable for a certain time.

## REMOTE PORT NO.

Sets the port number for remote control via ETHERNET. (Default: 10001.)

## User Authentication

User authentication is required to connect to the instrument from a PC over an Ethernet network. If the user name is anonymous, a password is not required. This instrument supports plain text authentication and the MD5 Message Digest Algorithm by RSA Data Security, Inc.

## Remote Monitoring

You can use the ETHERNET port to monitor the AQ6370C/AQ6370D/AQ6373B screen or control the AQ6370C/AQ6370D/AQ6373B from a PC over a network.

To use this feature, you need remote monitoring software (not included).

For information on remote monitoring software, contact your nearest YOKOGAWA dealer.

## Sharing Directories

The user area directory of the AQ6370D/AQ6373B internal memory can be shared on a PC.

When the user area directory is shared, the following files can be copied to the PC over the network.

You cannot save files to the AQ6370D/AQ6373B.

## Remote Control Using Commands

The AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 can be remote controlled using the LAN port.

For remote commands, use the same commands as those for control via the GP-IB interface.

## Switching Interfaces

Select GP-IB, RS-232C, or ETHERNET as an interface to use for remote control. When set to ETHERNET, the LAN mode connection status is reset. Otherwise, the connection is kept open unless closed by the controller.

## Remote Commands

As with GP-IB-based remote control, you can select the command format from the AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375 mode or from the AQ6317-compatible mode.

## Interrupt by SRQ

An SRQ interrupt does not occur during LAN-based remote control.

## Status Register

The status registers operate in the same manner as in remote control via the GP-IB interface. Using the “\*SPOOL?” command dedicated for remote control using the LAN port allows you to read the status registers, as in the case with serial polling via the GP-IB interface.

\*STB?: When AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 is the setting of the COMMAND FORMAT key

SPOLL?: When AQ6317 is the setting of the COMMAND FORMAT key

## Delimiter

The delimiter for LAN-based remote control is fixed to CR + LF.

## Transmission of Talker Data

When the instrument receives talker data from an external PC, it sends the data to the external PC's buffer. It receives the external PC's buffer data and stores the query data.

## **3.2 Setting Up Ethernet**

---

### **Connection**

The instrument can only be connected to one controller (an external PC or other device). If the instrument receives a connection request from a controller while already connected to another controller, the new connection is not opened and the existing connection is kept open.

### **Computer Name**

The instrument's computer name is as follows.

For the AQ6370C

"6370C@@@@@@@@" (where "@@@@@@@@@" is the serial number)

For the AQ6370D

"6370D@@@@@@@@" (where "@@@@@@@@@" is the serial number)

For the AQ6373

"6373@@@@@@@@" (where "@@@@@@@@@" is the serial number)

For the AQ6375B,

"AQ6375B@@@@@@@@" (where "@@@@@@@@@" is the serial number)

For the AQ6375,

"AQ6375@@@@@@@@" (where "@@@@@@@@@" is the serial number)

The machine number is a 9-digit alphanumeric number on the back of the unit. You can not change the computer name.

## Commands that are Necessary for Remote Control over the LAN

The authentication by OPEN command is required to remote control over the LAN.

Both the OPEN and CLOSE commands are also valid in AQ6317 mode.

### OPEN

**Function** Sends the user name and starts user authentication.

**Syntax** OPEN<wsp>"username"

username = the user name

**Example** OPEN "yokogawa"

-> AUTHENTICATE CRAM-MD5.

**Explanation** Authentication is carried out with the OPEN command as follows.

For Plain Text Authentication

1. Send OPEN "username" to the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.

The response message is received from the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.

2. Confirm that the received message is "AUTHENTICATE CRAM-MD5."

3. Send the password to the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375  
(anything can be input if the user name is anonymous).

4. If the message, "READY" is received from the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375, authentication was successful. The AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375's REMOTE indicator lights, and sending of remote commands is enabled. If the user name and password are incorrect, authentication fails and the connection is closed.

For Encrypted Authentication

1. Send OPEN "username" to the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.

The response message is received from the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.

2. Confirm that the received message is "AUTHENTICATE CRAM-MD5."

3. Send "AUTHENTICATE CRAM-MD5 OK" to the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375. The response message (challenge string) is received from the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375.

4. The received challenge string and password are processed with an MD5 hash algorithm (anything can be input if the user name is anonymous).

5. Send the returned hash data (as a 32-character hexadecimal string in lower case) to the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375, and receive the response message.

6. If the message, "READY" is received from the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375, authentication was successful. The AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375's REMOTE indicator lights, and sending of remote commands is enabled. If the user name and password are incorrect, authentication fails and the connection is closed.

### CLOSE

**Function** Closes the connection (turns it OFF), and switches to local mode.

**Syntax** CLOSE

**Example** CLOSE

## 3.3 Sample Program

### Sample Program 1

Sending an invalid talker command to the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 and then receiving data with the instrument specified as a talker causes the GP-IB bus to stop because the instrument has no data to send. In this case, a GPIB timeout occurs, followed by recovery of the GP-IB bus.

The following shows an example of controlling the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 remotely using the Ethernet port. The sample program uses Visual Basic 6.0 as the programming language. The program sets the measurement conditions (center wavelength, span, sensitivity, and the sampling number) and then performs a sweep. After completing this sweep, the program executes a thresh-based spectrum width analysis and then outputs the results to the screen. The conditions are the same as those of the GP-IB sample program in section 2.6, "Sample Program."

```
Private Sub AQ637XTEST()
    Dim intData As Integer
    Dim dblMeanWL As Double
    Dim dblSpecWd As Double
    Dim strData As String

    ' === Connect ===
    Winsock1.RemoteHost = "192.168.1.100"           ' OSA IP address
    Winsock1.RemotePort = 10001                         ' OSA remote port num
    Winsock1.Connect

    ' === Wait to connect complete ===
    While (Winsock1.State <> sckConnected)
        DoEvents
    Wend

    ' === Authentication by OPEN Command ===
    SendLan "open ""anonymous"""
    ReceiveLan strData
    SendLan " "
    ReceiveLan strData
    If (Left(strData, 5) <> "ready") Then
        MsgBox "User authentication error."
        Exit Sub
    End If

    ' === Set the measurement parameter ===
    SendLan "*RST"
    SendLan "CFORM1"                                     ' Setting initialize
                                                       ' Command mode set
                                                       '(AQ637X mode)
    SendLan ":sens:wav:cent 1550nm"                     ' sweep center wl
    SendLan ":sens:wav:span 10nm"                        ' sweep span
    SendLan ":sens:sens mid"                            ' sens mode = MID
    SendLan ":sens:sweep:points:auto on"                ' Sampling Point = AUTO

    ' === Sweep execute ===
    SendLan ":init:smode 1"                             ' single sweep mode
    SendLan "*CLS"                                      ' status clear
    SendLan ":init"                                     ' sweep start
```

```

' === Wait for sweep complete ===
Do
    SendLan ":stat:oper:even?"                                ' get Operation Event
    Register
    ReceiveLan strData
    intData = Val(strData)
Loop While ((intData And 1) <> 1)                                ' Bit0: Sweep status

' === Analysis ===
SendLan ":calc:category swth"                                     ' Spectrum width
analysis(THRESH type)
SendLan ":calc"
SendLan ":calc:data?"                                         ' Analysis Execute
ReceiveLan strData                                              ' get data

' === Capture analytical results ===
dblMeanWL = Val(Left(strData, 16))                                ' get mean wavelegnth
dblSpecWd = Val(Mid(strData, 18, 16))                               ' get spectrum width

' === Output the result to the screen ===
MsgBox ("MEAN WL: " & dblMeanWL * 1000000000# & " nm" & vbCrLf &
        "SPEC WD: " & dblSpecWd * 1000000000# & " nm")

' === Disconnect ===
Winsock1.Close

'Wait to disconnect complete
While (Winsock1.State <> sckClosed)
    DoEvents
Wend

End Sub

'=====
' Sub routine
' Send Remote Command
'=====
Sub SendLan(strData As String)
    Winsock1.SendData strData & vbCrLf
    DoEvents
End Sub

'=====
' Sub routine
' Receive query data
'=====
Sub ReceiveLan(strData As String)
    Dim strData2 As String
    strData = ""
    Do
        Winsock1.GetData strData2, vbString
        strData = strData + strData2
        DoEvents
    Loop While (Right(strData, 1) <> vbLf)
End Sub

```

### 3.3 Sample Program

---

#### Sample Program 2

Save an image of the instrument's screen to a BMP file, then use a file transfer command to load the file onto the PC. Save the image on the PC under the file name, "C:\test.bmp". The conditions are the same as the GP-IB sample program in section 2.6, "Sample Programs."

```
Const TIMEOUT = 1                                ' time out(sec)

Private Sub cmdConnect_Click()
    Dim strData As String
    Dim byteData() As Byte
    Dim lngDataSize As Long

    '==== Connect ====
    If (ConnectLan("192.168.1.100", 10001) = False) Then
        MsgBox "Connection error"
        Winsock1.Close
        Exit Sub
    End If

    ' === Authentication by OPEN Command ===
    SendLan "open ""anonymous"""
    lngDataSize = ReceiveLan(strData)                ' Send user name
    If (lngDataSize = -1) Then
        MsgBox "Data Receive Error"
        Winsock1.Close
        Exit Sub
    End If

    SendLan " "
    lngDataSize = ReceiveLan(strData)                ' Send password
    If (lngDataSize = -1) Then
        MsgBox "Data Receive Error"
        Winsock1.Close
        Exit Sub
    End If
    If (Left(strData, 5) <> "ready") Then
        MsgBox "User authentication error."
        Winsock1.Close
        Exit Sub
    End If

    '----- send command to OSA
    Call SendLan("CFORM1")                          ' Command mode
                                                    ' set (AQ637X mode)
    Call SendLan(":mmem:stor:grap color,bmp,\"test\"",int")
                                                    ' Save bmp file to internal memory
    Call SendLan(":mmem:data? \"test.bmp\"",int)     ' get file data from
                                                    ' OSA
    lngDataSize = ReceiveBinaryLan(byteData())        ' Recieve binary block data

    '----- save data to binary file
    Open "c:\test.bmp" For Binary As #1
        Put #1, , byteData
    Close #1

    '----- Disconnect
    Winsock1.Close

    'Wait to disconnect complete
    While (Winsock1.State <> sckClosed)
        DoEvents
    Wend
    MsgBox "Complete"
End Sub
```

```

' =====
' Sub routine
' Connect OSA via ETHERNET
'   in: strIP   IP Address(Ex. "192.168.1.100") or Computer Name
'         intPort   port number (Ex. 10001)
'   out:    none
'   ret:    OK/NG  true: OK, false: NG
' =====
Function ConnectLan(strIP As String, intPort As Integer) As Boolean
    Dim sglStart As Single
    Dim sglEnd As Single
    Dim sglNow As Single
    Dim bConnect As Boolean

    sglStart = Timer()
    sglEnd = sglStart + TIMEOUT
    bConnect = True

    ' === Connect ===
    Winsock1.RemoteHost = strIP                                ' OSA IP address
    Winsock1.RemotePort = intPort                               ' OSA remote port num
    Winsock1.Connect

    ' === Wait to connect complete ===
    While ((Winsock1.State <> sckConnected) And (bConnect = True))
        DoEvents
        ' Timeout check
        sglNow = Timer()
        If (sglNow < sglStart) Then sglNow = sglNow + 86400
        If sglNow >= sglEnd Then bConnect = False
    Wend

    '----- return value set
    ConnectLan = bConnect
End Function

' =====
' Sub routine
' Send Remote Command
' =====
Sub SendLan(strData As String)
    Winsock1.SendData strData & vbCrLf
    DoEvents
End Sub

' =====
' Sub routine
' Receive query data
'   in:    none
'   out:  strData      Receive data
'   ret:  Receive data size (Error: -1)
' =====
Function ReceiveLan(strData As String) As Long
    Dim strData2 As String
    Dim sglStart As Single
    Dim sglEnd As Single
    Dim sglNow As Single
    Dim bTimeout As Boolean

    sglStart = Timer()
    sglEnd = sglStart + TIMEOUT
    bTimeout = False

```

### 3.3 Sample Program

---

```
strData = ""
Do
    ' data receive
    DoEvents
    Winsock1.GetData strData2, vbString
    strData = strData + strData2

    ' Timeout check
    sglNow = Timer()
    If (sglNow < sglStart) Then sglNow = sglNow + 86400
    If sglNow >= sglEnd Then bTimeout = True
Loop While ((Right(strData, 1) <> vbLf) And (bTimeout = False))

    ' return value set
If bTimeout = True Then
    ReceiveLan = -1
Else
    ReceiveLan = Len(strData)
End If

End Function

'=====
' Sub routine
' Recieve Binary query data
'   in:    none
'   out:   byteArray      Receive data (byte array)
'   ret:   Receive data size (Error: -1)
'=====

Function ReceiveBinaryLan(byteArray() As Byte) As Long
    Dim lngPos As Long
    Dim lngTempPos As Long
    Dim bData As Byte
    Dim intI As Integer
    Dim intJ As Integer
    Dim strA As String
    Dim lngDataLength As Long
    Dim byteDummy() As Byte
    Dim sglStart As Single
    Dim sglEnd As Single
    Dim sglNow As Single
    Dim bTimeout As Boolean

    sglStart = Timer()
    sglEnd = sglStart + TIMEOUT
    bTimeout = False
    '-----
    ' Header block
    '-----
    Call ReadIPBin(bData)           ' Receive 1byte

    If bData = Asc("#") Then
        Call ReadIPBin(bData)       ' Receive 1byte

        intI = bData - Asc("0")
        strA = ""
        For intJ = 0 To intI - 1
            Call ReadIPBin(bData)   ' Receive 1byte
            strA = strA + Chr(bData)
        Next intJ
        lngDataLength = Val(strA)     ' block data size

        ReDim byteArray(lngDataLength)
```

```

' -----
' Recieve binary data block
' -----
lngPos = 0
lngTempPos = 0
ReDim byteDummy(lngDataLength)
Winsock1.GetData byteDummy, vbArray + vbByte, lngDataLength
                           ' Receive binary data

Do
    DoEvents
    If (lngTempPos > UBound(byteDummy)) Then
        Winsock1.GetData byteDummy, vbArray + vbByte, lngDataLength
                           ' Continue to receive
        lngTempPos = 0
    Else
        byteArray(lngPos) = byteDummy(lngTempPos)
        lngPos = lngPos + 1
        lngTempPos = lngTempPos + 1
    End If

    'Timeout check
    sglNow = Timer()
    If (sglNow < sglStart) Then sglNow = sglNow + 86400
    If sglNow >= sglEnd Then bTimeout = True
    Loop Until ((lngPos = lngDataLength) Or (bTimeout = True))
    End If

    ' return value set
    If bTimeout = True Then
        ReceiveBinaryLan = -1
    Else
        ReceiveBinaryLan = lngDataLength
    End If
End Function

' =====
' Read binary data(1byte)
' =====
Sub ReadIPBin(byteData As Byte)
    Dim sglStart As Single
    Dim sglEnd As Single
    Dim sglNow As Single
    Dim bTimeout As Boolean

    sglStart = Timer()
    sglEnd = sglStart + TIMEOUT
    bTimeout = False

    '---- wait until data received or timeout
    Do
        DoEvents

        'Timeout check
        sglNow = Timer()
        If (sglNow < sglStart) Then sglNow = sglNow + 86400
        If sglNow >= sglEnd Then bTimeout = True
    Loop Until ((Winsock1.BytesReceived > 1) Or (bTimeout = True))

    Winsock1.GetData byteData, vbByte, 1           ' 1byte read
End Sub

```

## 4.1 Connecting via the Serial (RS-232) Interface

### Serial Interface Functions and Specifications

#### Receive Function

You can enter the same settings as can be entered with front panel keys.  
A settings output request is received.

#### Send Function


You can output settings and measured results.

#### Serial (RS-232) Interface Specifications


Electrical characteristics:	Conforms to the EIA-574 standard (EIA-232 (RS-232), 9-pin)
Connection type:	Point-to-point
Communication method:	Full duplex
Synchronization method:	Start-stop synchronization
Baud rate:	1200, 2400, 4800, 9600, 19200, 38400, 57600, 115200
Start bit:	1 bit, fixed
Data length:	8 bit, fixed
Parity:	Odd, Even, or None
Stop bit:	1 bit, fixed
Connector:	DELC-J9PAF-13L6 (JAE or equivalent)
Flow control:	Hardware handshaking using RS/CS or Non (selectable).

### Connection

Make the connection as shown in the figure below.

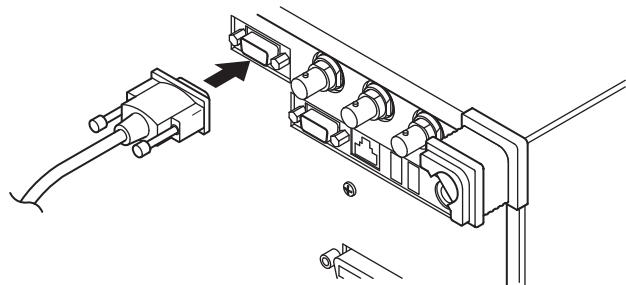


AQ6370C/AQ6373/AQ6375

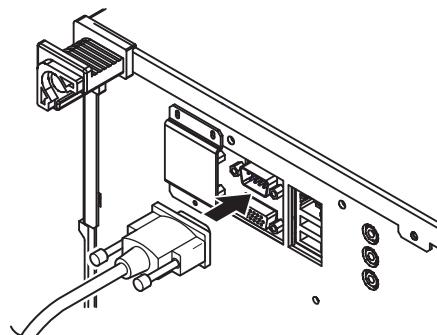

AQ6370D/AQ6373B

#### 4.1 Connecting via the Serial (RS-232C) Interface

##### Connector and Signal Names




DELC-J9PAF-13L6 or equivalent

- |                         |                                                                                   |
|-------------------------|-----------------------------------------------------------------------------------|
| 2 RD (received data):   | Data received from the PC.<br>Signal direction....input                           |
| 3 SD (send data):       | Data sent to the PC.<br>Signal direction....output                                |
| 5 SG (signal ground):   | Ground for the signal.                                                            |
| 7 RS (request to send): | Handshaking method when receiving data from the PC.<br>Signal direction....output |
| 8 CS (clear to send):   | Handshaking method when sending data to the PC.<br>Signal direction....input      |

\* Pins 1, 4, 6, and 9 are not used.


##### 9-Pin to 25-pin Adapter and Signal Names

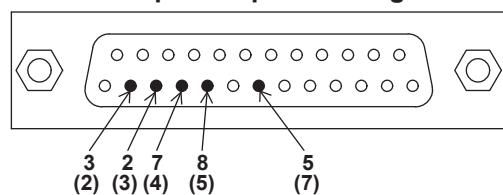

Numbers in parentheses are the pin numbers of the 25-pin connector.

##### Signal Direction

The directions of signals used by the instrument's serial interface are shown in the figure below.

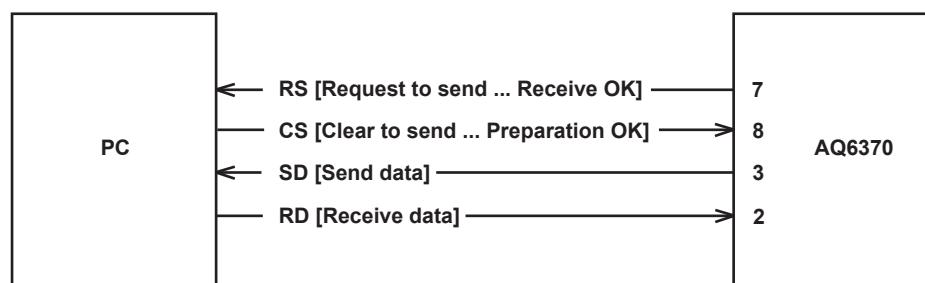

**List of RS-232 Standard Signals and JIS and CCITT Cable Addresses  
Signal Chart**


Pin Number (9-Pin Connector)	Code			Name
	RS-232	CCITT	JIS	
5	AB (GND)	102	SG	Signal ground
3	BA (TXD)	103	SD	Send data
2	BB (RXD)	104	RD	Receive data
7	CA (RTS)	105	RS	Request to send
8	CB (CTS)	106	CS	Clear to send

**Signal Wire Connection Example**


Pin numbers are for 9-pin connectors.

In most cases, use a cross cable.

• OFF-OFF/XON-XON



• Hard(CS-RS)



## 4.2 Remote Control Using Commands

The AQ6370C/AQ6370D/AQ6373/AQ6375 can be controlled remotely using the RS-232 port. When controlling the instrument remotely, use a cross cable to connect the instrument to the PC. Also, remote commands are the same as for remote control via GP-IB.

### Interrupt by SRQ

An SRQ interrupt does not occur during RS-232-based remote control.

### Status Registers

The status registers operate in the same manner as in remote control via the GP-IB interface. Using the “\*STB?” or “SPOLL?” command dedicated for remote control using the LAN port allows you to read the status registers, as in the case with serial polling via the GP-IB interface.

\*STB?: When AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 is the setting of the COMMAND FORMAT key

SPOLL?: When AQ6317 is the setting of the COMMAND FORMAT key

### Delimiter

The delimiter for RS-232-based remote control is fixed to CR + LF.

### Transmission of Talker Data


When the instrument receives talker data from an external PC, the data is sent to the external PC's buffer. It receives the external PC's buffer data and stores the query data.

## 4.3 Setting Up RS-232

### Procedure


#### Selecting the Communication Interface

1. Press **SYSTEM**. The system setting menu is displayed.
2. Press the **MORE1/4** soft key. The communication interface setting menu is displayed.
3. Press the **REMOTE INTERFACE** soft key. The setting menu for the interface to be used is displayed.
4. Press the **RS-232** soft key to specify **RS-232** as the communication interface.

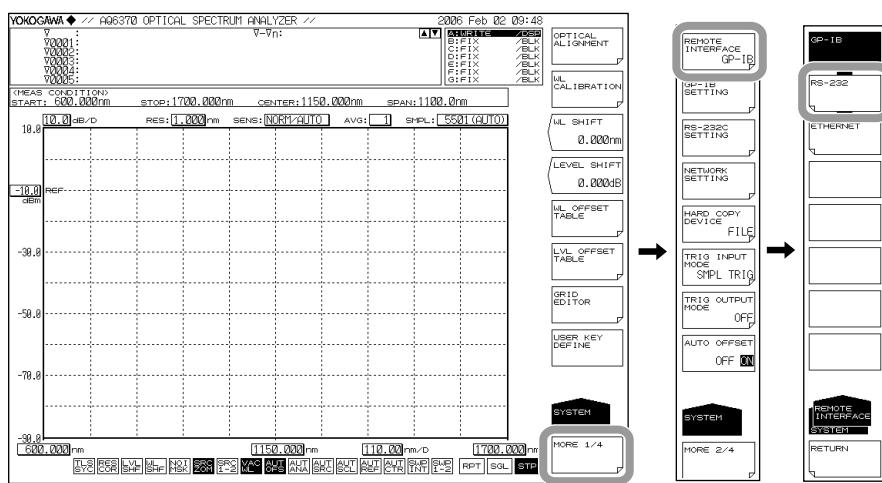


#### Setting the Baud Rate

5. Press the **RS-232 SETTING** soft key. The RS-232 setting menu is displayed.
6. Press the **BAUD RATE** soft key. The baud rate setting menu is displayed.
7. Press the soft key corresponding to the desired baud rate setting. The baud rate is set.

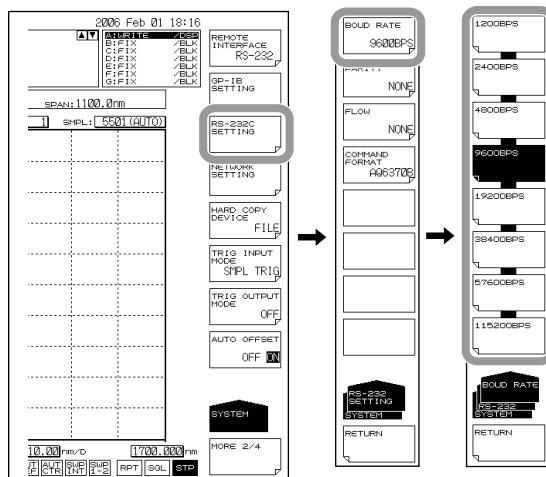


### Setting the Parity

8. Press the **PARITY** soft key. The parity setting menu is displayed.
9. Press the soft key corresponding to the desired parity setting. The parity is set.



### Setting the Flow Control

10. Press the **FLOW** soft key. The flow control setting menu is displayed.
11. Press the soft key corresponding to the desired flow control setting. The flow control is set.



### Setting the Command Format

12. Perform these steps if you will use AQ6317 commands.  
Press the **COMMAND FORMAT** soft key. The command format setting menu is displayed.
13. Normally, you will enter AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375. If you wish to use AQ6317 commands, enter AQ6317.

## Explanation

The settings below are used when entering the settings that can be entered using the instrument's panel keys from a controller, or when outputting settings or waveform data to the controller.

### Baud Rate Setting

Select a baud rate from the following.

1200 bps, 2400 bps, 4800 bps, 9600 bps, 19200 bps, 38400 bps, 57600 bps, or 115200 bps

### Parity Rate Setting

Select a parity from the following.

NONE, ODD, or EVEN

### Flow Control Setting

Select a Transmission data control-Receive data control from the following.

Xon/Xoff, HARDWARE, NONE

### Setting the Command Format

Normally, you will enter AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375 mode.

If you wish to use the commands of the AQ6317 (another product in the series), enter AQ6317. See the appendix for AQ6317 commands that are compatible with the AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375.

## 5.1 Connecting via GP-IB2

### GP-IB Cable

This instrument is equipped with an IEEE standard 488-1978 24-pin GP-IB connector. Use a GP-IB cable that conforms to the IEEE standard 488-1978.

### Connections

The instrument has two ports, GP-IB1 and GP-IB2. The GP-IB2 port is not available on the AQ6370D/AQ6373B.

GP-IB1 port: Can be connected to a PC for remote control of the instrument from the PC.

GP-IB2 port: Can be connected to another instrument for remote control of that instrument using the AQ6370C/AQ6373/AQ6375's program function.

For now, you will connect a PC to the GP-IB2 port.

Turn OFF all the power switches of the AQ6370C/AQ6373/AQ6375 and any devices to be connected to it. Connect a cable to the GP-IB2 port on the rear panel of the instrument.


### CAUTION

Always turn OFF the power to the instrument and the PC when connecting or disconnecting communication cables. Failure to turn OFF the power can result in malfunction or damage to internal circuitry.

### French

### ATTENTION

Veillez à mettre le PC et l'oscilloscope DLM4000 hors tension lorsque vous branchez ou débranchez les câbles de communication, car cela risquerait de provoquer des dysfonctionnements ou des courts-circuits internes.

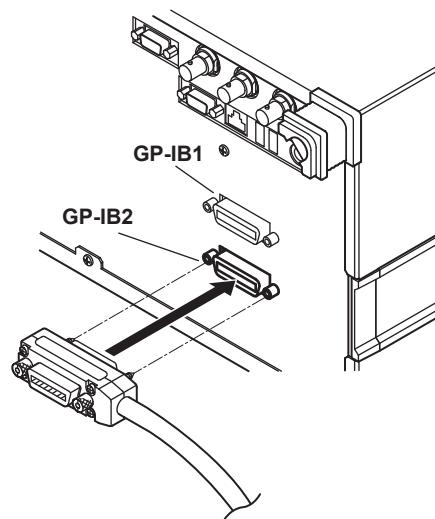

AQ6370C/AQ6373/AQ6375

For precautions when making connections, see chapter 2, section 2.1, "Connecting via GP-IB."

## 5.2 GP-IB Interface Specifications

### GP-IB Interface Specifications

Electromechanical specifications:	Conforms to IEEE std. 488-1978
Functional specifications:	See table below
Protocols:	Conforms to IEEE std. 488.2-1992
Encoding:	ISO (ASCII)
Mode:	Addressable mode
Address setting:	Addresses 0-30 can be set in the GP-IB setting screen in the SYSTEM menu.
Remote mode cancel:	Press LOCAL to cancel Remote mode. Note that this is disabled when under Local Lockout by the controller.

### Functional Specifications


Function	Subset	Description
Source handshake	SH1	All capabilities of send handshake
Acceptor handshake	AH1	All capabilities of receive handshake
Talker	T4	Basic talker function
Listener	L2	Basic listener function
Service request	SR0	Service request function not provided
Remote local	RL0	Local lockout function not provided
Parallel port	PP0	Parallel polling function not provided
Device clear	DC0	Device clear function not provided
Device trigger	DT0	Device trigger function
Controller	C1 C2 C3	System controller IFC transmission Controller in charge REN transmission
C28		Interface message transmission
Electrical characteristics	E1	Open collector

## 5.3 Setting the GP-IB Address

### Procedure


#### Selecting the Communication Interface

1. Press **SYSTEM**. The system setting menu is displayed.
2. Press the **MORE1/4** soft key. The communication interface setting menu is displayed.
3. Press the **REMOTE INTERFACE** soft key. The setting menu for the interface to be used is displayed.
4. Press the **GP-IB** soft key to specify GP-IB as the communication interface.

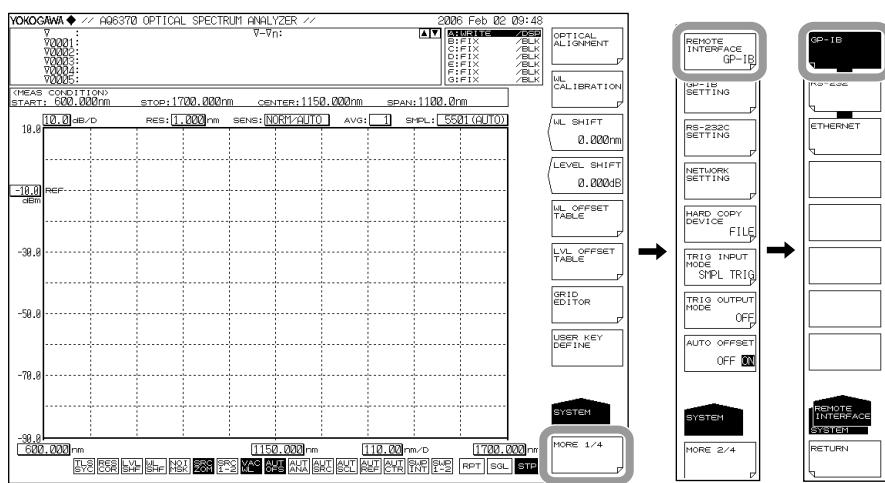

#### Setting the Address

5. Press the **GP-IB SETTING** soft key. The GP-IB setting menu is displayed.
6. Press the **GP-IB2 PORT ADDRESS** soft key. The GP-IB2 port address setting screen is displayed.
7. Set the GP-IB2 port address using the **rotary knob** or the **arrow keys**, and press **ENTER**.

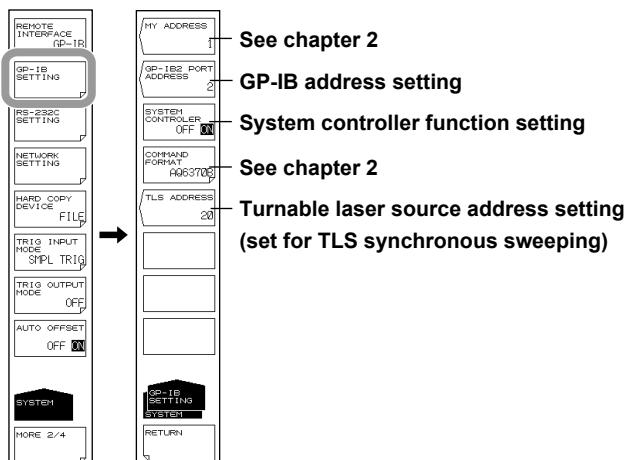

### 5.3 Setting the GP-IB Address

---

#### Turning the System Controller Function ON and OFF (On the AQ6370C, AQ6373 or AQ6375)

8. Press the **SYSTEM CONTROLLER** soft key to turn the function ON or OFF.  
Turn it ON to control an external device.

#### Setting the GP-IB Address of the Turnable Laser Source (for Synchronous Sweeping; On the AQ6370C, AQ6373 or AQ6375)

9. Press the **TLS ADDRESS** soft key. The TLS address setting screen is displayed.
10. Set the TLS address using the **rotary knob** or the **arrow keys**, and press **ENTER**.

#### Explanation

Enter the following settings to control an external device with the instrument's program function.

##### Setting the GP-IB2 Port Address

When in Addressable mode, set the instrument's address within the following range.

0–30

Each device that can be connected via GP-IB has its own unique GP-IB address. This address allows each device to be distinguished from other devices. Therefore, make sure not to set the same address on the instrument as any of the other devices. Also, set addresses other than the instrument's GP-IB address (MY ADDRESS).

##### Turning ON the System Controller Function

Turn ON this function to control an external device with the instrument's program function.

##### Setting the TLS Address

Specify the GP-IB address of the turnable laser source to be controlled by the instrument.

##### Note

- 
- A controller such as a PC that is connected to the GP-IB2 port cannot remotely control the AQ6370C/AQ6373/AQ6375.
  - Even if a turnable laser source or an external device to be controlled by the AQ6370C/AQ6373/AQ6375 using program functions is connected to the GP-IB1 port, it cannot remote control the AQ6370C/AQ6373/AQ6375.
  - The GP-IB1 and GP-IB2 ports are independent of each other. Thus, a controller connected to the GP-IB1 port cannot directly send a message to an external device connected to the GP-IB2 port.
  - When a PC or other controller is connected to the GP-IB1 port, connecting the GP-IB1 port with the GP-IB2 port results in improper operation. Do not connect these ports together, or turn OFF the system controller function. The default is ON.
-

## 6.1 Status Registers

This instrument is equipped with the status registers shown in the table below. See the next page for a diagram of all status registers.

This instrument has the following status registers defined by IEEE 488.2 and SCPI:


- Status byte registers
- Standard event registers
- Operation status registers
- Questionable status registers

Also, this instrument has an operation status bit (OPS) and a questionable status bit (QUS), each of which contains the summary information of each piece of register information, as the extension bits of the status byte register.

### List of Status Registers

Register Name	Description
Status byte registers	Register defined by IEEE 488.2
STB: Status Byte Register	Same as the above
SRE: Service Request Enable Register	Same as the above
Standard event registers	Register defined by IEEE 488.2
ESR: Standard Event Status Register	Same as the above
ESE: Standard Event Status Register	Same as the above
Operation status registers	Provides information on operation execution (such as being swept, copied, or under calibration).
Operation Event Register	A register indicating the presence/absence of an event. Event will be latched.
Operation Event Enable Register	A condition mask register used when the summary bit (OPS) is created.
Questionable status registers	Not assigned yet.
Questionable Event Register	A register indicating the presence/absence of an event. An event will be latched.
Questionable Event Enable Register	A condition mask register used when the summary bit (QUS) is created.

## 6.1 Status Registers

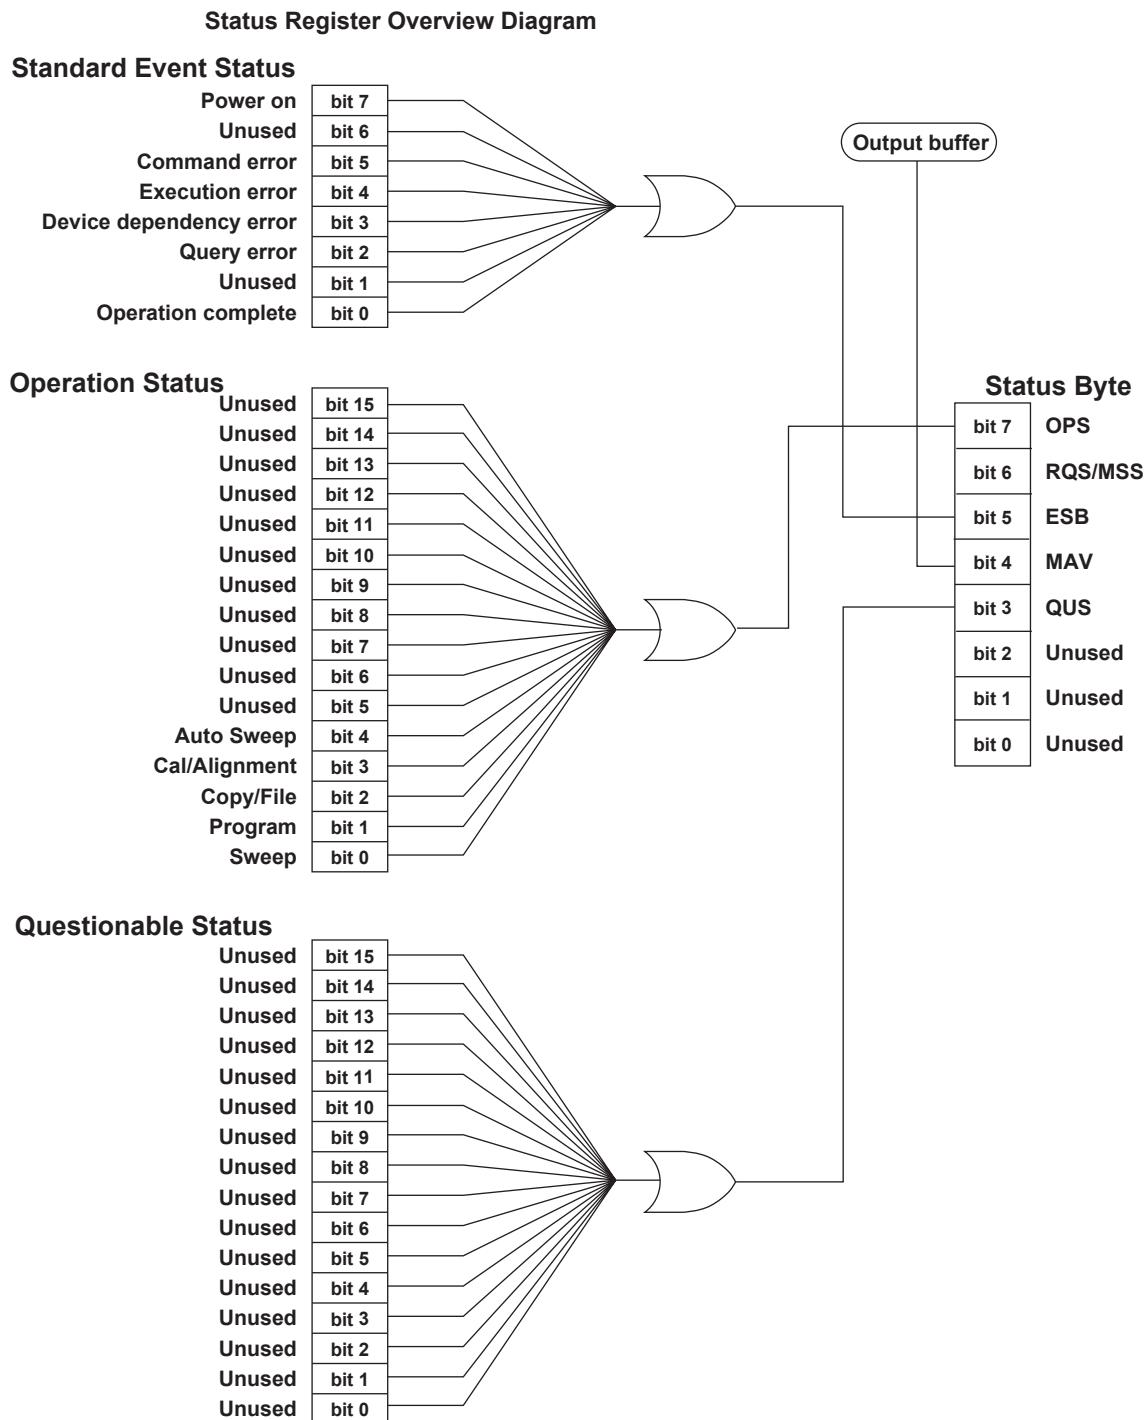


## 6.2 Status Byte Registers

### Structure

The structure of the status byte registers is shown below. The contents and actions of these registers comply with the IEEE 488.2 standards.

Also, the AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 also provides the extended OPS and QUS bits to the status byte register.

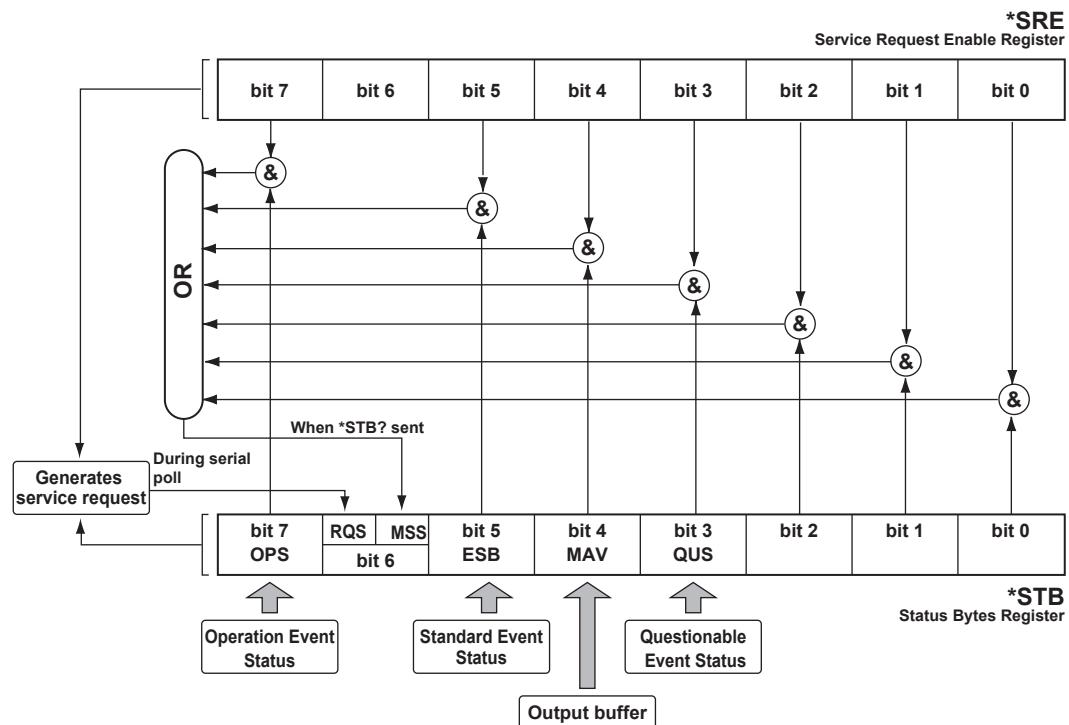

### Status Byte Register Contents

Bit	Event Name	Description	Decimal Value
Bit 7	OPS	Summary bit of operation status	128
Bit 6	RQS, MSS	"1" if there is more than one service request	64
Bit 5	ESB	Summary bit of standard event status register	32
Bit 4	MAV	"1" if the output buffer contains data	16
Bit 3	QUIS	Summary bit of questionable status	8
Bit 2	None	Not used (always 0)	0
Bit 1	None	Not used (always 0)	0
Bit 0	None	Not used (always 0)	0

## 6.2 Status Byte Registers

---

### Status Byte Register

#### Read

This register can be read by a serial poll or the common \*STB? query. Note that the information of bit 6 changes with a different reading method.

- When read by serial polling  
An RQS message is read as bit 6 information.  
After reading, the RQS message will be cleared.
- When read by an \*STB? common query  
An MSS summary message is read as bit 6 information.  
Even after reading, the MSS message will be held.

Bits other than bit 6 do not change.

The read action complies with the IEEE 488.2 standard.

#### Write

The contents of the register will be rewritten only when the status of an assigned status data structure has been changed. The write action complies with the IEEE 488.2 standard.

#### Clear

All event registers and queues, not including the output queues and MAV bit, will be cleared by the common \*CLS command.

The clear action complies with the IEEE 488.2 standard.

### Service Request Enable Register

#### Read

This register can be read by the common \*SRE? query.

The value of bit 6, an unassigned bit, is always “0.” The contents of the register are not cleared even when read. The read action complies with the IEEE 488.2 standard.

#### Write

This register can be written by the common \*SRE command.

The set value of bit 6, an unassigned bit, is always ignored. The write action complies with the IEEE 488.2 standard.

#### Clear

This register will be cleared under any of the following conditions.

- Data “0” is set using the common \*SRE command.
- Power ON

The contents of the register are not cleared in the following cases.


- Receipt of the \*RST command
- Receipt of the \*CLS command
- Device clear (DCL, SDC)

The clear action complies with the IEEE 488.2 standard.

## 6.3 Standard Event Status Registers

### Structure

The structure of the standard event status registers is shown below. The contents and actions of the registers comply with the IEEE 488.2 standards.

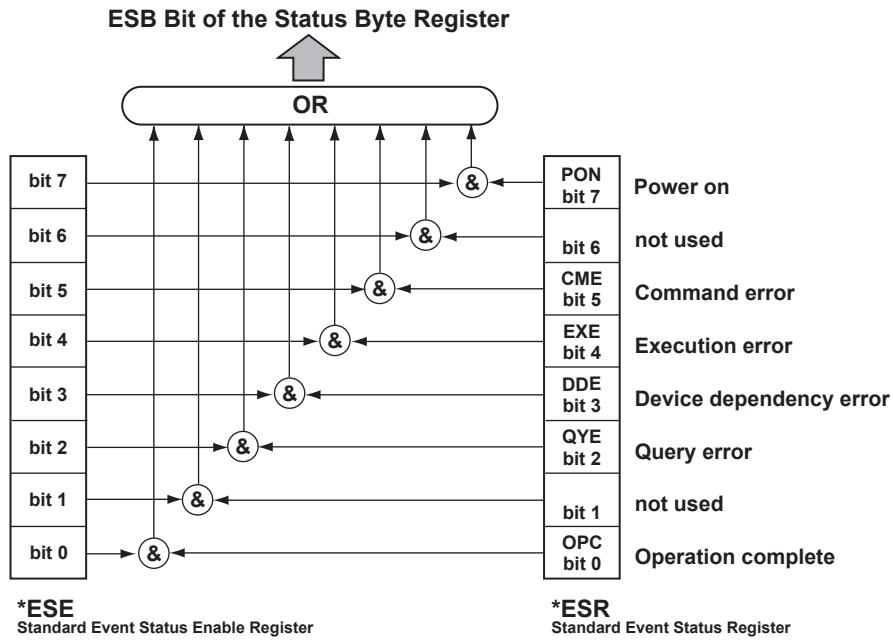

### Contents of the Standard Event Status Registers

Bit	Event Name	Description	Decimal Value
Bit 7	PON (Power ON)	Power is turned ON. Set to "1" at startup.	128
Bit 6	None	Not used (always 0)	0
Bit 5	CME (command error)	A syntax error or unrecognizable command is detected. GET is encountered between the 1st byte of a program message and the program message terminator.	32
Bit 4	EXE (Execution error)	Program data following the program header is out of the effective range. Receipt of a program message contradictory to device state.	16
Bit 3	DDE (Device-specific error)	Error caused by an event other than CME, EXE, or QYE.	8
Bit 2	QYE (Query error)	Access to an output queue was made with no output existing. Output queue data was lost.	4
Bit 1	None	Not used (always 0)	0
Bit 0	OPC (operation complete)	Completion of command action: Enabled only when *OPC is received Disabled if *OPC? is received	1

## 6.3 Standard Event Status Registers

---

### Standard Event Status Register

#### Read

This register can be read by the common \*ESR? query.

Its contents will be cleared when read. The read action complies with the IEEE 488.2 standard.

#### Write

Contents of the register can be cleared. The register can be cleared but not written to.

#### Clear

This register will be cleared under any of the following conditions.

- Common \*CLS command
- Common \*ESR? query

The clear action complies with the IEEE 488.2 standard.

### Standard Event Status Enable Register

#### Read

This register can be read by the common \*ESE? query.

The read action complies with the IEEE 488.2 standard.

#### Write

This register can be written by the common \*ESE command.

The write action complies with the IEEE 488.2 standard.

#### Clear

This register will be cleared under any of the following conditions.

- Data "0" is set using the common \*ESE command.
- Power ON

The register cannot be cleared in the following cases.

- Receipt of the \*RST command
- Receipt of the \*CLS command
- Device clear (DCL, SDC)

The clear action complies with the IEEE 488.2 standard.

## 6.4 Operation Status Registers


Operation status registers report the operation status of the instrument. The operation condition registers indicate the instrument's condition. A change in an operation condition register is latched into the operation event register. The user can refer to the operation event register to view changes in the operation status. The summary information of the instrument event register is set to the OPS bit of the status byte register. In this case, only statuses corresponding to bits specified as "1" in the operation enable register are included in the summary information.

### Structure

The structure of the operation status register is shown below.

#### Structure of the Operation Status Register

##### OPS Bit of the Status Byte Register

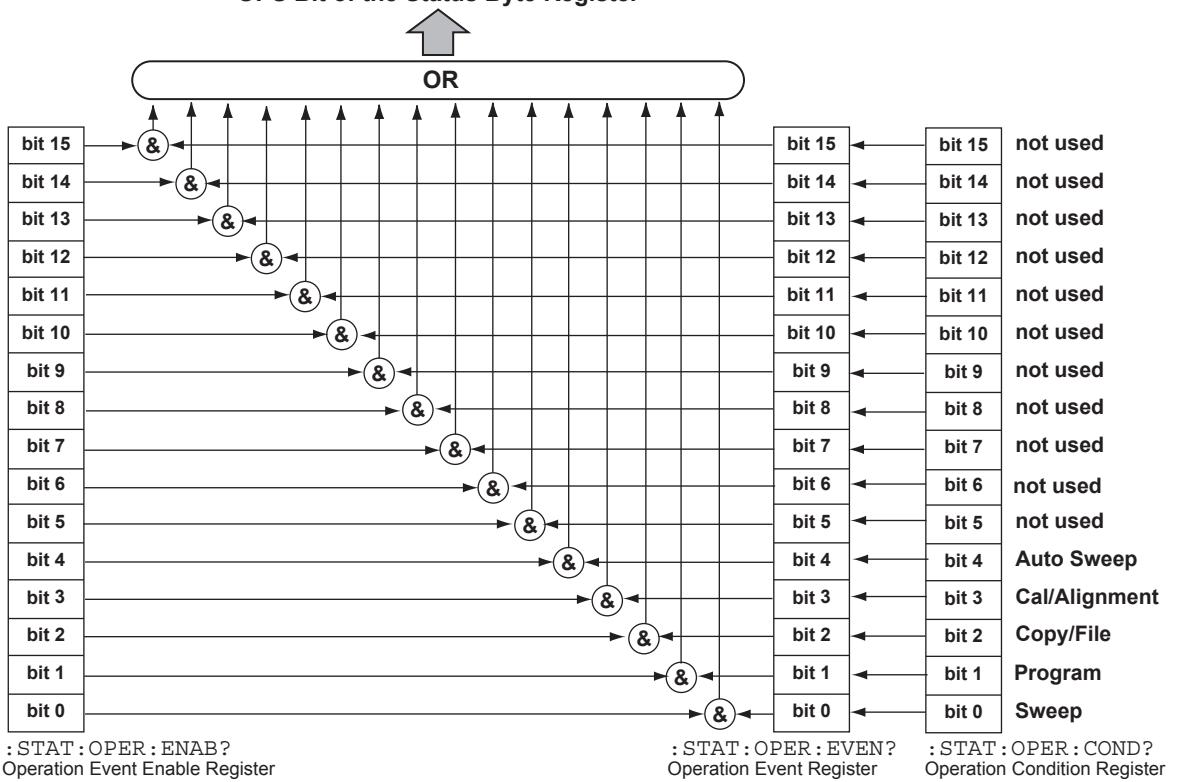

## 6.4 Operation Status Register

### Contents of the Operation Status Register

Bit	Event Name	Description	Decimal Value
Bit 15	Not used	Spare (always 0)	0
Bit 14	Not used	Spare (always 0)	0
Bit 13	Not used	Spare (always 0)	0
Bit 12	Not used	Spare (always 0)	0
Bit 11	Not used	Spare (always 0)	0
Bit 10	Not used	Spare (always 0)	0
Bit 9	Not used	Spare (always 0)	0
Bit 8	Not used	Spare (always 0)	0
Bit 7	Not used	Spare (always 0)	0
Bit 6	Not used	Spare (always 0)	0
Bit 5	Not used	Spare (always 0)	0
Bit 4	Auto Sweep	Completion of auto sweep running action	16
Bit 3	Cal/Alignment	Completion of wavelength calibration, alignment or resolution calibration	8
Bit 2	Copy/File	Completion of printout or file operation	4
Bit 1	Program	Completion of execution of the program functions	2
Bit 0	Sweep	Completion of a sweep	1

## Operation Condition Register

### Read

This register can be read by the :STATus:OPERation:CONDition? query command. Its contents will not be cleared even when read.

### Write

The register sets or resets a bit corresponding to a change in the status of the instrument only when that change occurs. It cannot be written to.

### Clear

The register cannot be cleared.

## Operation Event Register

### Read

This register can be read by the :STATus:OPERation[:EVENT?] query command. Its contents will be cleared when read.

### Write

Contents of the register can be cleared. The register can be cleared but not written to.

#### <Clear>

This register will be cleared under any of the following conditions.

- A read using the :STATus:OPERation[:EVENT?] query command
- An initialization by the :STATus:PRESet command
- The \*CLS common command
- Power ON
- Operation event enable register

### Read

This register can be read by the :STATus:OPERation:ENABLE? query command.

**Write**

The register can be written by the :STATus:OPERation:ENABLE command.

**Clear**

This register will be cleared under any of the following conditions.

- Data “0” is set by the :STATus:OPERation:ENABLE command.
- Power ON

The register cannot be cleared in the following cases.

- Receipt of the \*RST command
- Receipt of the \*CLS command
- Device clear (DCL, SDC)


## 6.5 Questionable Status Registers

The questionable status registers report the questionable status of the instrument. All bits of these registers are unassigned. However, the register read/write operations are performed normally. The summary information of an event register will be set to the QUS bit of the status byte register.

### Structure

The structure of the questionable status registers is shown below.

#### Structure of the Questionable Status Registers

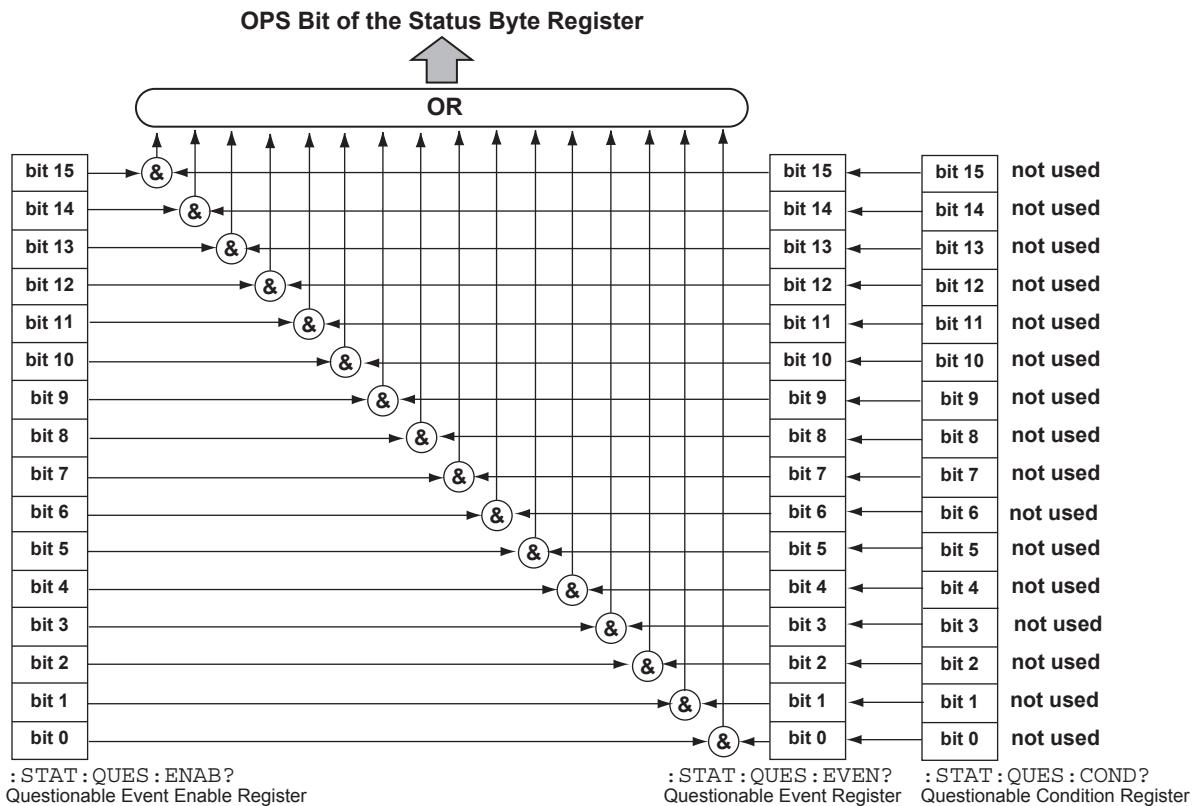

#### Contents of the Questionable Status Registers

Bit	Event Name	Description	Decimal Value
Bit 0–15	Not used	Spare (always 0)	0

## Questionable Condition Register

### Read

This register can be read by the :STATus:QUEStionable:CONDition? query command. Its contents will not be cleared even when read.

### Write

The register sets or resets a bit corresponding to a change in the status of the instrument only when that change occurs. It cannot be written to.

### Clear

The register cannot be cleared.

## Questionable Event Register

### Read

This register can be read by the :STATus:QUEStionable[:EVENT?] query command. Its contents will be cleared when read.

### Write

Contents of the register can be cleared. The register can be cleared but not written to.

### Clear

This register will be cleared under any of the following conditions.

- A read using the :STATus:QUEStionable[:EVENT?] query command
- Initialization by the :STATus:PRESet command
- Common \*CLS command
- Power ON

## Questionable Event Enable Register

### Read

This register can be read by the :STATus:QUEStionable:ENABLE? query command.

### Write

The register can be written to by the :STATus:QUEStionable:ENABLE command.

### Clear

This register will be cleared under any of the following conditions.

- Data “0” is set using the :STATus:QUEStionable:ENABLE command.
- Power ON

The register cannot be cleared in the following cases.

- Receipt of the \*RST command
- Receipt of the \*CLS command
- Device clear (DCL, SDC)

## 7.1 Rules of Syntax and Command Types

The following information is intended for the common commands and instrument-specific commands contained in this manual. Measured values and parameters are all sent and received using ASCII characters, not including special commands.

### Description of Rules of Syntax

Rule	Description
	Indicates that one of the elements in a list should be selected. E.g.: A B C = A, B, or C is used
[ ]	An item in square brackets is specified as desired.
{ }	An item in curly brackets can be specified multiple times within a command.
<wsp> <sup>1</sup>	Space
<integer>	Integer
<NRf>	Exponent indicating value
<"file name">	A file name can be a maximum of 56 characters, including extensions, excluding the directory part. Enclose a character string using double quotations ("").
<trace name>	Trace name (TRA TRB TRC TRD TRE TRF TRG)
<marker>	Marker number (0: moving marker, 1 to 1024: fixed markers)
<"string">	Character string Enclose a character string using double quotations ("").

1. Regarding white space (<wsp>):

*White space* is defined as a character corresponding to 00h to 20h (not including 0Ah (LF)) of the ASCII character sets. Aside from inserting it between a command and parameters (when specifying parameters) or using it as space in a character string such as a file name in a parameter, white space can be inserted as desired to make a program legible.

### Types of Commands

This unit's commands can be classified into the following three types:

#### Sequential Commands

- These commands are the most general commands.
- The action of another command is not performed until the running of a sequential command is complete.
- Another action is not started until the running of the other command is complete.

#### Overlappable Commands

- An overlappable command allows execution of an overlapping command while it is being run.

Ex. of command: :INITialte Makes a sweep.

#### Overlapping Commands

- An overlapping command can be executed while an overlappable command is being run.
- These commands cannot be executed while a sequential command is being executed or if it has not yet been processed.

Ex. of command: :ABORT Stops measurement or calibration action.  
\*STB? Reads status byte.

### Collective Transmission of Multiple Commands

You can create a command string using the commands described in section 7.5, "Common Commands," and section 7.6, "Instrument-Specific Commands" and send it to the instrument. If multiple commands are written in a single output statement by using a semicolon ";" to delimit each command, the commands will be executed in the order in which they have been written.

### Format of a Remote Command

#### Short and Long Forms

The instrument's GP-IB commands support both short and long forms.

For the commands contained in this manual, the part written in capital letters is the short form of the command concerned. The short form of the INITiate command is INIT.

#### Upper- and Lower-Case Letters

The instrument does not distinguish between upper- and lower-case letters.

Return values are all in upper-case letters.

### Grouping of SCPI Commands Using a Subsystem

The instrument supports the subsystem-based grouping of the SCPI commands.

Commands belonging to the same sub-system and existing at the same tree of the hierarchical structure of the subsystem can be sent in combination. In this case, each command should be delimited by a semicolon.

#### List of GP-IB commands used in examples

- |        |             |  |
|--------|-------------|--|
| :SENSe | :SETTing    |  |
|        | :ATTenuator |  |
|        | :WAVelength |  |
|        | :STOP       |  |
|        | :START      |  |
- SENSe:WAVelength:STARt 1500NM;STOP 1600NM (Y)
  - SENSe:WAVelength:STARt 1500NM;ATTenuator ON (X)  
(Reason: They are not in the same hierarchy.)
  - SENSe:WAVelength:STARt 1500NM;:STOP 1600NM (X)  
(Reason: A colon ":" is unnecessary after a semicolon ";".)

### Numerics

- This instrument supports multiple notation methods when receiving a numeric(s).
- This instrument uses only the basic units when transmitting a numeric(s).

The number of digits for the real part is fixed to a one digit integer (with a sign) and eight digits for decimal places. The number of digits for the exponential part is fixed to 3.

Ex.: Receivable numerics (in case of 1550 nm)

1550 nm, 1.55 um, 1550E-9, 1.55E-6, and others

Ex.: Transmittable numerics (in case of 1550 nm)

+1.5500000E-006 only

- If a received numeric has a precision higher than the range of numerics handled inside this unit, lower decimal places will be rounded off rather than being discarded.
- This instrument can handle the following multiplier suffixes:

Multiplier	Mnemonic	Multiplier	Mnemonic
1E18	EX (exa)	1E-3	M (milli)
1E15	PE (peta)	1E-6	U (micro)
1E12	T (tera)	1E-9	N (nano)
1E9	G (giga)	1E-12	P (pico)
1E6	MA (mega)	1E-15	F (femto)
1E3	K (kilo)	1E-18	A (atto)

### Specification of Parameters in a Command

To use parameters in a command, a space must be placed between the command and parameters. Each parameter is delimited by a comma “,”. A space may also be placed before and after a comma to make the command legible.

### AQ6317-Compatible Commands

The instrument supports AQ6317-compatible GP-IB commands. When using AQ6317-compatible GP-IB commands, call up the **SYSTEM** menu using the SYSTEM key and place the instrument in AQ6317-compatible mode.

### Differences from the AQ6370

This instrument's remote commands differ from those of the AQ6370 in the following respects.

**1. \*IDN query talker data**

AQ6370: "YOKOGAWA, AQ6370,---"  
 AQ6370C: "YOKOGAWA, AQ6370C,---"  
 AQ6370D: "YOKOGAWA, AQ6370D,---"  
 AQ6373: "YOKOGAWA, AQ6373,---"  
 AQ6373B: "YOKOGAWA, AQ6373B,---"  
 AQ6375: "YOKOGAWA, AQ6375,---"

**2. “CHOP” was eliminated from the <CHOP MODE> settings.**

If the AQ6370C/AQ6370D/AQ6373/AQ6373B receives a command that specifies “CHOP,” it is treated as “SWITCH.”

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

The tables below list the remote commands that correspond to the soft keys used when manipulating the various settings of the instrument.

If a command is valid for either the AQ6370C or AQ6375 only, the relevant model name is indicated in the notes.

For the AQ6370C, AQ6373, and AQ6375, if commands are valid for only some of the instruments, the models are indicated in the remarks column. Models are not noted for commands that are valid for all instruments.

### SWEEP

Function	Control Command
AUTO	:INITiate:SMODe<wsp>AUTO 3;INITiate
REPEAT	:INITiate:SMODe<wsp>REPeat 2;INITiate
SINGLE	:INITiate:SMODe<wsp>SINGle 1;INITiate
STOP	:ABORT
SEGMENT MEASURE	:INITiate:SMODe<wsp>SEGment 4;INITiate
SEGMENT POINT****	:SENSe:SWEep:SEGment:POINTS<wsp><integer>
SWEEP MKR L1-L2 ON/OFF	:SENSe:WAVelength:SRAnge<wsp>OFF ON 0 1
SWEEP INTVL ****sec	:SENSe:SWEep:TIME:INTerval<wsp><integer>[SEC]

### CENTER

Function	Control Command	Remarks
CENTER WL ****.***nm	:SENSe:WAVelength:CENTER<wsp><NRf>[M]	
CENTER FREQ ***.***THz	:SENSe:WAVelength:CENTER<wsp><NRf>[HZ]	
CENTER WNUM ****.***cm-1	:SENSe:WAVelength:CENTER<wsp><NRf>	AQ6375
START WL ****.***nm	:SENSe:WAVelength:START<wsp><NRf>[M]	
START FREQ ***.***THz	:SENSe:WAVelength:START<wsp><NRf>[HZ]	
STOP WNUM ****.***cm-1	:SENSe:WAVelength:START<wsp><NRf>	AQ6375
STOP WL ****.***nm	:SENSe:WAVelength:STOP<wsp><NRf>[M]	
STOP FREQ ***.***THz	:SENSe:WAVelength:STOP<wsp><NRf>[HZ]	
START WNUM ****.***cm-1	:SENSe:WAVelength:STOP<wsp><NRf>	AQ6375
PEAK → CENTER	:CALCulate:MARKer:SCENter	
AUTO CENTER ON/OFF	:CALCulate:MARKer:MAXimum:SCENter:AUTO<wsp>OFF ON 0 1	
VIEW→MEAS	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:SMScale	

### SPAN

Function	Control Command	Remarks
SPAN****.*nm	:SENSe:WAVelength:SPAN<wsp><NRf>[M]	
SPAN WNUM****.*cm-1	:SENSe:WAVelength:SPAN<wsp><NRf>	AQ6375
START WL ****.***nm	:SENSe:WAVelength:START<wsp><NRf>[M]	
START FREQ ***.***THz	:SENSe:WAVelength:START<wsp><NRf>[HZ]	
START WNUM****.***cm-1	:SENSe:WAVelength:START<wsp><NRf>	AQ6375
STOP WL ****.***nm	:SENSe:WAVelength:STOP<wsp><NRf>[M]	
STOP FREQ ***.***THz	:SENSe:WAVelength:STOP<wsp><NRf>[HZ]	
STOP WNUM****.***cm-1	:SENSe:WAVelength:STOP<wsp><NRf>	AQ6375
0nm SWEEP TIME**sec	:SENSe:SWEep:TIME:0NM<wsp><integer>[SEC]	
VIEW→MEAS	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:SMScale	

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### LEVEL

Function	Control Command
REF LEVEL	
LOG	:DISPlay[:WINDOW]:Y1[:SCALE]:RLEVel<wsp><NRf>[D BM]
LINEAR	:DISPlay[:WINDOW]:Y1[:SCALE]:RLEVel<wsp><NRf> [NW UM MW]
LOG SCALE**.*dB/D	:DISPlay[:WINDOW]:TRACe:Y1[:SCALE]:PDIVision<wsp> <NRf> [DB]
LIN SCALE	:DISPlay[:WINDOW]:TRACe:Y1[:SCALE]:SPACing<wsp> LINEar 1
LIN BASE LEVEL**.*mW	:DISPlay[:WINDOW]:Y1[:SCALE]:BLEvel<wsp><NRf>[MW]
PEAK→REF LEVEL	:CALCulate:MARKer:MAXimum:SRLevel

### Function

Function	Control Command
AUTO REF LEVEL ON/OFF	:CALCulate:MARKer:MAXimum:SRLevel:AUTO
LEVEL UNIT dBm / dBm/nm	:DISPlay[:WINDOW]:TRACe:Y1[:SCALE]:UNIT<wsp> DBM DBM/NM
Y SCALE SETTING	
Y SCALE DIVISION 8/10/12	:DISPlay[:WINDOW]:TRACe:Y[:SCALE]:DNUmber<wsp> 8  10 12
REF LEVEL POSITION **DIV	:DISPlay[:WINDOW]:TRACe:Y1[:SCALE]:RPosition<wsp> <integer>[DIV]
SUB LOG**.*dB/D	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:PDIVision<wsp> <NRf>[DB]
SUB LIN**.*%/D	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:PDIVision<wsp> <NRf>
SUB SCALE**.*dB/km	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:PDIVision<wsp> <NRf>[DB/KM]
SUB SCALE**.*%/D	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:PDIVision<wsp> <NRf>[%]
OFST LVL or SCALE MIN **.*dB	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:OLEvel<wsp> <NRf>[DB]
LENGTH**.*km	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:LENGTH<wsp> <NRf>[KM]
AUTO SUB SCALE ON/OFF	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:AUTO<wsp>OFF  ON 0 1
SUB REF LVL POSITION **DIV	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:RPosition<wsp> <integer>[DIV]

### Note

For the AQ6375, dBm/nm and W/nm cannot be selected for LEVEL UNIT when the horizontal axis is wavenumber. (DBM/NM parameters cannot be set. )

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### SETUP

Function	Control Command	Remarks
RESOLUTION *.*nm	:SENSe:BANDwidth[:BWIDth][:RESolution]<wsp><NRf>[M Hz]	
SENS/MODE @@@@		
NORM/HOLD	:SENSe:SENSe<wsp>NHLD 0	
NORM/AUTO	:SENSe:SENSe<wsp>NAUT 1	
NORM	:SENSe:SENSe<wsp>NORMal 6	
MID	:SENSe:SENSe<wsp>MID 2	
HIGH1	:SENSe:SENSe<wsp>HIGH1 3	AQ6370C/AQ6373/ AQ6370D/AQ6373B
HIGH1/CHOP	:SENSe:SENSe<wsp>HIGH1 3	AQ6375
HIGH2	:SENSe:SENSe<wsp>HIGH2 4	AQ6370C/AQ6373/ AQ6370D/AQ6373B
HIGH2/CHOP	:SENSe:SENSe<wsp>HIGH2 4	AQ6375
HIGH3	:SENSe:SENSe<wsp>HIGH3 5	AQ6370C/AQ6373/ AQ6370D/AQ6373B
HIGH3/CHOP	:SENSe:SENSe<wsp>HIGH3 5	AQ6375
CHOP MODE @@@@		
OFF	:SENSe:CHOPPer<wsp>OFF 0	AQ6370C/AQ6373/ AQ6370D/AQ6373B
SWITCH	:SENSe:CHOPPer<wsp>SWITch 2	AQ6370C/AQ6373/ AQ6370D/AQ6373B
AVG TIMES ***	:SENSe:AVERage:COUNT<wsp><integer>	
SAMPLING POINT	:SENSe:SWEep:POInTs:AUTO<wsp>OFF  ON 0 1	
SAMPLING POINT ****	:SENSe:SWEep:POInTs<wsp><integer>	
SAMPLING INTVL	:SENSe:SWEep:STEP<wsp><NRf> [M]	
*.*nm		
MEAS WL AIR/VAC	:SENSe:CORRection:RVELOCITY:MEDium <wsp>AIR VACuum 0 1	
SWEET SPEED 1x/2x	:SENSe:SWEep:SPEed<wsp>1x 2x 0 1	AQ6370C/ AQ6373B/AQ6370D
HORZN SCALE nm/Thz	:UNIT:X<wsp>WAveLength FREQuency 0 1	AQ6370C/AQ6373/ AQ6370D/AQ6373B
HORZN SCALE @@@@		
nm	:UNIT:X<wsp>WAveLength 0	
Thz	:UNIT:X<wsp>FREQuency 1	
cm-1	:UNIT:X<wsp>WNUMber 2	AQ6375
PLS LIGHT MEASURE		
PEAK HOLD	:TRIGger[:SEQUence]:STATE<wsp>	AQ6370C/
**msec	OFF ON PHOLd 0 1 2	AQ6370D/AQ6373B
EXT TRIGGER	:TRIGger[:SEQUence]:STATE<wsp>	AQ6370C/
MODE	OFF ON PHOLd 0 1 2	AQ6370D/AQ6373B
GATE MODE	:TRIGger[:SEQUence]:GATE:TIME	AQ6370C/
***.*msec		AQ6370D/AQ6373B
GATE LOGIC	:TRIGger[:SEQUence]:GATE:LOGic	AQ6370C/
		AQ6370D/AQ6373B
TRIGGER SETTING		
EDGE RISE/FALL	:TRIGger[:SEQUence]:SLOPe<wsp>RISE  FALL 0 1	
DELAY ****.*μs	:TRIGger[:SEQUence]:DELy<wsp><NRf> [S]	
TLS SYNC SWEEP ON/OFF	:SENSe:SWEep:TLSSync<wsp>OFF ON 0 1	AQ6370C/AQ6375
RESOLN CORRECT	:SENSe:SETting:CORRection<wsp> OFF ON 0 1	AQ6370C/AQ6373/ AQ6370D/AQ6373B
SMOOTHING ON/OFF	:SENSe:SETting:SMoothering<wsp> OFF ON 0 1	AQ6373/AQ6373B
FIBER CORE SIZE	:SENSe:SETting:FIBer<wsp>SMAll LAR Ge 0 1	AQ6373/AQ6373B
FIBER CONNECTOR	:SENSe:SETting:FCOnnector<wsp> NORMAL ANGLeD 0 1	AQ6370C/ AQ6370D

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### ZOOM

Function	Control Command	Remarks
ZOOM CENTER WL ****.***nm	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:CENTer<wsp><NRf>[M]	
ZOOM CENTER FREQ ***.***THz	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:CENTer<wsp><NRf>[HZ]	
ZOOM CENTER WNUM ****.***cm-1	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:CENTer<wsp><NRf>	AQ6375
ZOOM SPAN ****.*nm	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:SPAN<wp><NRf>[M]	
ZOOM SPAN ***.*THz	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:SPAN<wp><NRf>[HZ]	
ZOOM SPAN WNUM ****.*cm-1	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:SPAN<wp><NRf>	AQ6375
ZOOM START WL ****.***nm	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:START<wp><NRf>[M]	
ZOOM START FREQ ***.***THz	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:START<wp><NRf>[HZ]	
ZOOM START WNUM ****.***cm-1	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:START<wp><NRf>	AQ6375
ZOOM STOP WL ****.***nm	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:STOP<wp><NRf>[M]	
ZOOM STOP FREQ ***.***THz	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:STOP<wp><NRf>[HZ]	
ZOOM STOP WNUM ****.***cm-1	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:STOP<wp><NRf>	AQ6375
PEAK→ZOOM CTR	:CALCulate:MARKer:MAXimum:SZCEnter	
OVERVIEW DISPLAY OFF/ L/R	:DISPlay[:WINDOW]:OVIew:POSITION<wp>OFF LEFT RIGHT 0 1 2	
OVERVIEW SIZE	:DISPlay[:WINDOW]:OVIew:SIZE<wp>	
LARGE/SMALL	LARGE SMALL 0 1	
INITIAL	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:INITialize	

### DISPLAY

Function	Control Command	Remarks
NORMAL DISPLAY	:DISPlay[:WINDOW]:SPLIT<wp>OFF 0	
SPLIT DISPLAY	:DISPlay[:WINDOW]:SPLIT<wp>ON 1	
SPLIT DISPLAY		
TRACE A UP/LOW	:DISPlay[:WINDOW]:SPLIT:POSITION<wp>TRA,UP LOW 0 1	
TRACE B UP/LOW	:DISPlay[:WINDOW]:SPLIT:POSITION<wp>TRB,UP LOW 0 1	
TRACE C UP/LOW	:DISPlay[:WINDOW]:SPLIT:POSITION<wp>TRC,UP LOW 0 1	
TRACE D UP/LOW	:DISPlay[:WINDOW]:SPLIT:POSITION<wp>TRD,UP LOW 0 1	
TRACE E UP/LOW	:DISPlay[:WINDOW]:SPLIT:POSITION<wp>TRE,UP LOW 0 1	
TRACE F UP/LOW	:DISPlay[:WINDOW]:SPLIT:POSITION<wp>TRF,UP LOW 0 1	
TRACE G UP/LOW	:DISPlay[:WINDOW]:SPLIT:POSITION<wp>TRG,UP LOW 0 1	
HOLD		
UPPER HOLD ON/ OFF	:DISPlay[:WINDOW]:SPLIT:HOLD:UPPer<wp>OFF ON 0 1	
LOWER HOLD ON/ OFF	:DISPlay[:WINDOW]:SPLIT:HOLD:LOWer<wp>OFF ON 0 1	
LABEL	:DISPlay[:WINDOW]:TEXT:DATA<wp><string>	
NOISE MASK ***dB	:DISPlay[:WINDOW]:TRACe:Y:NMASK<wp><NRf>[DB]	
MASK LINE VERT/HRZN	:DISPlay[:WINDOW]:TRACe:Y:NMASK:TYPE<wp>VERTical HORIZONTAL 0 1	
TRACE CLEAR		
ALL TRACE	:DISPlay[:WINDOW]:TEXT:CLEar	
DISPLAY OFF	:DISPlay[:WINDOW]<wp>OFF ON 0 1	AQ6370C/ AQ6370D/ AQ6373B

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### TRACE

Function	Control Command	Remarks
ACTIVE TRACE		
A	:TRACe:ACTIve<wsp>TRA	
B	:TRACe:ACTIve<wsp>TRB	
C	:TRACe:ACTIve<wsp>TRC	
D	:TRACe:ACTIve<wsp>TRD	
E	:TRACe:ACTIve<wsp>TRE	
F	:TRACe:ACTIve<wsp>TRF	
G	:TRACe:ACTIve<wsp>TRG	
VIEW @ DISP/BLANK	:TRACe:STATE:<:TRACe name><wsp> ON OFF 1 0	
WRITE @	:TRACe:ATTRibute:<:TRACe name><wsp> WRITE 0	
FIX @	:TRACe:ATTRibute:<tarce name><wsp> FIX 1	
HOLD @		
MAX HOLD	:TRACe:ATTRibute:<:TRACe name><wsp> MAX 2	
MIN HOLD	:TRACe:ATTRibute:<:TRACe name><wsp> MIN 3	
ROLL AVG @ ***	:TRACe:ATTRibute:RAVG:<:TRACe name> <wsp><integer>	
CALCULATE C@@@@@		
LOG MATH@@@@@		
C = A-B(LOG)	:CALCulate:MATH:TRC<wsp>A-B (LOG)	
C = B-A(LOG)	:CALCulate:MATH:TRC<wsp>B-A (LOG)	
C = A+B(LOG)	:CALCulate:MATH:TRC<wsp>A+B (LOG)	
LIN MATH@@@@@		
C = A+B(LIN)	:CALCulate:MATH:TRC<wsp>A+B (LIN)	
C = A-B(LIN)	:CALCulate:MATH:TRC<wsp>A-B (LIN)	
C = B-A(LIN)	:CALCulate:MATH:TRC<wsp>B-A (LIN)	
C = 1-k(A/B) k: *.*.*.*	:CALCulate:MATH:TRC:K<wsp><NRF>; :CALCulate:MATH:TRC<wsp>1-K (A/B)	
C = 1-k(B/A) k: *.*.*.*	:CALCulate:MATH:TRC:K<wsp><NRF>; :CALCulate:MATH:TRC<wsp>1-K (B/A)	
CALCULATE F@@@@@		
LOG MATH@@@@@		
F = C-D(LOG)	:CALCulate:MATH:TRF<wsp>C-D (LOG)	
F = D-C(LOG)	:CALCulate:MATH:TRF<wsp>D-C (LOG)	
F = C+D(LOG)	:CALCulate:MATH:TRF<wsp>C+D (LOG)	
F = D-E(LOG)	:CALCulate:MATH:TRF<wsp>D-E (LOG)	
F = E-D(LOG)	:CALCulate:MATH:TRF<wsp>E-D (LOG)	
F = D+E(LOG)	:CALCulate:MATH:TRF<wsp>D+E (LOG)	
CALCulate F@@@@@		
LIN MATH@@@@@		
F = C+D(LIN)	:CALCulate:MATH:TRF<wsp>C+D (LIN)	
F = C-D(LIN)	:CALCulate:MATH:TRF<wsp>C-D (LIN)	
F = D-C(LIN)	:CALCulate:MATH:TRF<wsp>D-C (LIN)	
F = D+E(LIN)	:CALCulate:MATH:TRF<wsp>D+E (LIN)	
F = D-E(LIN)	:CALCulate:MATH:TRF<wsp>D-E (LIN)	
F = E-D(LIN)	:CALCulate:MATH:TRF<wsp>E-D (LIN)	
POWER/NBW@@@@@@@		
F=PWR/NBW A	:CALCulate:MATH:TRF<wsp>PWRNBWA	AQ6370D
F=PWR/NBW B	:CALCulate:MATH:TRF<wsp>PWRNBWB	AQ6370D
F=PWR/NBW C	:CALCulate:MATH:TRF<wsp>PWRNBWC	AQ6370D
F=PWR/NBW D	:CALCulate:MATH:TRF<wsp>PWRNBWD	AQ6370D
F=PWR/NBW E	:CALCulate:MATH:TRF<wsp>PWRNBWE	AQ6370D
BANDWIDTH	:CALCulate:MATH:TRF:PNBW:BWIDth BAND	AQ6370D

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

Function	Control Command
CALCulate G@{@@@@	
LOG MATH@{@@@@	
G = C-F(LOG)	:CALCulate:MATH:TRG<wsp>C-F (LOG)
G = F-C(LOG)	:CALCulate:MATH:TRG<wsp>F-C (LOG)
G = C+F(LOG)	:CALCulate:MATH:TRG<wsp>C+F (LOG)
G = E-F(LOG)	:CALCulate:MATH:TRG<wsp>E-F (LOG)
G = F-E(LOG)	:CALCulate:MATH:TRG<wsp>F-E (LOG)
G = E+F(LOG)	:CALCulate:MATH:TRG<wsp>E+F (LOG)
LIN MATH@{@@@@	
G = C+F(LIN)	:CALCulate:MATH:TRG<wsp>C+F (LIN)
G = C-F(LIN)	:CALCulate:MATH:TRG<wsp>C-F (LIN)
G = F-C(LIN)	:CALCulate:MATH:TRG<wsp>F-C (LIN)
G = E+F(LIN)	:CALCulate:MATH:TRG<wsp>E+F (LIN)
G = E-F(LIN)	:CALCulate:MATH:TRG<wsp>E-F (LIN)
G = F-E(LIN)	:CALCulate:MATH:TRG<wsp>F-E (LIN)
NORMALIZE@{@@@@	
G = NORM A	:CALCulate:MATH:TRG<wsp>NORMA
G = NORM B	:CALCulate:MATH:TRG<wsp>NORMB
G = NORM C	:CALCulate:MATH:TRG<wsp>NORMC
CURVE FIT@{@@@@	
G = CVFIT A	:CALCulate:MATH:TRG<wsp>CVFTA
G = CVFIT B	:CALCulate:MATH:TRG<wsp>CVFTB
G = CVFIT C	:CALCulate:MATH:TRG<wsp>CVFTC
G = MKR FIT	:CALCulate:MATH:TRG<wsp>MKRFT
THRESH **dB	:CALCulate:MATH:TRG:CVFT:THResh<wsp><NRf> [DB]
OPERATION AREA	:CALCulate:MATH:TRG:CVFT:OPARea<wsp>ALL INL1-L2 OUTL1-L2 0 1 2
FITTING ALGO	:CALCulate:MATH:TRG:CVFT:FALGo<wsp>GAUSS LORENz 3RD 4TH 5TH 0 1 2 3 4
CURVE FIT PK@{@@@@	
G = PKCVFIT A	:CALCulate:MATH:TRG<wsp>PKCVFTA
G = PKCVFIT B	:CALCulate:MATH:TRG<wsp>PKCVFTB
G = PKCVFIT C	:CALCulate:MATH:TRG<wsp>PKCVFTC
THRESH **dB	:CALCulate:MATH:TRG:PCVFT:THResh<wsp><NRf> [DB]
OPERATION AREA	:CALCulate:MATH:TRG:CVFT:OPARea<wsp>ALL INL1-L2 OUTL1-L2 0 1 2
FITTING ALGO	:CALCulate:MATH:TRG:CVFT:FALGo<wsp>GAUSS LORENz 3RD 4TH 5TH 0 1 2 3 4
TRACE LIST	-
TRACE COPY	:TRACe:COPY<wsp><source:TRACe name>,<destination:TRACe name>
TRACE CLEAR	:TRACe:DELeTe<wsp><:TRACe name>

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### MARKER

Function	Control Command	Remarks
MKR ACTIVE ON/OFF , SET MARKER	:CALCulate:MARKer[:STATE]<wsp><marker>, ON 1 :CALCulate:MARKer:X<wsp><marker>,<NRf>[M HZ]	
CLEAR MARKER	:CALCulate:MARKer[:STATE]<wsp><marker>,OFF 0	
MARKER→CENTER	:CALCulate:MARKer:SCENter	
MARKER →ZOOM CTR	:CALCulate:MARKer:SZCenter	
MARKER →REF LEVEL	:CALCulate:MARKer:SRLevel	
ADVANCED MARKER		
MARKER 1 SELECT @@@@@@@	:CALCulate:AMARKer[1]:X<wsp><NRf>[M AQ6370C/AQ6370D  Hz]	
MARKER TRACE		
A	:CALCulate:AMARKer[1]:TRACe<wsp>TRA	AQ6370C/AQ6370D
B	:CALCulate:AMARKer[1]:TRACe<wsp>TRB	AQ6370C/AQ6370D
C	:CALCulate:AMARKer[1]:TRACe<wsp>TRC	AQ6370C/AQ6370D
D	:CALCulate:AMARKer[1]:TRACe<wsp>TRD	AQ6370C/AQ6370D
E	:CALCulate:AMARKer[1]:TRACe<wsp>TRF	AQ6370C/AQ6370D
G	:CALCulate:AMARKer[1]:TRACe<wsp>TRG	AQ6370C/AQ6370D
OFF	:CALCulate:AMARKer[1] [:STATE]<wsp>OFF 0	AQ6370C/AQ6370D
NORMAL	:CALCulate:AMARKer[1]:FUNCTION:PRESet	AQ6370C/AQ6370D
POWER DENSITY	:CALCulate:AMARKer[1]:FUNCTION:PDEN sity :NOISE[:STATE]<wsp>ON 1	AQ6370C/AQ6370D
INTEGRAL POWER	:CALCulate:AMARKer[1]:FUNCTION:INTe gral[:STATE]<wsp>ON 1	AQ6370C/AQ6370D
INTEGRAL RANGE ***.*GHz	:CALCulate:AMARKer[1]:FUNCTION:INTe gral:IRAnge<wsp><integer>[Hz]	AQ6370C/AQ6370D
MARKER 2 SELECT @@@@@@@	:CALCulate:AMARKer2:X<wsp><NRf>[M  Hz]	AQ6370C/AQ6370D
MARKER TRACE		
A	:CALCulate:AMARKer2:TRACe<wsp>TRA	AQ6370C/AQ6370D
B	:CALCulate:AMARKer2:TRACe<wsp>TRB	AQ6370C/AQ6370D
C	:CALCulate:AMARKer2:TRACe<wsp>TRC	AQ6370C/AQ6370D
D	:CALCulate:AMARKer2:TRACe<wsp>TRD	AQ6370C/AQ6370D
E	:CALCulate:AMARKer2:TRACe<wsp>TRF	AQ6370C/AQ6370D
G	:CALCulate:AMARKer2:TRACe<wsp>TRG	AQ6370C/AQ6370D
OFF	:CALCulate:AMARKer2[:STATE]<wsp>O FF 0	AQ6370C/AQ6370D
NORMAL	:CALCulate:AMARKer2:FUNCTION:PRESet	AQ6370C/AQ6370D
POWER DENSITY	:CALCulate:AMARKer2:FUNCTION:PDENSi ty :NOISE[:STATE]<wsp>ON 1	AQ6370C/AQ6370D
INTEGRAL POWER	:CALCulate:AMARKer2:FUNCTION:INTegr al[:STATE]<wsp>ON 1	AQ6370C/AQ6370D
INTEGRAL RANGE ***.*GHz	:CALCulate:AMARKer2:FUNCTION:INTegr al:IRAnge<wsp><integer>[Hz]	AQ6370C/AQ6370D/AQ6373B
MARKER 3 SELECT @@@@@@@	:CALCulate:AMARKer3:X<wsp><NRf>[M  Hz]	AQ6370C/AQ6370D/AQ6373B

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

Function	Control Command	Remarks
MARKER TRACE		
A	:CALCulate:AMARKer3:TRACe<wsp>TRA	AQ6370C/ AQ6370D/AQ6373B
B	:CALCulate:AMARKer3:TRACe<wsp>TRB	AQ6370C/ AQ6370D/AQ6373B
C	:CALCulate:AMARKer3:TRACe<wsp>TRC	AQ6370C/ AQ6370D/AQ6373B
D	:CALCulate:AMARKer3:TRACe<wsp>TRD	AQ6370C/ AQ6370D/AQ6373B
E	:CALCulate:AMARKer3:TRACe<wsp>TRF	AQ6370C/ AQ6370D/AQ6373B
G	:CALCulate:AMARKer3:TRACe<wsp>TRG	AQ6370C/ AQ6370D/AQ6373B
OFF	:CALCulate:AMARKer3[:STATe]<wsp>O FF 0	AQ6370C/ AQ6370D/AQ6373B
NORMAL	:CALCulate:AMARKer3:FUNCTION:PRESet	AQ6370C/ AQ6370D/AQ6373B
POWER DENSITY	:CALCulate:AMARKer3:FUNCTION:PDENsi ty :NOISE[:STATe]<wsp>ON 1	AQ6370C/ AQ6370D/AQ6373B
INTEGRAL POWER	:CALCulate:AMARKer3:FUNCTION:INTegr al[:STATe]<wsp>ON 1	AQ6370C/ AQ6370D/AQ6373B
INTEGRAL RANGE ***.*GHz	:CALCulate:AMARKer3:FUNCTION:INTegr al:IRAnge<wsp><integer>[Hz]	AQ6370C/ AQ6370D/AQ6373B
MARKER 4 SELECT @@@@	:CALCulate:AMARKer4:X<wsp><NRF>[M] Hz]	AQ6370C/ AQ6370D/AQ6373B
MARKER TRACE		
A	:CALCulate:AMARKer4:TRACe<wsp>TRA	AQ6370C/ AQ6370D/AQ6373B
B	:CALCulate:AMARKer4:TRACe<wsp>TRB	AQ6370C/ AQ6370D/AQ6373B
C	:CALCulate:AMARKer4:TRACe<wsp>TRC	AQ6370C/ AQ6370D/AQ6373B
D	:CALCulate:AMARKer4:TRACe<wsp>TRD	AQ6370C/ AQ6370D/AQ6373B
E	:CALCulate:AMARKer4:TRACe<wsp>TRF	AQ6370C/ AQ6370D/AQ6373B
G	:CALCulate:AMARKer4:TRACe<wsp>TRG	AQ6370C/ AQ6370D/AQ6373B
OFF	:CALCulate:AMARKer4[:STATe]<wsp>O FF 0	AQ6370C/ AQ6370D/AQ6373B
NORMAL	:CALCulate:AMARKer4:FUNCTION:PRESet	AQ6370C/ AQ6370D/AQ6373B
POWER DENSITY	:CALCulate:AMARKer4:FUNCTION:PDENsi ty :NOISE[:STATe]<wsp>ON 1	AQ6370C/ AQ6370D/AQ6373B
INTEGRAL POWER	:CALCulate:AMARKer4:FUNCTION:INTegr al[:STATe]<wsp>ON 1	AQ6370C/ AQ6370D/AQ6373B
INTEGRAL RANGE ***.*GHz	:CALCulate:AMARKer4:FUNCTION:INTegr al:IRAnge<wsp><integer>[Hz]	AQ6370C/ AQ6370D/AQ6373B
SEARCH		
PEAK SEARCH	:CALCulate:AMARKer[1 2 3 4]:MAXimum	AQ6370C/ AQ6370D/AQ6373B
BOTTOM SEARCH	:CALCulate:AMARKer[1 2 3 4]:MINimum	AQ6370C/ AQ6370D/AQ6373B
NEXT LEVEL SEARCH	:CALCulate:AMARKer[1 2 3 4]:MAXimum :NEXT :CALCulate:AMARKer[1 2 3 4]:MINimum :NEXT	AQ6370C/ AQ6370D/AQ6373B
NEXT SEARCH RIGHT	:CALCulate:AMARKer[1 2 3 4]:MAXimum :RIGHT :CALCulate:AMARKer[1 2 3 4]:MINimum :RIGHT	AQ6370C/ AQ6370D/AQ6373B

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

Function	Control Command	Remarks
NEXT SEARCH LEFT	:CALCulate:AMARKer[1 2 3 4]:MAXimum :LEFT :CALCulate:AMARKer[1 2 3 4]:MINimum :LEFT	AQ6370C/ AQ6370D/AQ6373B
BANDWIDTH **.*nm	:CALCulate:AMARKer[1 2 3 4]:FUNCTio n:PDENsity :NOiSe:BWIDth :BANDwidth <wsp><NRf> [M]	AQ6370C/ AQ6370D/AQ6373B
ALL CLEAR	:CALCulate:AMARKer[1 2 3 4]:AOFF	AQ6370C/ AQ6370D/AQ6373B
ALL MARKER CLEAR	:CALCulate:MARKer:AOFF	
LINE MKR 1 ON/OFF	:CALCulate:LMARKer:X<wsp>1,<NRf> [M]	
LINE MKR 2 ON/OFF	:CALCulate:LMARKer:X<wsp>2,<NRf> [M]	
LINE MKR 3 ON/OFF	:CALCulate:LMARKer:Y<wsp>3,<NRf> [DBM]	
LINE MKR 4 ON/OFF	:CALCulate:LMARKer:Y<wsp>4,<NRf> [DBM]	
MKR L1-L2→SPAN	:CALCulate:LMARKer:SSPAn	
MKR L1-L2→ZOOM SPAN	:CALCulate:LMARKer:SZSPAn	
LINE MARKER ALL CLEAR	:CALCulate:LMARKer:AOFF	
MARKER DISPLAY		
OFFSET	:CALCulate:MARKer:FUNCTION:FORMAT <wsp>OFFSet 0	
SPACING	:CALCulate:MARKer:FUNCTION:FORMAT <wsp>SPACing 1	
MARKER AUTO UPDATE ON/OFF	:CALCulate:MARKer:FUNCTION:UPDateQ <wsp> OFF ON 0 1	
MARKER UNIT nm THz	:CALCulate:MARKer:UNIT<wsp> WAvelength  FREQuency 0 1	AQ6370C/ AQ6370D/AQ6373B
MARKER UNIT @@@@		AQ6375
nm	:CALCulate:MARKer:UNIT<wsp> WAvelength 0	AQ6375
THz	:CALCulate:MARKer:UNIT<wsp> FREQuency 1	AQ6375
cm-1	:CALCulate:MARKer:UNIT<wsp> WNUMber 2	AQ6375
SEARCH/ANA L1-L2 ON/OFF	:CALCulate:LMARKer:SRAnge<wsp>OFF  ON 0 1	
SEARCH/ANA ZOOM AREA ON/OFF	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:Q SRAnge<wsp> OFF ON 0 1	
MARKER LIST PRINT	:HCOPY[:IMMEDIATE]:FUNCTION:MARKer: LIST	AQ6370C/AQ6373/ AQ6375

## PEAK SEARCH

Function	Control Command	Remarks
PEAK SEARCH	:CALCulate:MARKer:MAXimum	
BOTTOM SEARCH	:CALCulate:MARKer:MINimum	
NEXT LEVEL SEARCH	:CALCulate:MARKer:MAXimum:NEXT or :CALCulate:MARKer:MINimum:NEXT	
NEXT SEARCH RIGHT	:CALCulate:MARKer:MAXimum:RIGHT or :CALCulate:MARKer:MINimum:RIGHT	
NEXT SEARCH LEFT	:CALCulate:MARKer:MAXimum:LEFT or :CALCulate:MARKer:MINimum:LEFT	
SET MARKER	:CALCulate:MARKer[:STATE]<wsp><marker>, ON 1	
CLEAR MARKER	:CALCulate:MARKer[:STATE]<wsp><marker>,OFF 0	
ALL MARKER CLEAR	:CALCulate:MARKer:AOFF	
AUTO SEARCH ON/OFF	:CALCulate:MARKer:AUTO<wsp>OFF ON 0 1	
MODE DIFF **.*dB	:CALCulate:PARAmeter:COMMON:MDIFF<w sp><NRf> [DB]	
SEARCH/ANA L1-L2 ON/OFF	:CALCulate:LMARKer:SRAnge<wsp>OFF  ON 0 1	
SEARCH/ANA ZOOM AREA ON/OFF	:DISPlay[:WINDOW]:TRACe:X[:SCALE]:S RANGE<wsp>OFF ON 0 1	
SEARCH MODE SINGL/MULTI	:CALCulate:MARKer:MSearch<wsp>OFF  ON 0 1	AQ6370C/ AQ6370D/AQ6373B

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

Function	Control Command	Remarks
THRESH **.*dB	:CALCulate:MARKer:MSearch:THresh<ws p><NRF>[DB]	AQ6370C/ AQ6370D/AQ6373B
SORT BY WL/LVL	:CALCulate:MARKer:MSearch:SORt<wsp>WAVelengtH LEVel 0 1	AQ6370C/ AQ6370D/AQ6373B

### ANALYSIS

Function	Control Command	Remarks
SPEC WIDTH@{@@}		
THRESH	:CALCulate:CATegory<wsp>SWTHresh 0	
ENVELOPE	:CALCulate:CATegory<wsp>SWEEnvelope 1	
RMS	:CALCulate:CATegory<wsp>SWRMs 2	
PEAK RMS	:CALCulate:CATegory<wsp>SWPKrms 3	
NOTCH	:CALCulate:CATegory<wsp>NOTCh 4	
ANALYSIS1@{@@}		
DFB-LD	:CALCulate:CATegory<wsp>DFBLd 5	
FP-LD	:CALCulate:CATegory<wsp>FPLD 6	
LED	:CALCulate:CATegory<wsp>LED 7	
SMSR	:CALCulate:CATegory<wsp>SMSR 8	
POWER	:CALCulate:CATegory<wsp>POWer 9	
PMD	:CALCulate:CATegory<wsp>PMD 10	
ANALYSIS2@{@@}		
OSNR (WDM)	:CALCulate:CATegory<wsp>OSNR 11	AQ6373
WDM	:CALCulate:CATegory<wsp>WDM 11	AQ6370C/AQ6375
EDFA-NF	:CALCulate:CATegory<wsp>NF 12	
FILTER-PK	:CALCulate:CATegory<wsp>FILPk 13	
FILTER-BTM	:CALCulate:CATegory<wsp>FILBtm 14	
WDM FIL-PK	:CALCulate:CATegory<wsp>WFPeak 15	AQ6370C/AQ6375
WDM FIL-BTM	:CALCulate:CATegory<wsp>WFbtm 16	AQ6370C/AQ6375
COLOR	:CALCulate:CATegory<wsp>COLOr 17	AQ6373/AQ6373B
ANALYSIS EXECUTE (@{@@})	:CALCulate[:IMMEDIATE]	
SPEC WIDTH THRESH **.*dB	:CALCulate:PARameter[:CATegory]:SWT Hresh:TH<wsp><NRF>[DB]	
SWITCH DISPLAY		AQ6370C/ AQ6370D/AQ6373B
TRACE&TABLE	:CALCulate:DISPlay<wsp>0	AQ6370C/ AQ6370D/AQ6373B
TABLE	:CALCulate:DISPlay<wsp>1	AQ6370C/ AQ6370D/AQ6373B
TRACE	:CALCulate:DISPlay<wsp>2	AQ6370C/ AQ6370D/AQ6373B
GRAPH&TABLE	:CALCulate:DISPlay<wsp>3	AQ6370C/ AQ6370D/AQ6373B
GRAPH	:CALCulate:DISPlay<wsp>4	AQ6370C/ AQ6370D/AQ6373B
LINE MARKER Y1/Y2	:CALCulate:DISPlay:GRAph:LMARKer:Y<wsp>1 2,<NRF>[DB]	AQ6370C/AQ6370D
AUTO ANALYSIS ON/ OFF	:CALCulate[:IMMEDIATE]:AUTO<wsp>OFF ON 0 1	
RESULT PRINT	:HCOPY[:IMMEDIATE]:FUNCTION: CALCulate:LIST	
RESULT SAVE	MMEMemory:STORE:ARESult<wsp><"file name">[, INTernal EXTernal]	
SEARCH/ANA L1-L2	:CALCulate:LMARKer:SRAnge<wsp>OFF ON 0 1ON/OFF	
SEARCH/ANA ZOOM AREA ON/OFF	:DISPlay[:WINDOW]:TRACe:X[:SCALE] :SRAnge<wsp>OFF ON 0 1	

#### Note

For the AQ6375, all soft keys included in ANALYSIS2 are disabled when the horizontal axis is wavenumber.

Analysis functions included in ANALYSIS2 cannot be executed. Also, these parameters cannot be set.

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### MEMORY

Function	Control Command
SAVE	
A TRACE →MEMORY	:MEMory:STORe<wsp><integer>,TRA
B TRACE →MEMORY	:MEMory:STORe<wsp><integer>,TRB
C TRACE →MEMORY	:MEMory:STORe<wsp><integer>,TRC
D TRACE →MEMORY	:MEMory:STORe<wsp><integer>,TRD
E TRACE →MEMORY	:MEMory:STORe<wsp><integer>,TRE
F TRACE →MEMORY	:MEMory:STORe<wsp><integer>,TRF
G TRACE →MEMORY	:MEMory:STORe<wsp><integer>,TRG
REC ALL	
MEMORY →A TRACE	:MEMory:LOAD<wsp><integer>,TRA
MEMORY →B TRACE	:MEMory:LOAD<wsp><integer>,TRB
MEMORY →C TRACE	:MEMory:LOAD<wsp><integer>,TRC
MEMORY →D TRACE	:MEMory:LOAD<wsp><integer>,TRD
MEMORY →E TRACE	:MEMory:LOAD<wsp><integer>,TRE
MEMORY →F TRACE	:MEMory:LOAD<wsp><integer>,TRF
MEMORY →G TRACE	:MEMory:LOAD<wsp><integer>,TRG
MEMORY CLEAR	:MEMory:CLEar<wsp><integer>

### FILE

Function	Control Command	Remarks
WRITE		
DRIVE INT/EXT	:MMEMemory:CDRive<wsp>INTernal EXTernal	
FILE NAME (TRACE)	:MMEMemory:CDIRectory<wsp><directory name>	
(ALL TRACE)	:MMEMemory:STORE:TRACe<wsp><trace name>, BIN CSV,<"file name">[, INTernal EXTernal]	
(MEMORY)	:MMEMemory:STORE:MEMory<wsp><integer>,BIN  CSV,<"file name">[, INTernal EXTernal]	
(GRAPHICS)	:MMEMemory:STORE:GRAphics<wsp>B&W COLOR, BMP TIFF,<"file name">[, INTernal EXTernal]	
(SETTING)	:MMEMemory:STORE:SETTING<wsp><"file name"> [, INTernal EXTernal]	
(DATA)	:MMEMemory:STORE:DATA<wsp><"file name"> [, INTernal EXTernal]	
OUTPUT ITEM SETTING		
DATE&TIME ON/OFF	:MMEMemory:STORE:DATA:TEM<wsp>DATE, OFF ON 0 1	
LABEL ON/OFF	:MMEMemory:STORE:DATA:ITEM<wsp>LABel,OFF  ON 0 1	
DATA AREA ON/OFF	:MMEMemory:STORE:DATA:TEM<wsp>DATA, OFF ON 0 1	
CONDITION ON/OFF	:MMEMemory:STORE:DATA:ITEM<wsp>CONDition ,OFF ON 0 1	
TRACE DATA ON/ OFF	:MMEMemory:STORE:DATA:ITEM<wsp>TRACe,OFF  ON 0 1	
FILE TYPE CSV/DT6	:MMEemory:STORE:DATA:TYPE<wsp>CSV  DT 0 1	
WRITE MODE ADD/ OVER (PROGRAM)	:MMEMemory:STORE:DATA:MODE<wsp> ADD OVER 0 1	
(TEMPLATE)	:MMEMemory:STORE:TEMPlate<wsp><template>	AQ6370C/
	<"file name">[, INTernal EXTernal]	AQ6370D/
(LOGGING)	:MMEMemory:STORE:DLOGging<wsp> <"file name">[, INTernal EXTernal]	AQ6370C/
		AQ6370D
<CSV DATA SAVE>	:MMEMemory:STORE:DLOGging:CSAVe<wsp>OFF  ON 0 1	AQ6370C/
		AQ6370D
<TRACE DATA SAVE>	:MMEMemory:STORE:DLOGging:TSAVe<wsp>OFF  ON 0 1	AQ6370C/
		AQ6370D

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

Function	Control Command	Remarks
READ		
DRIVE INT/EXT	:MMEMory:CDRive<wsp>INTernal EXTernal	
(TRACE)	:MMEMory:LOAD:TRACe<wsp><trace name>, <"file name">[, INTernal EXTernal]	
(ALL TRACE)	:MMEMory:LOAD:ATRacE<wsp><"file name">[, INTernal   EXTernal]	
(MEMORY)	:MMEMory:LOAD:MEMORY<wsp><integer>, <"file name">[, INTernal EXTernal]	
(SETTING)	:MMEMory:LOAD:SETTing<wsp><"file name"> [, INTernal EXTernal]	
(DATA)	:MMEMory:LOAD:DATA<wsp><"file name"> [, INTernal EXTernal]	
(PROGRAM)	:MMEMory:LOAD:PROGram<wsp><integer>, <"file name">[, INTernal EXTernal]	
(TEMPLATE)	:MMEMory:LOAD:PROGram<wsp><template> <"file name">[, INTernal EXTernal]	
(LOGGING)	:MMEMory:LOAD:DLOGging<wsp><"file name"> [, INTernal EXTernal]	AQ6370C/ AQ6370D/ AQ6373B
AUTO FILE NAME	:MMEMory:ANAMe<wsp>NUMBER DATE	AQ6370D
REMOVE USB STORAGE	:MMEMORY:REMove	
FILE OPERATION		
DRIVE INT/EXT	:MMEMory:CDRive<wsp>INTernal EXTernal	
DELETE	:MMEMory:DELeTe<wsp><"file name">[, INTernal EXTernal]	
COPY	:MMEMory:COPy<wsp><"source file name">, [INTernal EXTernal],<"destination file name"> [, INTernal EXTernal]	
RENAME	:MMEMory:REName<wsp><"new file name">, <"old file name">[, INTernal EXTernal]	
MAKE DIRECTORY	:MMEMory:MDIRectory<wsp><"directory name">[, INTernal EXTernal]	

## PROGRAM

Function	Control Command
PROGRAM EXECUTE	:PROGram:EXECute<wsp><integer>

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### SYSTEM

Function	Control Command	Remarks
OPTICAL ALIGNMENT	:CALibration:ALIGN[:IMMediate]	
BUILT-IN SOURCE	:CALibration:INTernal[:IMMedia te]	AQ6370D-L0 (Without Light source)
EXTERNAL LASER	:CALibration:EXTernal[:IMMedia te]	AQ6370D-L0 (Without Light source)
WL CALIBRATION		
BUILT-IN SOURCE	:CALibration:WAVelength:INTernal[:IMMediate]	AQ6370C/AQ6375
EXTERNAL LASER	:CALibration:WAVelength:EXTernal ****.***nm :SOURce<wsp>LASer 0; :CALibration:WAVelength:EXTernal :WAVelength<wsp><NRf>[M]	
EXTERNAL GAS CELL	:CALibration:WAVelength:EXTernal ****.***nm :SOURce<wsp>GASCell 1; :CALibration:WAVelength :EXTernal: WAVelength<wsp><NRf>[M]	AQ6370C/AQ6375
EMISSION LINE	:CALibration:WAVelength:SOURce ****.***nm :<wsp>EMIssion 2; :CALibration:WAVelength:EXTernal :WAVelength<wsp><NRf>[M]	AQ6373B
WL SHIFT **.***nm	:SENSe:CORRection:WAVelength:SHI Ft<wsp><NRf>[M]	
LVL SHIFT ***.***dB	:SENSe:CORRection:LEVel:SHIFT <wsp><NRf>[DB]	
WL OFFSET TABLE	:CALibration:WAVelength:OFFSet:T ABle<wsp><integer>,<NRf>[DB]	
LVL OFFSET TABLE	:CALibration:POWer:OFFSet:TABLE <wsp><integer>,<NRf>[DB]	
GRID EDITOR		
200GHz SPACING	:SYSTem:GRID<wsp>200GHZ 4	AQ6370C/AQ6375
100GHz SPACING	:SYSTem:GRID<wsp>100GHZ 3	AQ6370C/AQ6375
50GHz SPACING	:SYSTem:GRID<wsp>50GHZ 2	AQ6370C/AQ6375
25GHz SPACING	:SYSTem:GRID<wsp>25GHZ 1	AQ6370C/AQ6375
12.5GHz SPACING	:SYSTem:GRID<wsp>12.5GHZ 0	AQ6370C/AQ6375
CUSTOM	:SYSTem:GRID<wsp>CUSTom 5	AQ6370C/AQ6375
START WL ****.****nm	:SYSTem:GRID:CUSTOM:START<wsp><NRf>[M HZ]	AQ6370C/AQ6375
STOP WL ****.****nm	:SYSTem:GRID:CUSTOM:STOP<wsp><NRf>[M HZ]	AQ6370C/AQ6375
SPACING ***.*GHz	:SYSTem:GRID:CUSTOM:SPACing <wsp> <NRf>[GHZ]	AQ6370C/AQ6375
VALUE EDIT	-	
INSERT	:SYSTem:GRID:CUSTOM:INSert<wsp><NRf>[M HZ]	AQ6370C/AQ6375
DELETE	:SYSTem:GRID:CUSTOM:DElete<wsp><integer>	AQ6370C/AQ6375
REFERENCE	:SYSTem:GRID:REFerence<wsp><NRf>	AQ6370C/AQ6375
WAVELENGTH ****.****nm [HZ]	-	
USER KEY DEFINE	-	

### Note

On the AQ6375, the GRID EDITOR soft key is not available when in Frequency mode.

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

Function	Control Command	Remarks
GP-IB2 PORT ADDRESS **	:SYSTem:COMMUnicatE:GP-IB2:ADDReSS <wsp><integer>	
COMMAND FORMAT	:SYSTem:COMMUnicatE:CFORmat<wsp> AQ6317 AQ6370C 0 1 :SYSTem:COMMUnicatE:CFORmat<wsp> AQ6317 AQ6373 0 1 :SYSTem:COMMUnicatE:CFORmat<wsp> AQ6317 AQ6375 0 1 :SYSTem:COMMUnicatE:CFORmat<wsp> AQ6317 AQ6373B 0 1	AQ6370C AQ6373 AQ6375 AQ6373B
TLS ADDRESS **	:SYSTem:COMMUnicatE:GP-IB2:TLS: ADDReSS<wsp><integer>	AQ6370C/AQ6375
MONITOR PORT ON/OFF	:SYSTem:COMMUnicatE:RMONitor<wsp> OFF ON 0 1	AQ6370C/ AQ6370D/AQ6373B
HARD COPY DEVICE		AQ6370C/ AQ6373/AQ6375
INTERNAL	:HCOPY:DESTination<wsp>INTernal 0	
EXTERNAL	:HCOPY:DESTination<wsp>EXTernal 1	
FILE	:HCOPY:DESTination<wsp>FILE 2	
TRIG INPUT MODE	:TRIGger[:SEQUence]:INPut<wsp> ETRigger STRigger SENable 0 1 2	"SENable" and "2" can be used on the AQ6370C.
TRIG OUTPUT MODE	:TRIGger[:SEQUence]:OUTPut<wsp> OFF SStatus 0 1	
AUTO OFFSET ON/OFF	:CALibration:ZERO[:AUTO]<wsp>OFF ON 0  1 ONCE	AQ6370C/AQ6375
AUTO OFFSET SETTING		
AUTO OFFSET ON/ OFF	:CALibration:ZERO[:AUTO]<wsp>OFF  ON 0 1	AQ6373/AQ6373B
INTERVAL ***min	:CALibration:ZERO[:AUTO]:INTerval <wsp><integer>	AQ6373/AQ6373B
UNCAL WARN DISPLAY	:SYSTem:DISPlay:UNCal<wsp>OFF ON 0 1	
ON/OFF		
BUZZER SETTING		
CLICK ON/OFF	:SYSTem:BUZZer:CLICk<wsp>OFF ON 0 1	
WARNING ON/OFF	:SYSTem:BUZZer:WARNING<wsp>OFF ON 0 1	
LEVEL DISP		
1DIG	:UNIT:POWer:DIGIt<wsp>1	
2DIG	:UNIT:POWer:DIGIt<wsp>2	
3DIG	:UNIT:POWer:DIGIt<wsp>3	
WINDOW TRANSPARENT	:SYSTem:DISPlay:TRANsparent<wsp> ON/OFF OFF ON 0 1	
SET CLOCK	:SYSTem:DATE<wsp><year>,<month>,<day> :SYSTem:TIME<wsp><hour>,<minutes>, <seconds>	
SELECT COLOR		
COLOR 1	:DISPlay:COLOR<wsp>1	
COLOR 2	:DISPlay:COLOR<wsp>2	
COLOR 3	:DISPlay:COLOR<wsp>3	
COLOR 4	:DISPlay:COLOR<wsp>4	
COLOR 5	:DISPlay:COLOR<wsp>5	
B&W	:DISPlay:COLOR<wsp>0	
REMOVE USB STRAGE	:MMEMory:REMove	
SYSTEM INFORMATION		
SYSTEM INFO	:SYSTem:INFormation?<wsp>0 1	
RES BW CALIBRATION	:CALibration{[:BANDwidth BWIDth]}[:IMMEDIATE]	
EXECUTE	:CALibration{[:BANDwidth BWIDth]}[:IMMEDIATE]	
INITIALIZE	:CALibration{[:BANDwidth BWIDth]}[:IMMEDIATE]	
PARAMETER INITIALIZE		
ALL CLEAR	:SYSTem:PRESet	
VERSION	-	

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### ADVANCE

Function	Control Command	Remarks
<b>TEMPLATE</b>		
GO/NO GO ON/OFF	:TRACe:TEMPlate:GONogo<wsp>OFF ON 0 1	
<b>TEMPLATE DISPLAY</b>		
UPPER LINE	:TRACe:TEMPlate:DISPlay<wsp>UPPer,	
DISPLAY ON/OFF	OFF ON 0 1	
LOWER LINE	:TRACe:TEMPlate:DISPlay<wsp>LOWER,	
DISPLAY ON/OFF	OFF ON 0 1	
TARGET LINE	:TRACe:TEMPlate:DISPlay<wsp>TARGET	
DISPLAY ON/OFF	,OFF ON 0 1	
<b>TYPE</b>		
UPPER	:TRACe:TEMPlate:TTYPe<wsp>UPPer	
LOWER	:TRACe:TEMPlate:TTYPe<wsp>LOWER	
UPPER & LOWER	:TRACe:TEMPlate:TTYPe<wsp>U&L	
<b>TEMPLATE EDIT</b>		
ALL DELETE	:TRACe:TEMPlate:DATA:ADElete<wsp>UPPer LOWER TARGET	
MODE ABS/REL	:TRACe:TEMPlate:DATA:MODE<wsp>UPPer LOWER TARGET, ABSolute RELative	
<b>EXTRA POL TYPE</b>		
TYPE A	:TRACe:TEMPlate:DATA:ETYPe<wsp>UPPer LOWER TARGET,A 1	
TYPE B	:TRACe:TEMPlate:DATA:ETYPe<wsp>UPPer LOWER TARGET,B 2	
NONE	:TRACe:TEMPlate:DATA:ETYPe<wsp>UPPer LOWER TARGET,NONE 0	
<b>TEMPLATE SHIFT</b>		
TEST	:TRACe:TEMPlate:LEvel:SHIFT<wsp><NRF>	
WAVELENGTH	:TRACe:TEMPlate:WAveLength:SHIFT<wsp><NRF>	
<b>DATA LOGGING</b>		
START/STOP	:APPLication:DLOGging:STATE<wsp>STOP START 0 1	AQ6370C/AQ6370D/AQ6373B
<b>SETUP</b>		
LOGGING PARAMETER		AQ6370C/AQ6370D/AQ6373B
LOGGING ITEM	:APPLication:DLOGging:LParameter:I TEM<wsp>0 1 2 3	AQ6370C/AQ6370D/AQ6373B
LOGGING MODE	:APPLication:DLOGging:LParameter:L MODE<wsp>1 2	AQ6370C/AQ6370D/AQ6373B
MINIMUM INTERVAL	:APPLication:DLOGging:LParameter:I NTerval<wsp><integer>[SEC]	AQ6370C/AQ6370D/AQ6373B
TEST DURATION	:APPLication:DLOGging:LParameter:T DURation<wsp><integer>[sec]	AQ6370C/AQ6370D/AQ6373B
PEAK THRESH TYPE	:APPLication:DLOGging:LParameter:P DETect:TTYPe<wsp>ABSolute RELative	AQ6370C/AQ6370D/AQ6373B
THRESH(ABS)	:APPLication:DLOGging:LParameter:P DETect:ATHresh<NRF>[DBM]	AQ6370C/AQ6370D/AQ6373B
THRESH(REL)	:APPLication:DLOGging:LParameter:P DETect:RTHresh<NRF>[DB]	AQ6370C/AQ6370D/AQ6373B
CH MATCHING λ THRESH	:APPLication:DLOGging:LParameter:M THResh<wsp><NRF>[M]	AQ6370C/AQ6370D/AQ6373B
TRACE LOGGING	:APPLication:DLOGging:LParameter:T LOGging<wsp>OFF ON 0 1	AQ6370C/AQ6370D/AQ6373B
DESTINATION MEMORY	:APPLication:DLOGging:LParameter:M EMory<wsp>INTERNAL EXTERNAL	AQ6370C/AQ6370D/AQ6373B
LOGGING DATA SAVE	:MMEMory:STORE:DLOGging<wsp><"file name">[,INTERNAL EXTERNAL]	AQ6370C/AQ6370D/AQ6373B
LOGGING DATA LOAD	:MMEMory:LOAD:DLOGging<wsp><"file name">[,INTERNAL EXTERNAL]	AQ6370C/AQ6370D/AQ6373B

## 7.2 Table of Correspondence between Soft Keys and Remote Commands

### COPY

Function	Control Command
COPY	:HCOPY[:IMMEDIATE]

### FEED

Function	Control Command	Remarks
FEED	:HCOPY[:IMMEDIATE]:FEED	AQ6370C/AQ6373/AQ6375

## 7.3 ANALYSIS Setting Parameters

In setting ANALYSIS key setting parameters, the analysis parameters differ with the analysis type. Thus, the PARAMETER SETTING key commands are set independently of the regular key commands. An analysis parameter setting command is shown below.

### SPEC WIDTH

ANALYSIS Parameters	Control Command
THRESH	
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEgory]:SWTHresh:TH<wsp><NRf>[DB]
K **.*	:CALCulate:PARameter[:CATEgory]:SWTHresh:K<wsp><NRf>
MODE FIT ON/OFF	:CALCulate:PARameter[:CATEgory]:SWTHresh:MFIT<wsp>OFF ON 0 1
ENVELOPE	
THRESH LEVEL1**.*dB	:CALCulate:PARameter[:CATEgory]:SWENvelope:TH1<wsp><NRf>[DB]
THRESH LEVEL2 **.*dB	:CALCulate:PARameter[:CATEgory]:SWENvelope:TH2<wsp><NRf>[DB]
K **.*	:CALCulate:PARameter[:CATEgory]:SWENvelope:K
PEAK RMS	
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEgory]:SWPKrms:TH<wsp><NRf>[DB]
K **.*	:CALCulate:PARameter[:CATEgory]:SWPKrms:K<wsp><NRf>[DB]
NOTCH	
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEgory]:NOTCh:TH<wsp><NRf>[DB]
K **.*	:CALCulate:PARameter[:CATEgory]:NOTCh:K<wsp><NRf>[DB]
Type	
PEAK	:CALCulate:PARameter[:CATEgory]:NOTCh:TYPE<wsp>PEAK 0
BOTTOM	:CALCulate:PARameter[:CATEgory]:NOTCh:TYPE<wsp>BOTTOM 1

### ANALYSIS 1

ANALYSIS Parameters	Control Command
DFB-LD	
-XdB WIDTH	
ALGO	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, ALGO,<data>
THRESH **.*dB	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, TH,<NRf>[DB]
THRESH2 **.*dB	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, TH2,<NRf>[DB]
K	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, K,<NRf>
MODE FIT ON/OFF	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, MFIT, OFF ON 0 1
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, MDIFF,<NRf>[DB]
SWIDth	
ALGO	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, ALGO,<data>
THRESH **.*dB	:CALCulate:PARameter[:CATEgory]:DFBLd<wsp>SWIDth, TH,<NRf>[DB]

ANALYSIS Parameters	Control Command	Remarks
THRESH2 **.**dB	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>SWIDth, TH2, <NRF>[DB]	
K	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>SWIDth, K, <NRF>	
MODE FIT ON/ OFF	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>SWIDth, MFIT, OFF ON 0 1	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>SWIDth, MDIFF, <NRF>[DB]	
SMSR		
SMSR MODE	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>SMSR, SMode, SMSR1 SMSR2 SMSR3 SMSR4	"SMSR3" and "SMSR4" can be used on the AQ6370C/AQ6370D.
SMSR MASK ±*.**nm	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>SMSR, SMASK, <NRF>[M]	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>SMSR, MDIFF, <NRF>[DB]	
RMS		AQ6370C/AQ6370D/AQ6373B
ALGO	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>RMS, ALGO, <data>	AQ6370C/AQ6370D/AQ6373B
THRESH **.**dB	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>RMS, TH, <NRF>[DB]	AQ6370C/AQ6370D/AQ6373B
K	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>RMS, K, <NRF>	AQ6370C/AQ6370D/AQ6373B
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>RMS, MDIFF, <NRF>[DB]	AQ6370C/AQ6370D/AQ6373B
POWER		AQ6370C/AQ6370D/AQ6373B
SPAN **.**nm	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>POWER, SPAN, <NRF>[M]	AQ6370C/AQ6370D/AQ6373B
OSNR		AQ6370C/AQ6370D/AQ6373B
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, MDIFF, <NRF>[DB]	AQ6370C/AQ6370D/AQ6373B
NOISE ALGO	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, NALGo, <data>	AQ6370C/AQ6370D/AQ6373B
NOISE AREA **.**nm	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, NARea, <NRF>[M]	AQ6370C/AQ6370D/AQ6373B
MASK AREA *.*nm	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, MARea, <NRF>[M]	AQ6370C/AQ6370D/AQ6373B
FITTING ALGO	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, FALGo, <data>	AQ6370C/AQ6370D/AQ6373B
NOISE BW **.**nm	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, NBW, <NRF>[M]	AQ6370C/AQ6370D/AQ6373B
SIGNAL POWER	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, SPower, <data>	AQ6370C/AQ6370D/AQ6373B
INTEGRAL RANGE	:CALCulate:PARameter[:CATegory]:DFBLd <wsp>OSNR, IRAnge, <NRF>	AQ6370C/AQ6370D/AQ6373B
FP-LD		
SPECTRUM WIDTH		
ALGO	:CALCulate:PARameter[:CATegory]:FPLD <wsp>SWIDth, ALGO, <data>	
THRESH **.**dB	:CALCulate:PARameter[:CATegory]:FPLD <wsp>SWIDth, TH, <NRF>[DB]	
THRESH2 **.**dB	:CALCulate:PARameter[:CATegory]:FPLD <wsp>SWIDth, TH2, <NRF>[DB]	
K	:CALCulate:PARameter[:CATegory]:FPLD <wsp>SWIDth, K, <NRF>	
MODE FIT ON/ OFF	:CALCulate:PARameter[:CATegory]:FPLD <wsp>SWIDth, MFIT, OFF ON 0 1	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:FPLD <wsp>SWIDth, MDIFF, <NRF>[DB]	

### 7.3 ANALYSIS Setting Parameters

ANALYSIS Parameters	Control Command	Remarks
<b>MEAN WAVELENGTH</b>		
ALGO	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MWAVelength,ALGO,<data>	
THRESH **.*dB	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MWAVelength,TH,<NRF>[DB]	
THRESH2 **.*dB	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MWAVelength,TH2,<NRF>[DB]	
K	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MWAVelength,K,<NRF>	
MODE FIT ON/ OFF	:CALCulate:PARameter[:CATegory]:FPLD <wsp>MWAVelength,MFIT,OFF ON 0 1	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:FPLD <wsp>MWAVelength,MDIFF,<NRF>[DB]	
<b>TOTAL POWER</b>		
OFFSET LEVEL *.*dB	:CALCulate:PARameter[:CATegory]:FPLD <wsp>TPOWer,OFFSet,<NRF>[DB]	
<b>MODE NO.</b>		
ALGO	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MNUMber,ALGO,<data>	
THRESH **.*dB	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MNUMber,TH,<NRF>[DB]	
THRESH2 **.*dB	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MNUMber,TH2,<NRF>[DB]	
K	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MNUMber,K,<NRF>	
MODE FIT ON/ OFF	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MNUMber,MFIT,OFF ON 0 1	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:FP LD<wsp>MNUMber,MDIFF,<NRF>[DB]	
<b>LED</b>		
<b>SPECTRUM WIDTH</b>		
ALGO	:CALCulate:PARameter[:CATegory]:LE D<wsp>SWIDth,ALGO,<data>	
THRESH **.*dB	:CALCulate:PARameter[:CATegory]:LE D<wsp>SWIDth,TH,<NRF>[DB]	
THRESH2 **.*dB	:CALCulate:PARameter[:CATegory]:LE D<wsp>SWIDth,TH2,<NRF>[DB]	
K	:CALCulate:PARameter[:CATegory]:LE D<wsp>SWIDth,K,<NRF>	
MODE FIT ON/ OFF	:CALCulate:PARameter[:CATegory]:LE D<wsp>SWIDth,MFIT,OFF ON 0 1	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:LE D<wsp>SWIDth,MDIFF,<NRF>[DB]	
<b>MEAN WAVELENGTH</b>		
ALGO	:CALCulate:PARameter[:CATegory]:LE	
THRESH **.*dB	:CALCulate:PARameter[:CATegory]:LE D<wsp>MWAVelength,TH,<NRF>[DB]	
THRESH2 **.*dB	:CALCulate:PARameter[:CATegory]:LE D<wsp>MWAVelength,TH2,<NRF>[DB]	
K	:CALCulate:PARameter[:CATegory]:LE	
MODE FIT ON/ OFF	:CALCulate:PARameter[:CATegory]:LED <wsp>MWAVelength,MFIT,OFF ON 0 1	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATegory]:LED <wsp>MWAVelength,MDIFF,<NRF>[DB]	
<b>TOTAL POWER</b>		
OFFSET LEVEL *.*dB	:CALCulate:PARameter[:CATegory]:LED <wsp>TPOWer,OFFSet,<NRF>[DB]	
<b>SMSR</b>		
SMSR MODE	:CALCulate:PARameter[:CATegory]:SMSR:M "SMSR3" and ODE<wsp>SMSR1 SMSR2 SMSR3 SMSR4 "SMSR4" can be used on theAQ6370C.	
SMSR MASK ±.*dB	:CALCulate:PARameter[:CATegory]:SM SR:MASK<wsp><NRF>[M] POWER	
<b>POWER</b>		
OFFSET LEVEL *.*dB	:CALCulate:PARameter[:CATegory]:PO Wer:OFFSet<wsp><NRF>[DB]	
<b>PMD</b>		
THRESH LEVEL *.*dB	:CALCulate:PARameter[:CATegory]:PM D:TH<wsp><NRF>[DB]	

**ANALYSIS 2 (disabled when in Wavenumber mode)**

For the AQ6375, these parameters cannot be set when in Wavenumber mode.

<b>ANALYSIS Parameters</b>	<b>Control Command</b>
WDM (On the AQ6373/AQ6373B, the soft key appears as OSNR(WDM)).	
CHANNEL DETECTION SETTING	
THRESH LEVEL	:CALCulate:PARameter[:CATEgory]:WDM:TH<wsp><NRf>[DB]
MODE DIFF **.**dB	:CALCulate:PARameter[:CATEgory]:WDM:MDIFF<wsp><NRf>[DB]
DISPLAY MASK OFF/ON *.*dB	:CALCulate:PARameter[:CATEgory]:WDMASK<wsp><NRf>[DB]
INTERPOLATATION SETTING	
NOISE ALGO	
AUTO-FIX	:CALCulate:PARameter[:CATEgory]:WDM:NALGo<wsp>AFIX 0
MANUAL-FIX	:CALCulate:PARameter[:CATEgory]:WDM:NALGo<wsp>MFIX 1
AUTO-CTR	:CALCulate:PARameter[:CATEgory]:WDM:NALGo<wsp>ACENTer 2
MANUAL-CTR	:CALCulate:PARameter[:CATEgory]:WDM:NALGo<wsp>MCENTER 3
PIT	:CALCulate:PARameter[:CATEgory]:WDM:NALGo<wsp>PIT 4
FITTING AREA	:CALCulate:PARameter[:CATEgory]:WDM:NARea<wsp><NRf>[M]
MASK AREA	:CALCulate:PARameter[:CATEgory]:WDM:MARea<wsp><NRf>[M]
FITTING ALGO	
LINEAR	:CALCulate:PARameter[:CATEgory]:WDM:FALGo<wsp>LINEar 0
GAUSS	:CALCulate:PARameter[:CATEgory]:WDM:FALGo<wsp>GAUSS 1
LORENZ	:CALCulate:PARameter[:CATEgory]:WDM:FALGo<wsp>LOREnz 2
3RD POLY	:CALCulate:PARameter[:CATEgory]:WDM:FALGo<wsp>3RD 3
4TH POLY	:CALCulate:PARameter[:CATEgory]:WDM:FALGo<wsp>4TH 4
5TH POLY	:CALCulate:PARameter[:CATEgory]:WDM:FALGo<wsp>5TH 5
NOISE BW *.*nm	:CALCulate:PARameter[:CATEgory]:WDM:NBW<wsp><NRf>[M]
DUAL TRACE ON/OFF	:CALCulate:PARameter[:CATEgory]:WDM:DUAL<wsp>OFF ON 0 1
DISPLAY SETTING	
DISPLAY TYPE	
ABSOLUTE	:CALCulate:PARameter[:CATEgory]:WDM:DTPe<wsp>ABSolute 0
RELATIVE	:CALCulate:PARameter[:CATEgory]:WDM:DTPe<wsp>RELative 1 (On the AQ6373/AQ6373B, it cannot be set.)
DRIFT(MEAS)	:CALCulate:PARameter[:CATEgory]:WDM:DTPe<wsp>MDRift 2
DRIFT(GRID)	:CALCulate:PARameter[:CATEgory]:WDM:DTPe<wsp>GDRift 3 (On the AQ6373/AQ6373B, it cannot be set.)
CH RELATION	
OFFSET	:CALCulate:PARameter[:CATEgory]:WDM:RELation<wsp>OFFSet 0
SPACING	:CALCulate:PARameter[:CATEgory]:WDM:RELation<wsp>SPACing 1
REF CH	:CALCulate:PARameter[:CATEgory]:WDM:RCH<wsp><integer>
MAX/MIN RESET	:CALCulate:PARameter[:CATEgory]:WDM:MMReset
OUTPUT SLOPE ON/OFF	:CALCulate:PARameter[:CATEgory]:WDM:OSlope<wsp>OFF ON 0 1
POINT DISPLAY ON/OFF	:CALCulate:PARameter[:CATEgory]:WDM:PDISplay<wsp>OFF ON 0 1

### 7.3 ANALYSIS Setting Parameters

ANALYSIS Parameters	Control Command
OTHER SETTING (invalid if other than the AQ6370C/AQ6370D/AQ6373B.)	
SIGNAL POWER	:CALCulate:PARameter[:CATegory]:WDM:SPoWer<wsp> PEAK INtegral 0 1
INTEGRAL RANGE	:CALCulate:PARameter[:CATegory]:WDM:IRAnge<wsp> <NRf>
EDFA NF (It is not available on the AQ6373/AQ6373B.)	
CHANNEL DETECTION	
THRESH LEVEL **.**dB	:CALCulate:PARameter[:CATegory]:NF:TH<wsp><NRf> [DB]
MODE DIFF **.**dB	:CALCulate:PARameter[:CATegory]:NF:MDIFF<wsp> <NRf>[DB]
INTERPOLATION SETTING	
OFFSET(IN) **.**dB	:CALCulate:PARameter[:CATegory]:NF:IOFFset<wsp> <NRf>[DB]
OFFSET(OUT) **.**dB	:CALCulate:PARameter[:CATegory]:NF:OOffset<wsp> <NRf>[DB]
ASE ALGO	
AUTO-FIX	:CALCulate:PARameter[:CATegory]:NF:AALGo<wsp> AFIX 0
MANUAL-FIX	:CALCulate:PARameter[:CATegory]:NF:AALGo<wsp> MFix 1
AUTO-CTR	:CALCulate:PARameter[:CATegory]:NF:AALGo<wsp> ACenter 2
MANUAL-CTR	:CALCulate:PARameter[:CATegory]:NF:AALGo<wsp> MCenter 3
FITTING AREA	:CALCulate:PARameter[:CATegory]:NF:FARea<wsp> <NRf>[M]
MASK AREA	:CALCulate:PARameter[:CATegory]:NF:MARea<wsp> <NRf>[M]
FITTING ALGO	
LINEAR	:CALCulate:PARameter[:CATegory]:NF:FALGo<wsp> LInear 0
GAUSS	:CALCulate:PARameter[:CATegory]:NF:FALGo<wsp> GAUs 1
LORENZ	:CALCulate:PARameter[:CATegory]:NF:FALGo<wsp> LORenz 2
3RD POLY	:CALCulate:PARameter[:CATegory]:NF:FALGo<wsp>3RD 3
4TH POLY	:CALCulate:PARameter[:CATegory]:NF:FALGo<wsp>4TH 4
5TH POLY	:CALCulate:PARameter[:CATegory]:NF:FALGo<wsp>5TH 5
POINT DISPLAY ON/OFF	:CALCulate:PARameter[:CATegory]:NF:PDIStplay<wsp> >OFF ON 0 1
NF CALCULATION SETTING	
RES BW	:CALCulate:PARameter[:CATegory]:NF:RBWidth<wsp> MEASured CAL 0 1
SHOT NOISE	:CALCulate:PARameter[:CATegory]:NF:SNOise<wsp>0 FF ON 0 1
FILTER-PK	
SW ON/OFF	:CALCulate:PARameter[:CATegory]:FILPk<wsp> PLEvel,SW,OFF ON 0 1
PEAK WAVELENGTH	
SW ON/OFF	:CALCulate:PARameter[:CATegory]:FILPk<wsp> PWAVelength,SW,OFF ON 0 1
CENTER WAVELENGTH	
ALGO	:CALCulate:PARameter[:CATegory]:FILPk<wsp> MWAVelength,ALGO,<data>
THRESH LEVEL **.**dB	:CALCulate:PARameter[:CATegory]:FILPk<wsp> MWAVelength,TH,<NRf>[DB]
K	:CALCulate:PARameter[:CATegory]:FILPk<wsp> MWAVelength,K,<NRf>
MODE FIT ON/OFF	:CALCulate:PARameter[:CATegory]:FILPk<wsp> MWAVelength,MFIT,OFF ON 0 1

### 7.3 ANALYSIS Setting Parameters

ANALYSIS Parameters	Control Command
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>MWAVelength,MDIFF,<NRf>[DB]
<b>FILTER-PK</b>	
SPECTRUM WIDTH	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>SWIDth,SW,OFF ON 0 1
ALGO	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>SWIDth,ALGO,<data>
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>SWIDth,TH,<NRf>[DB]
K	:CALCulate:PARameter[:CATEGORY]: FILPk<wsp>SWIDth,K,<NRf>
MODE FIT ON/OFF	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>SWIDth,MFIT,OFF ON 0 1
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>SWIDth,MDIFF,<NRf>[DB]
<b>CROSS TALK</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,SW,OFF ON 0 1
ALGO	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,ALGO,<data>
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,TH,<NRf>[DB]
K	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,K,<NRf>
MODE FIT ON/OFF	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,MFIT,OFF ON 0 1
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,MDIFF,<NRf>[DB]
CH SPACE ±.*nm	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,CSPace,<NRf>[M]
SEARCH AREA ±.*nm	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>XTALK,SARea,<NRf>[M]
<b>RIPPLE WIDTH</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>RWIDth,SW,OFF ON 0 1
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp> RWIDth,TH,<NRf>[DB]
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEGORY]:FILPk<wsp>RWIDth,MDIFF,<NRf>[DB]

### 7.3 ANALYSIS Setting Parameters

ANALYSIS Parameters	Control Command
<b>FILTER BOTTOM</b>	
BOTTOM LEVEL	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>BLEVel,SW,OFF ON 0 1
<b>BOTTOM WAVELENGTH</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>BWAVelength,SW,OFF ON 0 1
<b>CENTER WAVELENGTH</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>CWAVelength,SW,OFF ON 0 1
ALGO	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>CWAVelength,ALGO,<data>
THRESH LEVEL**.*dB	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>CWAVelength,TH,<NRF>[DB]
<b>CENTER WAVELENGTH</b>	
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>CWAVelength,MDIFF,<NRF>[DB]
<b>NOTCH WIDTH</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>NWIDth,SW,OFF ON 0 1
ALGO	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>NWIDth,ALGO,<data>
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>NWIDth,TH,<NRF>[DB]
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEgory]: FILBtm <wsp>NWIDth,MDIFF,<NRF>[DB]
<b>CROSS TALK</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>XTALK,SW,OFF ON 0 1
ALGO	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>XTALK,ALGO,<data>
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>XTALK,TH,<NRF>[DB]
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>XTALK,MDIFF,<NRF>[DB]
CH SPACE ±*.*nm	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>XTALK,CSPace,<NRF>[M]
SEARCH AREA ±*.*nm	:CALCulate:PARameter[:CATEgory]:FILBtm <wsp>XTALK,SARea,<NRF>[M]
<b>WDM FIL-PK (It is not available on the AQ6373/AQ6373B.)</b>	
<b>CHANNEL DETECTION/ NOMINAL WAVELENGTH</b>	
ALGO	:CALCulate:PARameter[:CATEgory]:WFPeak <wsp>NWAVelength,ALGO,<data>
THRESH LEVEL **.*dB	:CALCulate:PARameter[:CATEgory]:WFPeak <wsp>NWAVelength,TH,<NRF>[DB]
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEgory]:WFPeak <wsp>NWAVelength,MDIFF,<NRF>[DB]
TEST BAND *.*nm	:CALCulate:PARameter[:CATEgory]:WFPeak <wsp>NWAVelength,TBAND<NRF>[DB]
<b>PEAK WAVELENGTH/LEVEL</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:WFPeak <wsp>PWAVelength,SW,OFF ON 0 1

ANALYSIS Parameters	Control Command
<b>WDM FIL-PK</b>	
XdB WIDTH/CENTER WAVELENGTH	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> CWAVelength, SW, OFF ON 0 1
THRESH LEVEL **.**dB	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> CWAVelength, TH, <NRf>[DB]
<b>XdB STOP BAND</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> SBAnd, SW, OFF ON 0 1
THRESH LEVEL**.**dB	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> SBAnd, TH, <NRf>[DB]
<b>XdB PASS BAND</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> PBAnd, SW, OFF ON 0 1
THRESH LEVEL	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> PBAnd, TH, <NRf>[DB]
TEST BAND *.*nm	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> PBAnd, TBAnd, <NRf>[DB]
<b>RIPPLE</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> RIPPle, SW, OFF ON 0 1
TEST BAND *.*nm	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> RIPPle, TBAnd, <NRf>[DB]
<b>CROSS TALK</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> XTALK, SW, OFF ON 0 1
SPACING *.*nm	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> XTALK, SPACing, <NRf>[M]
TEST BAND *.*nm	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> XTALK, TBAnd, <NRf>[DB]
<b>WDM FIL-BTM (It is not available on the AQ6373/AQ6373B.)</b>	
<b>CHANNEL DETECTION/ NOMINAL WAVELENGTH</b>	
ALGO	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> NWAVelength, ALGO, <data>
THRESH LEVEL**.**dB	:CALCulate:PARameter[:CATEGORY]:WFPeak<wsp> WFBottom, TH, <NRf>[DB]
MODE DIFF *.*dB	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> NWAVelength, MDIFF, <NRf>[DB]
TEST BAND *.*nm	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> NWAVelength, TBAnd<NRf>[DB]
<b>BOTTM WAVELENGTH/LEVEL</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> BWAVelength, SW, OFF ON 0 1
<b>XdB NOTCH WIDTH/CENTER</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> CWAVelength, SW, OFF ON 0 1
<b>XdB STOP BAND</b>	
ALGO	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> SBAnd, ALGO, <data>
THRESH LEVEL **.**dB	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> SBAnd, TH, <NRf>[DB]
<b>XdB ELIMINATION BAND</b>	
SW ON/OFF	:CALCulate:PARameter[:CATEGORY]:WFBottom<wsp> EBAnd, SW, OFF ON 0 1

### 7.3 ANALYSIS Setting Parameters

ANALYSIS Parameters	Control Command
WDM FIL-BTM	
XdB ELIMINATION BAND	
THRESH LEVEL	:CALCulate:PARameter[:CATEgory]:WFBottom<wsp>
**.**dB	EBAND, TH, <NRf> [DB]
TEST BAND *.*nm	:CALCulate:PARameter[:CATEgory]:WFBottom<wsp>
	EBAND, TBAND, <NRf> [DB]
RIPPLE	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:WFBottom<wsp>
	RIPPLE, SW, OFF ON 0 1
TEST BAND *.*nm	:CALCulate:PARameter[:CATEgory]:WFBottom<wsp>
	RIPPLE, TBAND, <NRf> [DB]
CROSS TALK	
SW ON/OFF	:CALCulate:PARameter[:CATEgory]:WFBottom<wsp>
	XTALK, SW, OFF ON 0 1
SPACING *.*nm	:CALCulate:PARameter[:CATEgory]:WFBottom<wsp>
	XTALK, SPACing, <NRf> [M]
TEST BAND *.*nm	:CALCulate:PARameter[:CATEgory]:WFBottom<wsp>
	XTALK, TBAND, <NRf> [DB]

### Parameter Corresponding to <ANALYSIS PARAMETER> of the Data Logging Function

The parameter corresponding to <ANALYSIS PARAMETER> accessed through ADVANCE -> <DATA LOGGING> -> <SETUP> varies depending on the logging item.

- **When the Logging Item Is WDM**

The ANALYSIS2 parameter accessed through the ANALYSIS key in this section corresponds to <ANALYSIS PARAMETER>.

- **When the Logging Item Is DFB-LD**

The ANALYSIS1 parameter accessed through the ANALYSIS key in this section corresponds to <ANALYSIS PARAMETER>.

## 7.4 Remote Command Tree

Command	Parameter	Page
<b>COMMON command</b>		
*CLS	none	7-38
*ESE	<integer>	7-38
*ESE?	none	7-38
*ESR?	none	7-38
*IDN?	none	7-38
*OPC	none	7-38
*OPC?	none	7-38
*RST	none	7-39
*SRE	<integer>	7-39
*SRE?	none	7-39
*STB?	none	7-39
*TRG	none	7-39
*TST?	none	7-39
*WAI	none	7-39
<b>ABORt</b>	none	7-40
<b>APPLication</b>		
:DLOGging		
:ETIMe?	none	7-40
:LPARameter		
:INTerval	<integer>	7-40
:ITEM	0 1 2 3	7-41
:LMODe	1 2	7-41
:MEMORY	INTERNAL EXTERNAL	7-41
:MTHResh	<NRF>	7-41
:PDETect		
:ATHResh	<NRF>	7-42
:RTHResh	<NRF>	7-42
:TTYPE	ABSolute RELative	7-42
:TDURation	<integer>	7-42
:TLOGging	OFF ON 0 1	7-43
:STATE	STOP START 0 1	7-43
<b>CALCulate</b>		
:AMARKer[1 2 3 4]		7-43
:AOFF	none	7-43
:FUNCTION		
:INTEGRal		
:IRANGE	<NRF>[Hz]	7-44
:RESult?	none	7-44
[:STATE]	OFF ON 0 1	7-44
:PDENsity NOISE		
:BWIDTH BANDwidth	<NRF>[M]	7-45
:RESult?	none	7-45
[:STATE]	OFF ON 0 1	7-45
:PRESet	none	7-45
:MAXimum	none	7-46
:LEFT	none	7-46
:NEXT	none	7-46
:RIGHT	none	7-46
:MINimum	none	7-46
:LEFT	none	7-46
:NEXT	none	7-47
:RIGHT	none	7-47
[:STATE]	OFF ON 0 1	7-47
:TRACe	TRA TRB TRC TRD TRE TRF TRG	7-47
:X	<NRF>[M Hz]	7-47
:Y?	none	7-48
:ARESolution?	<Trace name>, [<start point>,<stop point>]	7-48
:CATegory	SWTHresh SWENvelope SWRMs SWPKrms  NOTCh DFBLd  FPLD LED SMSR POWer  PMD WDM NF FILPk FILBtm WFPeak  WFBtm OSNR COLor	7-48

## 7.4 Remote Command Tree

Command	Parameter	Page
:DATA?	none	7-49
:CGAin?	none	7-49
:CNF?	none	7-49
:CPowers?	none	7-49
:CSNR?	none	7-49
:CWAVelengths	none	7-50
:DFBLd?	none	7-50
:NCHannels	none	7-50
:OSLope?	none	
:DISPlay	0 1 2 3 4	7-50
:GRAPh:LMARKer:Y	1 2,<NRf>[DB]	7-50
[ :IMMediate]	none	7-51
:AUTO	OFF ON 0 1	7-51
:LMARKer		
:AOFF	none	7-51
:SRAnge	OFF ON 0 1	7-51
:SSPAn	none	7-51
:SZSPAn	none	7-51
:X	1 2,<NRf>[M HZ]	7-51
:Y	3 4,<NRf>[DBM/DB/%]	7-51
:MARKer		
:AOFF	none	7-51
:AUTO	OFF ON 0 1	7-52
:FUNCTION		
:FORMat	OFFSet SPACing 0 1	7-52
:UPDate	OFF ON 0 1	7-52
:MAXimum	none	7-52
:LEFT	none	7-52
:NEXT	none	7-52
:RIGHT	none	7-52
:SCENTER	none	7-52
:AUTO	OFF ON 0 1	7-52
:SRLevel	none	7-53
:AUTO	OFF ON 0 1	7-53
:SZCenter	none	7-53
:MINimum	none	7-53
:LEFT	none	7-53
:NEXT	none	7-53
:RIGHT	none	7-53
:MSearch	OFF ON 0 1	7-53
:SORT	WAVelength LEVel 0 1	7-53
:THResh	<NRf>[DB]	7-54
:SCEnter	none	7-54
:SRLevel	none	7-54
[:STATE]	<marker>,OFF ON 0 1	7-54
:SZCenter	none	7-54
:UNIT	WAVelength FREQuency WNUMBER	7-54
:X	<marker>,<NRf> [M HZ]	7-54
:Y?	<marker>	7-55
:MATH		
:TRC	A-B (LOG)  B-A (LOG)  A+B (LOG)  A+B (LIN)  A-B (LIN)  B-A (LIN)  1-K(A/B)  1-K(B/A)	7-55
:K	<NRf>	7-55
:TRF	C-D (LOG)  D-C (LOG)  C+D (LOG)  D-E (LOG)  E-D (LOG)  D-C (LIN)  D+E (LIN)  D-E (LIN)  E-D (LIN)  PWRNBWA   PWRNBWB   PWRNBWC   PWRNBWD   PWRNBWE	7-55
:PNBW:BWIDth	<NRf>[M]	7-55
:TRG	C-F (LOG)  F-C (LOG)  C+F (LOG)  E-F (LOG)  F-E (LOG)  E+F (LOG)  C+F (LIN)  C-F (LIN)  F-C (LIN)  E+F (LIN)  E-F (LIN)  F-E (LIN)  NORMA   NORMB   NORMC   CVFTA   CVFTB   CVFTC   MKRFT   PKCVFTA   PKCVFTB   PKCVFTC	7-56

## 7.4 Remote Command Tree

Command	Parameter	Page
:CVFT		
:FALGo	GAUSS LORENz 3RD 4TH 5TH 0 1 2 3 4	7-56
:OPARea	ALL INL1-L2 OUTL1-L2 0 1 2	7-56
:THresh	<integer>[DB]	7-56
:PCVft:THResh	<integer>[DB]	7-56
:PARameter		
[:CATegory]		
:DFBLd	<item>,<paramater name>,<data>	7-57
:FILBtm	<item>,<paramater name>,<data>	7-57
:FILPk	<item>,<paramater name>,<data>	7-58
:FPLD	<item>,<paramater name>,<data>	7-58
:LED	<item>,<paramater name>,<data>	7-59
:NF		
:AALGo	AFIX MFIx ACENter MCENter 0 1 2 3	7-59
:FALGo	LINear GAUss LORenz 3RD 4TH 5TH 0 1 2 3 4 5	7-59
:FARea	<NRF>[M]	7-60
:IOFFset	<NRF>[DB]	7-60
:MARea	<NRF>[M]	7-60
:MDIFF	<NRF>[DB]	7-60
:OOFFset	<NRF>[DB]	7-60
:PDISplay	OFF ON 0 1	7-60
:TH	<NRF>[DB]	7-61
:RBWidth	MEASURED CAL 0 1	7-61
:SNoise	OFF ON 0 1	7-61
:NOTCh		
:K	<NRF>	7-61
:TH	<NRF>[DB]	7-61
:TYPE	PEAK BOTTom 0 1	7-61
:PMd		
:TH	<NRF>[DB]	7-61
:POWer		
:OFFSet	<NRF>[DB]	7-62
:SMSR		
:MASK	<NRF>[M]	7-62
:MODE	SMSR1 SMSR2 SMSR3 SMSR4	7-62
:SWEnvelope		
:K	<NRF>	7-62
:TH1	<NRF>[DB]	7-62
:TH2	<NRF>[DB]	7-62
:SWPKrms		
:K	<NRF>	7-62
:TH	<NRF>[DB]	7-63
:SWRMs		
:K	<NRF>	7-63
:TH	<NRF>[DB]	7-63
:SWThresh		
:K	<NRF>	7-63
:MFIT	OFF ON 0 1	7-63
:TH	<NRF>[DB]	7-63
:WDM		
:DMASK	<NRF>[DB]	7-64
:DTPe	ABSolute RELative MDrift GDrift 0 1 2 3	7-64
:DUAL	OFF ON 0 1	7-64
:FALGo	LINear GAUss LORenz 3RD 4TH 5TH 0 1 2 3 4 5	7-64
:IRange	<NRF>	7-65
:MARea	<NRF>[M]	7-65
:MDIFF	<NRF>[DB]	7-65
:MMReset	None	7-65
:NALGo	AFIX MFIx ACENter MCENter PIT 0 1 2 3 4	7-65
:NARea	<NRF>[M]	7-65
:NBW	<NRF>[M]	7-65
:OSlope	OFF ON 0 1	7-66
:PDISplay	OFF ON 0 1	7-66

## 7.4 Remote Command Tree

Command	Parameter	Page
:RCH	<integer>	7-66
:RELation	OFFSet   SPACing 0 1	7-66
:SPoWer	PEAK INTegral 0 1	7-66
:TH	<NRF>[DB]	7-66
:WFBottom	<item>,<paramater name>,<data>	7-67
:WFPeak	<item>,<paramater name>,<data>	7-67
:COMMON		
:MDIFF	<NRF>[DB]	7-67
<b>CALibration</b>		
:ALIGn		
:EXTernal[:IMMediate]	none	7-68
[::IMMediate]	none	7-68
:INTernal[:IMMediate]	none	7-68
:BANDwidth[:BWIDth]		
[::IMMediate]	none	7-68
:INITialize	none	7-68
:WAVelength?	none	7-68
:POWeR		
:OFFSet:TABLE	<integer>,<NRF>[DB]	7-68
:WAVelength		
:EXTernal		
[::IMMediate]	none	7-69
:SOURce	LASEr GASCell EMISSION	7-69
:WAVelength	<NRF>M	7-69
:INTernal[:IMMediate]	none	7-69
:OFFSet:TABLE	<integer>,<NRF>	7-69
:ZERO[:AUTO]	OFF ON 0 1 ONCE	7-70
:INTerval	<integer>	7-70
:STATus?	none	7-70
<b>DISPlay</b>		
:COLor	0 1 2 3 4 5	7-70
[::WINDOW]	OFF ON 0 1	7-70
:OVView		
:POSITION	OFF LEFT RIGHT 0 1 2	7-70
:SIZE	LARGE SMALL 0 1	7-70
:SPLIT	OFF ON 0 1	7-71
:HOLD		
:LOWer	OFF ON 0 1	7-71
:UPPer	OFF ON 0 1	7-71
:POSITION	<trace name>,UP LOW 0 1	7-71
:TEXT		
:CLEar	none	7-71
:DATA	<"string">	7-71
:TRACe		
:X[:SCALE]		
:CENTer	<NRF>[M HZ]	7-71
:INITialize	none	7-71
:SMScale	none	7-72
:SPAN	<NRF>[M HZ]	7-72
:SRANGE	OFF ON 0 1	7-72
:START	<NRF>[M HZ]	7-72
:STOP	<NRF>[M HZ]	7-72
:Y		
:NMASK	<NRF>DB	7-72
:TYPE	VERTical HORIZONTAL 0 1	7-73
[::SCALE]		
:DNUmber	8 10 12	7-73
:Y1		
[::SCALE]		
:BLEvel	<NRF>[W MW UW NW]	7-73
:PDIvision	<NRF>[DB]	7-73
:RLEvel	<NRF>[DBM W	7-73
:RPosition	<integer>[DIV]	7-74
:SPACing	LOGarithmic LINear 0 1	7-74
:UNIT	DBM W DBM/NM W/NM 0 1 2 3	7-74

Command	Parameter	Page
:Y2		
[:SCALE]		
:AUTo	OFF ON 0 1	7-74
:LENGth	<NRF>[KM]	7-74
:OLEVel	<NRF>[DB DB/KM]	7-74
:PDIVisiOn	<NRF>[DB DB KM %]	7-75
:RPOSITION	<integer>[DIV]	7-75
:SMINimum	<NRF>[%]	7-75
:UNIT	DB LINEar DB/KM % 0 1 2 3	7-75
FORMAT		
[:DATA]	REAL[,64 ,32] ASCii	7-76
HCOPy		
:DESTination	INTernal FILE 0 2	7-76
[:IMMediate]	none	7-76
:FEED	[<integer>]	7-76
:FUNCTION		
:CALCulate:LIST	none	7-76
:MARKer:LIST	none	7-76
INITiate		
[:IMMediate]	none	7-77
:SMODE	SINGLe REPeat AUTO SEGment 1 2 3 4	7-77
MEMory		
:MMEMory:ANAMe	NUMBER DATE	7-77
:CLEar	<integer>	7-77
:EMPtY?	<integer>	7-77
:LOAD	<integer>,<trace name>	7-77
:STORe	<integer>,<trace name>	7-77
MMEMemory		
:CATalog?	[INTernal EXTernal]	7-78
:CDIRectory	<"directory name">	7-78
:CDRive	INTernal EXTernal	7-78
:COPY	<"source file name">, [INTernal EXTernal], <"destination file name">[,INTernal  EXTernal]	7-78
:DATA?	<"file name">[,INTernal EXTernal]	7-78
:DElete	<"file name">[,INTernal EXTernal]	7-78
:LOAD		
:ATRace	<"file name">[,INTernal EXTernal]	7-79
:DLOGing	<"file name">[,INTernal EXTernal]	7-79
:MEMORY	<integer>,<"filename">[,INTernal  EXTernal]	7-79
:PROGram	<integer>,<"filename">[,INTernal  EXTernal]	7-79
:SETTing	<"filename">[,INTernal EXTernal]	7-79
:TEMPlate	<template>,<"filename">[,INTernal  EXTernal]	7-79
:TRACe	<trace name>,<"filename">[,INTernal  EXTernal]	7-79
:MDIRectory	<"directory name">[,INTernal  EXTernal]	7-79
:REMove	None	7-79
:REName	<"new file name">,<"old file name"> [,INTernal EXTernal]	7-80
:STORe		
:ARESult	<"filename">[,INTernal EXTernal]	7-80
:ATRace	<"file name">[,INTernal EXTernal]	7-80
:DATA	<"filename">,[,INTernal EXTernal]	7-80
:ITEM	DATE LABel DATA CONDition TRACe,OFF  ON 0 1	7-80
:MODE	ADD OVER 0 1	7-80
:TYPE	CSV DT 0 1	7-80
:DLOGging	<"filename">[,INTernal EXTernal]	7-81
:CSAVe	OFF ON 0 1	7-81
:TSAVe	OFF ON 0 1	7-81

## 7.4 Remote Command Tree

Command	Parameter	Page
:GRAphics	B&W COLOR PCOLOR,BMP TIFF,<"filename"> [,INTERNAL EXTERNAL]	7-81
:MEMory	<integer>,BI CSV,<"filename"> [,INTERNAL EXTERNAL]	7-81
:PROGram	<integer>,<"filename">[,INTERNAL EXTERNAL]	7-81
:SETTING	<"filename">[,INTERNAL EXTERNAL]	7-82
:TEMPplate	<template>,<"filename">[,INTERNAL EXTERNAL]	7-82
:TRACe	<trace name>,BIN   CSV,<"filename"> [,INTERNAL EXTERNAL]	7-82
<b>PROGram</b>		
:EXECutE	<integer>	7-82
<b>SENSe</b>		
:AVERage:COUNt	<integer>	7-83
:BANDwidth[:BWIDth]	<NRf>[M Hz]	7-83
[ :RESolution]		
:CHOPper	OFF SWITch 0 2	7-83
:CORRection		
:LEVel:SHIFT	<NRf>[DB]	7-83
:RVELocity:MEDIUM	AIR VACUum 0 1	7-83
:WAVelength:SHIFT	<NRf>[M]	7-83
:SENSe	NHLD NAUT NORMAL MID HIGH1 HIGH2  HIGH3 0 1 6 2 3 4 5	7-83
:SETTING		
:CORRection	OFF ON 0 1	7-84
:FCONnetcor	NORMAL ANGLe 0 1	7-84
:FIBer	SMALL LARGE 0 1	7-84
:SMOOthing	OFF ON 0 1	7-84
:SWEep		
:POINTs	<integer>	7-84
:AUTO	OFF ON 0 1	7-84
:SEGment:POINTS	<integer>	7-84
:SPEED	1x 2x 0 1	7-85
:STEP	<NRf>[M]	7-85
:TIME		
:ONM	<integer>[SEC]	7-85
:INTERval	<integer>[SEC]	7-85
:TLSSync	OFF ON 0 1	7-85
:WAVelength		
:CENTer	<NRf>[M HZ]	7-85
:SPAN	<NRf>[M HZ]	7-85
:SRANGE	OFF ON 0 1	7-86
:START	<NRf>[M HZ]	7-86
:STOP	<NRf>[M HZ]	7-86
<b>STATus</b>		
:OPERation		
:CONDition?	none	7-86
:ENABL	<integer>	7-86
[ :EVENT]?	none	7-86
:PRESet	none	7-86
:QUEstionable		
:CONDition?	none	7-87
:ENABLE	<integer>	7-87
[ :EVENT]?	none	7-87

## 7.4 Remote Command Tree

Command	Parameter	Page
<b>SYSTem</b>		
<b>:BUZZer</b>		
<b>:CLIC</b>	OFF ON 0 1	7-87
<b>:WARNING</b>	OFF ON 0 1	7-87
<b>:COMMUnicate</b>		
<b>:CFORmat</b>	AQ6317 AQ6370 AQ6375 AQ6370C AQ6373  AQ6370D 0 1	7-87
<b>:GP-IB2</b>		
<b>:ADDResS</b>	<integer>	7-88
<b>:SCONtroller</b>	OFF ON 0 1	7-88
<b>:TLS:ADDResS</b>	<integer>	7-88
<b>:LOCKout</b>	OFF ON 0 1	7-88
<b>:RMONitor</b>	OFF ON 0 1	7-89
<b>:DATE</b>	YYYY,mm,dd	7-89
<b>:DISPlay</b>		
<b>:TRANsparent</b>	OFF ON 0 1	7-89
<b>:UNCal</b>	OFF ON 0 1	7-89
<b>:ERRor</b>		
<b>[ :NEXT]?</b>	none	7-89
<b>:GRID</b>	12.5GHZ 25GHz 50GHz 100GHz 200GHz  CUSTom 0 1 2 3 4 5	7-89
<b>:CUSTom</b>		
<b>:CLEar:ALL</b>	none	7-89
<b>:DElete</b>	<grid number>	7-89
<b>:INsert</b>	<NRf>[M HZ]	7-90
<b>:SPACing</b>	<NRf>[GHZ]	7-90
<b>:STARt</b>	<NRf>[M HZ]	7-90
<b>:STOP</b>	<NRf>[M HZ]	7-90
<b>:REFerence</b>	<NRf>[M HZ]	7-90
<b>:INFormation?</b>	0 1	7-90
<b>:PRESet</b>	none	7-91
<b>:TIME</b>	hh,mm,ss	7-91
<b>:VERSion?</b>		7-91

## 7.4 Remote Command Tree

Command	Parameter	Page
<b>TRACe</b>		
:ACTIVE	<trace name>	7-91
:ATTRibute[:<trace name>]	WRITE FIX MAX MIN RAVG CALC	7-91
:RAVG[:<trace name>]	<integer>	7-92
:COPY	<source trace>,<destination trace>	7-92
[ :DATA]		
:SNUmber?	<trace name>	7-92
:X?	<trace name>[,<start point>,<stop point>]	7-92
:Y?	<trace name>[,<start point>,<stop point>]	7-92
:PDENSity?	<trace name>,<NRF>[,<start point>,<stop point>]	7-93
:DELETE	<trace name>	7-93
:ALL		7-93
:STATE[:<trace name>]	OFF ON 0 1	7-93
:TEMPplate		
:DATA	<template>,<wavelength>,<level>	7-93
:ADElete	<template>	7-94
:ETYPE	<template>,NONE A B 0 1 2	7-94
:MODE	<template>,ABSolute RELative 0 1	7-94
:DISPLAY	<template>,OFF ON 0 1	7-94
:GONogo	OFF ON 0 1	7-94
:LEVel:SHIFT	<NRF>[DB]	7-94
:RESult?		7-94
:TTYPe	UPPer LOWER U&L 0 1 2	7-95
:WAVelength:SHIFT	<NRF>[M]	7-95
<b>TRIGger</b>		
[ :SEQUence]		
:DELAY	<NRF>[S MS US]	7-95
:SLOPe	RISE FALL 0 1	7-96
:STATE	OFF ON PHOLD 0 1 2	7-96
:INPUT	ETRigger STRigger SENable 0 1 2	7-96
:OUTPut	OFF SStatus 0 1	7-96
:PHOLD:HTIME	<NRF>[s]	7-96
<b>UNIT</b>		
:POWER:DIGit	1 2 3	7-97
:X	WAveLength FREQuency WNUMBer 0 1 2	7-97

## 7.5 Common Commands

The instrument supports the “Required” common commands listed in the table below.

Cmd	Name	IEEE 488.2 Std.	AQ6370C/AQ6373 AQ6370DAQ6375
*AAD	Accept Address Command	Option	
*CAL?	Calibration Query	Option	
*CLS	Clear Status Command	Required	Y
*DDT	Define Device Trigger Command	*DT1 option	
*DDT?	Define Device Trigger Query	DT1 option	
*DLF	Disable Listener Function Command	Option	
*DMC	Define Macro Command	Option	
*EMC	Enable Macro Command	Option	
*EMC?	Enable Macro Query	Option	
*ESE	Standard Event Status Enable Command	Required	Y
*ESE?	Standard Event Status Enable Query	Required	Y
*ESR?	Standard Event Status Register Query	Required	Y
*GMC?	Get Macro Contents Query	Option	
*IDN?	Identification Query	Required	Y
*IST?	Individual Status Query	Required for PP1	
*LMC?	Learn Macro Query	Option	
*LRN?	Learn Device Setup Query	Option	
*OPC	Operation Complete Command	Required	Y
*OPC?	Operation Complete Query	Required	Y
*OPT	Option Identification Query	Option	
*PCB	Pass Control Back Command	Required if not C0	
*PMC	Purge Macro Command	Option	
*PRE	Parallel Poll Register Enable Command	Required for PP1	
*PRE?	Parallel Poll Register Enable Query	Required for PP1	
*PSC	Power On Status Clear Command	Option	
*PSC?	Power On Status Clear Query	Option	
*PUD	Protected User Data Command	Option	
*PUD?	Protected User Data Query	Option	
*RCL	Recall Command	Option	
*RDT	Resource DescriptionTransfer Command	Option	
*RDT?	Resource Description Transfer Query	Option	
*RST	Reset Command	Required	Y
*SAV	Save Command	Option	
*SRE	Service Request Enable Command	Required	Y
*SRE?	Service Request Enable Query	Required	Y
*STB?	Read Status Byte Query	Required	Y
*TRG	Trigger Command	Required if DT1	Y
*TST?	Self-Test Query	Required	Y
*WAI	Wait-to-Continue Command	Required	Y

Y: Commands supported by the AQ6370C, AQ6373 and AQ6375

## 7.5 Common Commands

### \*CLS (Clear Status)

Function	Clears all event status registers, the summary of which is reflected in the status byte register.
Syntax	*CLS
Example	*CLS
Explanation	<ul style="list-style-type: none"> <li>• Clears all queues, with the exception of the output queue, and all event registers, with the exception of the MAV summary message.</li> <li>• After executing this command, OCIS (Operation Complete Command Idle State) and OQIS (Operation Complete Query Idle State) are brought about.</li> <li>• This is a sequential command.</li> </ul>

### \*ESE (Standard Event Status Enable)

Function	Sets/queries the standard event enable register.
Syntax	<pre>*ESE&lt;wsp&gt;&lt;integer&gt; *ESE? &lt;integer&gt; = 0–255</pre>
Example	<pre>*ESE 251 *ESE? -&gt; 251</pre>
Explanation	<ul style="list-style-type: none"> <li>• An item having had its bit set becomes enabled.</li> <li>• Resets to the default value in the following cases: <ul style="list-style-type: none"> <li>When power is ON</li> <li>When “0” is set</li> </ul> </li> <li>• The set value remains the same in the following cases: <ul style="list-style-type: none"> <li>*RST</li> <li>*CLS</li> </ul> </li> <li>• Device clear (DCL, SDC)</li> <li>• The default is 0.</li> <li>• This is a sequential command.</li> </ul>

### \*ESR? (Standard Event Status Register)

Function	Queries the standard event status register and simultaneously clears it.
Syntax	*ESR?
Example	*ESR? -> 251

Explanation

- The return value of this query is not affected by ESE (Event Status Enable Register).
- This is an overlapping command.

### \*IDN? (Identification)

Function	Queries the instrument type and firmware version.
Syntax	*IDN?
Example	*IDN? ->
	<pre>YOKOGAWA,AQ6370C,aaaaaaaa,bb.bb aaaaaaaa: Serial number (9 digit string) bb.bb: Firmware version</pre>

Explanation

- Outputs 4 field data delimited by a comma.
- Field 1: Manufacturer “YOKOGAWA”
- Field 2: Model “AQ6370C”, “AQ6373” “AQ6370D” or “AQ6375”
- Field 3: Instrument serial number
- Field 4: Firmware version
- For the AQ6370C, field 2 is “AQ6370C.”
- For the AQ6370D, field 2 is “AQ6370D.”
- For the AQ6373, field 2 is “AQ6373.”
- For the AQ6375, field 2 is “AQ6375.”
- This is a sequential command.

### \*OPC (Operation Complete)

Function	Sets/queries bit 0 (OPC) of the standard event status register (ESR) if operations waiting to be processed have all been completed.
Syntax	<pre>*OPC *OPC?</pre>
Example	<pre>*OPC *OPC? -&gt; 1</pre>
Explanation	<ul style="list-style-type: none"> <li>• At the time this command is recognized, the command changes from OCIS (Operation Complete Command Idle State) to OCAS (Operation Complete Command Active State). When the no-operation pending flag is set to “True,” it sets bit 0 (OCR) of ESR and returns to OCIS.</li> <li>• If any of the following conditions are established, this command is disabled and is forced to return to OCIS. <ul style="list-style-type: none"> <li>Power ON</li> <li>Device clear</li> <li>*CLS, *RST command</li> </ul> </li> <li>• This is an overlapping command.</li> </ul>

**\*RST (Reset)**

Function	Executes a device reset to return the instrument to the known (default) status.
Syntax	*RST
Example	*RST
Explanation	<ul style="list-style-type: none"> <li>• Stops operation being processed and returns the instrument to the known set value (default value) immediately.</li> <li>• This unit's parameters are cleared.</li> <li>• The following items will remain the same.</li> </ul> <p>GP-IB interface status</p> <p>GP-IB address</p> <p>Output queue</p> <p>SRE</p> <p>ESE</p> <p>Calibration data affecting the instrument's specifications</p> <ul style="list-style-type: none"> <li>• This is an overlapping command.</li> </ul>

**\*SRE (Service Request Enable)**

Function	Sets/queries the service request enable register.
Syntax	*SRE <wp><integer> *SRE? <integer> = 0–255
Example	*SRE 250 *SRE? -> 250
Explanation	<ul style="list-style-type: none"> <li>• An item having had its bit set becomes enabled.</li> <li>• Resets to the default value in the following cases: <ul style="list-style-type: none"> <li>When power is ON</li> <li>When "0" is set</li> </ul> </li> <li>• The set value remains the same in the following cases: <ul style="list-style-type: none"> <li>*RST</li> <li>*CLS</li> <li>Device clear (DCL, SDC)</li> </ul> </li> <li>• The default is 0.</li> <li>• This is a sequential command.</li> </ul>

**\*STB? (Read Status Byte)**

Function	Queries the current value of the status byte register.
Syntax	*STB?
Example	*STB? -> 251
Explanation	<ul style="list-style-type: none"> <li>• STB will not be cleared even when the contents of the register are read.</li> <li>• This is an overlapable command.</li> </ul>

**\*TRG (Trigger)**

Function	Performs a <SINGLE> sweep under the sweep conditions established immediately before receiving the command.
Syntax	*TRG
Example	*TRG

**\*TST? (Self Test)**

Function	Performs the instrument's self-test and queries the status.
Syntax	*TST?
Example	*TST? -> 0
Explanation	<ul style="list-style-type: none"> <li>• Of the initialization sequence to be run at startup, this command executes the following operations to output their results. During initialization, the screen maintains the waveform display.</li> <li>Motor's return to origin operation</li> <li>AMP auto-offset</li> <li>• Normally returns 0, or 1 for motor initialize error, or 2 for AMP offset error.</li> <li>• This is a sequential command.</li> </ul>

**\*WAI (Wait to Continue)**

Function	Prevents the instrument from executing another command until the execution of the current command is complete.
Syntax	*WAI
Example	*WAI

Explanation	<ul style="list-style-type: none"> <li>• Becomes invalid by device clear.</li> <li>• Meaningful if subsequent commands are overlapping. Meaningless with other commands.</li> <li>• This is a sequential command.</li> </ul>
-------------	------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

## 7.6 Instrument-Specific Commands

### ABORt Sub System Command

#### :ABORT

Function	Stops operations such as measurements and calibration.
Syntax	ABORT
Example	ABORT
Explanation	<ul style="list-style-type: none"><li>Operations to be stopped are as follows: :APPLication:DLOGging:STATE :CALibration:ALIGn[:IMMediate] :CALibration:ALIGn:EXTernal[:IMMediate] :CALibration:ALIGn:INTernal[:IMMediate] :CALibration:BANDwidth BWIDth[:IMMediate] :CALibration:WAveLength :INITiate :PROGram:EXECute :HCOPY[:INITiate] :HCOPY[:INITiate]:FUNCTION:CALCulate:LIST :HCOPY[:INITiate]:FUNCTION:MARKer:LIST</li><li>This is an overlapping command.</li></ul>

### APPLICATION Sub System Commands

#### Overview

- This subsystem consists of data logging commands.

#### :APPLICATION:DLOGging:ETIME?

Function	Queries the elapsed time of data logging (in seconds).
Syntax	:APPLICATION:DLOGging:ETIME? Response <integer> <integer> = Elapsed time [sec]
Example	:APPLICATION:DLOGGING:ETIME? -> 10220
Description	<ul style="list-style-type: none"><li>This is an overlap command.</li><li>This command can be used on the AQ6370D/AQ6370C/AQ6373B.</li><li>This command is invalid when data logging is paused.</li></ul>

#### :APPLICATION:DLOGging:LParameter:INTERval

Function	Sets or queries the measurement interval of data logging.
Syntax	:APPLICATION:DLOGging:LParameter:INTERval<wsp><integer>[SEC] :APPLICATION:DLOGging:LParameter:INTERval? <integer> = Measurement interval [sec] (0 = SWEEP TIME)
Example	:APPLICATION:DLOGGING:LPARAMETER:INTERVAL 10 :APPLICATION:DLOGGING:LPARAMETER:INTERVAL? -> 10
Description	<ul style="list-style-type: none"><li>This command is invalid when data logging is in progress.</li><li>This is a sequential command.</li><li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li></ul>

<b>:APPLication:DLOGging:LParameter:IT EM</b>	
Function	Sets or queries the data logging source.
Syntax	:APPLication:DLOGging:LParameter:IT EM<wp>0 1 2 3 :APPLication:DLOGging:LParameter:IT EM? 0 1 2 3: Data logging source 0 = WDM, 1 = PEAK, 2 = MULTI-PEAK, 3 = DFB-LD
Example	:APPLICATION:DLOGGING:LPARAMETER:IT EM 0 :APPLICATION:DLOGGING:LPARAMETER:IT EM? -> 0
Description	<ul style="list-style-type: none"> <li>This command is invalid when data logging is in progress.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

<b>:APPLication:DLOGging:LParameter:LMO De</b>	
Function	Sets or queries the data logging mode (maximum channel mode or maximum logging mode).
Syntax	:APPLication:DLOGging:LParameter:LM ODE<wp>1 2 :APPLication:DLOGging:LParameter:LM ODE? 1 2: Mode 1 = Maximum channel mode (MODE1: MAX 1024ch, 2001 entries) 2 = Maximum logging mode (MODE2: MAX 256ch, 10001 entries)
Example	:APPLICATION:DLOGGING:LPARAMETER:LM ODE 1 :APPLICATION:DLOGGING:LPARAMETER:LM ODE -> 1
Description	<ul style="list-style-type: none"> <li>This command is invalid when data logging is in progress.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

<b>:APPLication:DLOGging:LParameter:MEM ory</b>	
Function	Sets or queries the temporary area for saving waveform files of data logging.
Syntax	:APPLication:DLOGging:LParameter:ME Mory<wp>INTERNAL EXTERNAL :APPLication:DLOGging:LParameter:ME Mory? INTERNAL = Internal memory EXTERNAL = USB storage media
Example	:APPLICATION:DLOGGING:LPARAMETER:ME MORY INTERNAL :APPLICATION:DLOGGING:LPARAMETER:ME MORY? -> INT
Description	<ul style="list-style-type: none"> <li>This command is invalid when data logging is in progress.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

<b>:APPLication:DLOGging:LParameter:MTH Resh</b>	
Function	Sets or queries the threshold of the channel-matching wavelength $\lambda$ for data logging.
Syntax	:APPLication:DLOGging:LParameter:MT HResh<wp><NRf>[M] :APPLication:DLOGging:LParameter:MT HResh? <NRf>[M] = Threshold of wavelength $\lambda$ [m]
Example	:APPLICATION:DLOGGING:LPARAMETER:MT HResh 0.1nm :APPLICATION:DLOGGING:LPARAMETER:MT HResh? -> +1.0000000E-010
Description	<ul style="list-style-type: none"> <li>This command is invalid when data logging is in progress.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## 7.6 Instrument-Specific Commands

### :APPLICATION:DLOGGING:LParameter:PDE

#### Tect:ATHResh

Function	Sets or queries the threshold (absolute value) for detecting the data logging mode.
Syntax	:APPLICATION:DLOGGING:LParameter:PD ETect:ATHResh<NRF> [DB] :APPLICATION:DLOGGING:LParameter:PD ETect:ATHResh? <NRF>[DB] = Peak detection threshold (absolute value) [dBm]
Example	:APPLICATION:DLOGGING:LParameter:PD ETECT:ATHRESH -20.0dbm :APPLICATION:DLOGGING:LParameter:PD ETECT:ATHRESH? -> -2.0000000E+001
Description	<ul style="list-style-type: none"><li>This command is invalid when data logging is in progress.</li><li>This is a sequential command.</li><li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li></ul>

### :APPLICATION:DLOGGING:LParameter:PDE

#### Tect:RTHResh

Function	Sets or queries the threshold (relative value) for detecting the data logging mode.
Syntax	:APPLICATION:DLOGGING:LParameter:PD ETect:RTHResh<NRF> [DB] :APPLICATION:DLOGGING:LParameter:PD ETect:RTHResh? <NRF>[DB] = Peak detection threshold (relative value) [dB]
Example	:APPLICATION:DLOGGING:LParameter:PD ETECT:RTHRESH 30.0db :APPLICATION:DLOGGING:LParameter:PD ETECT:RTHRESH? -> +3.0000000E+001
Description	<ul style="list-style-type: none"><li>This command is invalid when data logging is in progress.</li><li>This is a sequential command.</li><li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li></ul>

### :APPLICATION:DLOGGING:LParameter:PDE

#### Tect:TTYPE

Function	Sets or queries how the threshold for detecting the data logging mode (peak or bottom) is specified.
Syntax	:APPLICATION:DLOGGING:LParameter:PD ETect:TTYPE<wsp>ABSolute RELative :APPLICATION:DLOGGING:LParameter:PD ETect:TTYPE? ABSolute = Absolute value RELative = Relative value
Example	:APPLICATION:DLOGGING:LParameter:PD ETECT:TTYPE ABSOLUTE :APPLICATION:DLOGGING:LParameter:PD ETECT:TTYPE? -> ABS
Description	<ul style="list-style-type: none"><li>This command is invalid when data logging is in progress.</li><li>This is a sequential command.</li><li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li></ul>

### :APPLICATION:DLOGGING:LParameter:TDU

#### Ration

Function	Sets or queries the measurement duration of data logging (in seconds).
Syntax	:APPLICATION:DLOGGING:LParameter:TD URation<wsp><integer>[sec] :APPLICATION:DLOGGING:LParameter:TD URation? <integer> = Measurement duration [sec]
Example	:APPLICATION:DLOGGING:LParameter:TD URation 3600 :APPLICATION:DLOGGING:LParameter:TD URation? -> 3600
Description	<ul style="list-style-type: none"><li>This command is invalid when data logging is in progress.</li><li>This is a sequential command.</li><li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li></ul>

<b>:APPLication:DLOGging:LParameter:TLOGging</b>	
Function	Sets or queries whether waveforms will be logged during data logging.
Syntax	:APPLication:DLOGging:LParameter:TLOGging<wsp>OFF ON 0 1 :APPLication:DLOGging:LParameter:TLOGging? OFF = Waveform data save function off ON = Waveform data save function on
Example	:APPLICATION:DLOGGING:LPARAMETER:TLOGGING OFF :APPLICATION:DLOGGING:LPARAMETER:TLOGGING? -> 0
Description	<ul style="list-style-type: none"> <li>This command is invalid when data logging is in progress.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

<b>:APPLication:DLOGging:STATE</b>	
Function	Starts, stops, or queries data logging.
Syntax	:APPLication:DLOGging:STATE<wsp>STOP START 0 1 :APPLication:DLOGging:STATE? START = Starts data logging STOP = Stops data logging Response 0 = Stopped, 1 = Running
Example	:APPLICATION:DLOGGING:STATE 1 :APPLICATION:DLOGGING:STATE? -> 1
Description	<ul style="list-style-type: none"> <li>Only the following commands are valid when data logging is in progress.           <ul style="list-style-type: none"> <li>Common commands (excluding *TRG and *TST)</li> <li>All query commands</li> <li>ABORT</li> </ul> </li> <li>This is an overappable command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## CALCulate Sub System Command

### Outline

- Commands about the following functions are summarized in this sub system.
  - Analysis function (Spectrum Width, ANALYSIS1 , ANALYSIS2)
  - Peak/Bottom search function
  - Marker function ( $\Delta$  marker, line marker)
  - Calculation function of trace
  - Advanced marker function (moving marker, power density marker, integrated power marker)
- The following procedure is performed in order to carry out remote control of the Analysis function.
  - Select the analysis algorithm (CALCulate:CATegory command)
  - Set the Analysis Parameter (CALCulate:PARameter command)
  - Execute the analysis function (CALCulate[:IMMEDIATE] command)
  - Get the analysis results (CALCulate:DATA? command)
- The following command is used in order to carry out remote control of the Peak/Bottom search function. CALCulate:MARKer:MAXimum|MINimum command
- The following command is used to in order to carry out remote control of the Marker function.
  - $\Delta$  marker: CALCulate:MARKer command
  - Line marker: CALCulate:LMARKer command
- The following command is used to in order to carry out remote control of the trace Calculation function. CALCulate:MATH command

### **:CALCulate:AMARKer[1|2|3|4]:AOFF**

Function	Clears all advanced markers (moving markers, power density markers, and integrated power markers) and turns off the advanced marker function.
Syntax	:CALCulate:AMARKer[1 2 3 4]:AOFF [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:AOFF
Description	<ul style="list-style-type: none"> <li>After clearing, the advanced marker function automatically turns off.</li> <li>All advanced markers are cleared regardless of which advanced marker you specify.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## 7.6 Instrument-Specific Commands

**:CALCulate:AMARKer[1|2|3|4]:FUNCTION  
:INTEGRal:IRANGE**

Function	Sets or queries the integration frequency range of the specified integrated power marker.
Syntax	:CALCulate:AMARKer[1 2 3 4]:FUNCTION:INTEGRal:IRANGE<wsp><NRf>[Hz] :CALCulate:AMARKer[1 2 3 4]:FUNCTION:INTEGRal:IRANGE? [1 2 3 4]: Advanced marker number <NRf> = Integration frequency range [Hz]
Example	:CALCULATE:AMARKER:FUNCTION:INTEGRAL:IRANGE 40GHZ :CALCULATE:AMARKER:FUNCTION:INTEGRAL:IRANGE? -> 4.0000000E+010
Description	<ul style="list-style-type: none"> <li>• An execution error will occur if the specified advanced marker has not been assigned or is not an integrated power marker.</li> <li>• A query error will occur if the specified advanced marker has not been assigned or is not an integrated power marker.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

**:CALCulate:AMARKer[1|2|3|4]:FUNCTION  
:INTEGRal:RESUlt?**

Function	Queries the integration value of the specified integrated power marker.
Syntax	:CALCulate:AMARKer[1 2 3 4]:FUNCTION:INTEGRal:RESUlt? [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:FUNCTION:INTEGRAL:RESULT? -> -1.0000000E+001
Description	<ul style="list-style-type: none"> <li>• The unit of the returned marker level depends on the Y-axis unit of the assigned marker trace.</li> <li>• A query error will occur if the specified advanced marker has not been assigned or is not an integrated power marker.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

**:CALCulate:AMARKer[1|2|3|4]:FUNCTION  
:INTEGRal[:STATE]**

Function	Moves the specified integrated power marker to the center of the marker trace. Also queries the status of the specified integrated power marker.
Syntax	:CALCulate:AMARKer[1 2 3 4]:FUNCTION:INTEGRal[:STATE]<wsp>OFF ON 0 1 :CALCulate:AMARKer[1 2 3 4]:FUNCTION:INTEGRal[:STATE]?
Example	:CALCULATE:AMARKER:FUNCTION:INTEGRAL ON :CALCULATE:AMARKER:FUNCTION:INTEGRAL?
Description	<ul style="list-style-type: none"> <li>• If an integrated power marker is assigned, moving markers (:CALCulate:AMARKer[1 2 3 4][:STATE]) and power density markers (:CALCulate:AMARKer[1 2 3 4]:FUNCTION:PDENSity:NOISE[:STATE]) will be set to off.</li> <li>• If this command with the parameter set to OFF is specified on an advanced marker that has been assigned to integrated power marker, the advanced marker will change to a moving marker.</li> </ul> <p>If the advanced marker has not been assigned, using this command with the parameter set to OFF will leave the advanced marker unassigned.</p> <ul style="list-style-type: none"> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## 7.6 Instrument-Specific Commands

<b>:CALCulate:AMARKer[1 2 3 4]:FUNCTION:PDENsity[:NOISE:BWIDth]:BANDwidth</b>	
Function	Sets or queries the normalization bandwidth of the specified power density marker.
Syntax	:CALCulate:AMARKer:FUNCTION:PDENsity[:NOISE:BWIDth]:BANDwidth<wsp><NRf>[m] :CALCulate:AMARKer:FUNCTION:PDENsity[:NOISE:BWIDth]:BANDwidth?<NRf> = Normalization bandwidth [m]
Example	:CALCULATE:AMARKER:FUNCTION:PDENSITY:BWIDTH 0.1nm :CALCULATE:AMARKER:FUNCTION:PDENSITY:BWIDTH -> +1.0000000E-010
Description	<ul style="list-style-type: none"> <li>This command applies to advanced markers 1 to 4. The command operates in the same manner regardless of which advanced marker is specified.</li> <li>An execution error will occur if the specified advanced marker has not been assigned or is not a power density marker.</li> <li>A query error will occur if the specified advanced marker has not been assigned or is not a power density marker.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>
<b>:CALCulate:AMARKer[1 2 3 4]:FUNCTION:PDENsity[:NOISE:RESult?]</b>	
Function	Sets or queries the power density value of the specified power density marker.
Syntax	:CALCulate:AMARKer[1 2 3 4]:FUNCTION:PDENsity[:NOISE:RESult?][1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:FUNCTION:PDENSITY:RESULT? -> -1.0000000E+001
Description	<ul style="list-style-type: none"> <li>The unit of the returned marker level depends on the Y-axis unit of the assigned marker trace.</li> <li>A query error will occur if the specified advanced marker has not been assigned or is not a power density marker.</li> <li>If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>
<b>:CALCulate:AMARKer[1 2 3 4]:FUNCTION:PRESet</b>	
Function	Changes the specified advanced marker to a moving marker.
Syntax	:CALCulate:AMARKer[1 2 3 4]:FUNCTION:PRESet[1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:FUNCTION:PRESET
Description	<ul style="list-style-type: none"> <li>If an advanced marker is assigned to a power density marker or integrated power marker, the marker can be changed directly to a moving marker.</li> <li>This does not change the marker position.</li> <li>If the advanced marker has not been assigned, using this command will leave the advanced marker unassigned.</li> <li>If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## 7.6 Instrument-Specific Commands

### **:CALCulate:AMARKer[1|2|3|4]:MAXimum**

Function	Detects the peak and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MAXimum [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MAXIMUM
Description	<ul style="list-style-type: none"> <li>• If the specified advanced marker has not been assigned, a moving marker will be assigned.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:CALCulate:AMARKer[1|2|3|4]:MAXimum:**

#### **LEFT**

Function	Detects the closest peak to the left of the current specified advanced marker position and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MAXimum :LEFT [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MAXIMUM:LEFT
Description	<ul style="list-style-type: none"> <li>• If the specified advanced marker has not been assigned, a moving marker will be assigned.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:CALCulate:AMARKer[1|2|3|4]:MAXimum:**

#### **NEXT**

Function	Detects the highest peak whose level is less than or equal to that of the current specified advanced marker position and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MAXimum :NEXT [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MAXIMUM:NEXT
Description	<ul style="list-style-type: none"> <li>• If the specified advanced marker has not been assigned, a moving marker will be assigned.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:CALCulate:AMARKer[1|2|3|4]:MAXimum:**

#### **RIGHT**

Function	Detects the closest peak to the right of the current specified advanced marker position and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MAXimum :RIGHT [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MAXIMUM:RIGHT
Description	<ul style="list-style-type: none"> <li>• If the specified advanced marker has not been assigned, a moving marker will be assigned.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:CALCulate:AMARKer[1|2|3|4]:MINimum**

Function	Detects the bottom and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MINimum [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MINIMUM
Description	<ul style="list-style-type: none"> <li>• If the specified advanced marker has not been assigned, a moving marker will be assigned.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:CALCulate:AMARKer[1|2|3|4]:MINimum:**

#### **LEFT**

Function	Detects the closest bottom to the left of the current specified advanced marker position and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MINimum :LEFT [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MINIMUM:LEFT
Description	<ul style="list-style-type: none"> <li>• If the specified advanced marker has not been assigned, a moving marker will be assigned.</li> <li>• If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## 7.6 Instrument-Specific Commands

### :CALCulate:AMARKer[1|2|3|4]:MINimum:

#### NEXT

Function	Detects the lowest bottom whose level is greater than or equal to that of the current specified advanced marker position and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MINimum: :NEXT [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MINIMUM:NEXT

Description

- If the specified advanced marker has not been assigned, a moving marker will be assigned.
- If the advanced marker number is not specified, advanced marker 1 will be used.
- This is a sequential command.
- This command can be used on the AQ6370C/AQ6370D/AQ6373B.

### :CALCulate:AMARKer[1|2|3|4]:MINimum:

#### RIGHT

Function	Detects the closest bottom to the right of the current specified advanced marker position and sets the specified advanced marker there.
Syntax	:CALCulate:AMARKer[1 2 3 4]:MINimum: :RIGHT [1 2 3 4]: Advanced marker number
Example	:CALCULATE:AMARKER:MINIMUM:RIGHT

Description

- If the specified advanced marker has not been assigned, a moving marker will be assigned.
- If the advanced marker number is not specified, advanced marker 1 will be used.
- This is a sequential command.
- This command can be used on the AQ6370C/AQ6370D/AQ6373B.

### :CALCulate:AMARKer[1|2|3|4] [:STATE]

Function	Sets or queries whether the specified advanced marker is to be assigned.  Also queries the status of the specified moving marker.
Syntax	:CALCulate:AMARKer[1 2 3 4] [:STATE]<wsp>OFF ON 0 1 :CALCulate:AMARKer[1 2 3 4] [:STATE]? [1 2 3 4]: Advanced marker number Response 0 = Off, 1 = On
Example	:CALCULATE:AMARKER ON :CALCULATE:AMARKER? -> 1

Description

- If a moving marker is assigned, power density markers (:CALCulate:AMARKer[1|2|3|4]:UNCTION:PDENsity[:NOISE[:STATE]]) and integrated power markers (:CALCulate:AMARKer[1|2|3|4]:FUNCTION:INTEGRal[:STATE]) will be set to off.
- If the advanced marker number is not specified, advanced marker 1 will be used.

- This is a sequential command.
- This command can be used on the AQ6370C/AQ6370D/AQ6373B.

### :CALCulate:AMARKer[1|2|3|4]:TRACe

Function	Sets or queries the trace that the specified advanced marker is assigned to.
Syntax	:CALCulate:AMARKer[1 2 3 4]:TRACe<wsp><trace name> :CALCulate:AMARKer[1 2 3 4]:TRACe? [1 2 3 4]: Advanced marker number <trace name> = Trace TRA to TRG = Trace A to trace G
Example	:CALCULATE:AMARKER:TRACE TRA :CALCULATE:AMARKER:TRACE? -> TRA

Description

- Setting and querying are possible even when the specified advanced marker has not been assigned.
- If the advanced marker number is not specified, advanced marker 1 will be used.
- This is a sequential command.
- This command can be used on the AQ6370C/AQ6370D/AQ6373B.

### :CALCulate:AMARKer[1|2|3|4]:X

Function	Sets the specified advanced marker to the specified position.  Also queries the X value of the specified advanced marker.
Syntax	:CALCulate:AMARKer[1 2 3 4]:X<wsp><NRF>[M HZ] :CALCulate:AMARKer[1 2 3 4]:X? [1 2 3 4]: Advanced marker number <NRF> = Advanced marker position Response <NRF> = Advanced marker position
Example	:CALCULATE:AMARKER:X 1550.000nm :CALCULATE:AMARKER:X? -> +1.5500000E-006

Description

- The unit of the returned advanced marker X value depends on the :CALCulate:MARKer:UNIT setting.
- The unit of the returned advanced marker level depends on the :CALCulate:MARKer:UNIT setting.
- If this set command is used when the specified advanced marker has not been assigned, a moving marker will be assigned.
- If a query is made when the specified advanced marker has not been assigned, a query error will occur.
- If the advanced marker number is not specified, advanced marker 1 will be used.
- This is a sequential command.
- This command can be used on the AQ6370C/AQ6370D/AQ6373B.

## 7.6 Instrument-Specific Commands

	<b>:CALCulate:AMARKer[1 2 3 4]:Y?</b>
Function	Queries the Y value of the specified advanced marker.
Syntax	:CALCulate:AMARKer[1 2 3 4]:Y? [1 2 3 4]: Advanced marker number Response <NRF> = Advanced marker level
Example	:CALCULATE:AMARKER:X? -> -1.0000000E+001
Description	<ul style="list-style-type: none"> <li>The unit of the returned advanced marker level depends on the Y-axis unit of the assigned marker trace.</li> <li>Even if the advanced marker is an integrated power marker or power density marker, the moving marker level will be returned. The query does not return the integrated power value or the power density value.</li> <li>A query error will occur if the specified advanced marker has not been assigned.</li> <li>If the advanced marker number is not specified, advanced marker 1 will be used.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>
	<b>:CALCulate:ARESolution?</b>
Function	Queries the actual resolution data of the specified trace.
Syntax	:CALCulate:ARESolution?<wsp><trace name>,[<start point>,<stop point>] <trace name> Target trace (TRA TRB TRC TRD  TRE TRF TRG) <start point> Sample range to transfer (start point) (1 to 50001) <stop point> Sample range to transfer (stop point) (1 to 50001)
Example	CALCULATE:ARESOLUTION? -> +1.89759145E-009,+1.89744762E-009,+1.89730346E-009,....
Description	<ul style="list-style-type: none"> <li>The function outputs a wavelength value.</li> <li>If the &lt;start point&gt; and &lt;stop point&gt; parameters are omitted, the entire sample data of the specified trace will be output.</li> <li>The data is output in ASCII or BINARY format according to the :FORMAT[:DATA] setting.</li> <li>This command is for the AQ6370D.</li> <li>This is a sequential command.</li> </ul>

	<b>:CALCulate:CATegory</b>
Function	Sets/queries the type of analysis.
Syntax	:CALCulate:CATegory<wsp>{SWTHresh  SWENvelope SWRMs SWPKrms NOTCh  DFBLd FPLD LED SMSR POWer PMD OSNR  WDM NF FILPk FILBtm WFPeak WFBtm  COLor 0 1 2 3 4 5 6 7 8 9 10 11 12  13 14 15 16 17} :CALCulate:CATegory? SWTHresh 0 Spectrum width analysis (THRESH) SWENvelope 1 Spectrum width analysis (ENVELOPE) SWRMs 2 Spectrum width analysis (RMS) SWPKrms 3 Spectrum width analysis (PEAK-RMS) NOTCh 4 Notch width analysis DFBLd 5 DFB-LD parameter analysis FPLD 6 FP-LD parameter analysis LED 7 LED parameter analysis SMSR 8 SMSR analysis POWer 9 Power analysis PMD 10 PMD analysis OSNR WDM 11 OSNR(WDM), WDM analysis NF 12 NF analysis FILPk 13 Filter peak analysis FILBtm 14 Filter bottom analysis WFPeak 15 WDM FIL-PK analysis WFBtm 16 WDM FIL-BTM analysis COLor 17 Color analysis
Example	:CALCULATE:CATegory SWTHresh :CALCULATE:CATegory? -> 0
Explanation	<ul style="list-style-type: none"> <li>Even when this command is executed, no analysis is performed unless the CALCulate[:IMMEDIATE] command is executed.</li> <li>This is a sequential command.</li> <li>For the AQ6370C, the following parameters cannot be set. OSNR, COLor</li> <li>For the AQ6373/AQ6373B, the following parameters cannot be set. NF, WFPeak, WFBtm</li> <li>For the AQ6375, the following parameters cannot be set. OSNR, COLor</li> <li>For the AQ6375, when in Wavenumber mode, analysis functions included in ANALYSIS2 cannot be executed. The following parameters cannot be set. WDM, NF, FILPk, FILBtm, WFPeak, WFBtm</li> </ul>

**:CALCulate:DATA?**

**Function** Queries the analysis results.  
**Syntax** :CALCulate:DATA?  
**Example** :CALCULATE:DATA?  
**Explanation**

- Queries the analysis results from the last time analysis was executed.
- If the analysis function has not been executed, a query error occurs.
- For a response example, see section 7.7, "Output Format of Analysis Results."
- This is a sequential command.

**:CALCulate:DATA:CGAin?**

**Function** Queries the gain value of the EDFA-NF analysis results.  
**Syntax** :CALCulate:DATA:CGAin?  
**Example** :CALCULATE:DATA:CGAin?  
 $-> +1.00000000E+001,+1.00000000E+001$   
**Explanation**

- If the analysis function has not been executed, a query error occurs.
- "0" is returned if there is no relevant return value (such as if the analysis executed was not EDFA-NF analysis)
- The number of channels to be output can be acquired by the :CALCulate:DATA:NCHannels? command.
- Data is output in either ASCII or binary form, depending on the setting of :FORMAT[:DATA].
- With the AQ6373/AQ6373B, the command is invalid.
- This is a sequential command.

**:CALCulate:DATA:CNF?**

**Function** Queries the NF value of the EDFA-NF analysis results.  
**Syntax** :CALCulate:DATA:CNF?  
**Example** :CALCULATE:DATA:CNF?  $->$   
 $+1.00000000E+001,+1.00000000E+001$   
**Explanation**

- If :CALCulate[:IMMEDIATE] has not been executed, a query error occurs.
- "0" is returned if there is no relevant return value (such as if the analysis executed was not EDFA-NF analysis)
- The number of channels to be output can be acquired by the :CALCulate:DATA:NCHannels? command.
- Data is output in either ASCII or binary form, depending on the setting of :FORMAT[:DATA].
- With the AQ6373/AQ6373B, the command is invalid.
- This is a sequential command.

**:CALCulate:DATA:CPOWers?**

**Function** Queries the level value of the OSNR(WDM), WDM, EDFA-NF, WDM FIL-PK, or WDM FIL-BTM analysis results.  
**Syntax** :CALCulate:DATA:CPOWers?  
**Example** :CALCULATE:DATA:CPOWERS?  $->$   
 $+1.00000000E+001,+1.00000000E+001$   
**Explanation**

- If the analysis function has not been executed, a query error occurs.
- "0" is returned if there is no relevant return value.
- The number of channels to be output can be acquired by the :CALCulate:DATA:NCHannels? command.
- The value to be output depends on the analysis performed.

OSNR(WDM) : LEVEL or MEAS  
 WDM : LEVEL or MEAS LEVEL  
 EDFA-NF : INPUT LEVEL  
 WDM FIL-PK : PEAK LEVEL  
 (output even if SW is OFF)  
 WDM FIL-BTM: PEAK LEVEL  
 (output even if SW is OFF)

- Data is output in either ASCII or binary form, depending on the setting of :FORMAT[:DATA].
- This is a sequential command.

**:CALCulate:DATA:CSNR?**

**Function** Queries the SNR value from the last time WDM analysis was executed.  
**Syntax** :CALCulate:DATA:CSNR?  
**Example** :CALCULATE:DATA:CSNR?  $->$   
 $+4.00000000E+001,+4.00000000E+001$   
**Explanation**

- If the analysis function has not been executed, a query error occurs.
- "0" is returned if there is no relevant return value (for example, if analysis made is other than WDM analysis).
- The number of channels to be output can be acquired by the :CALCulate:DATA:NCHannels? command.
- Data is output in either ASCII or binary form, depending on the setting of :FORMAT[:DATA].
- This is a sequential command.

## 7.6 Instrument-Specific Commands

### **:CALCulate:DATA:CWAVelengths?**

Function	Queries the wavelength value of the OSNR(WDM), WDM, EDFA-NF, WDM FIL-PK, or WDM FIL-BTM analysis results.
Syntax	:CALCulate:DATA:CWAVelengths?
Example	:CALCULATE:DATA:CWAVELENGTHS? -> +1.5500000E-006,+1.5600000E-006
Explanation	<ul style="list-style-type: none"> <li>If the analysis function has not been executed, a query error occurs.</li> <li>"0" is returned if there is no relevant return value.</li> <li>The number of channels to be output can be acquired by the :CALCulate:DATA:NChannels? command.</li> <li>The value to be output depends on the analysis performed.</li> </ul> <p>OSNR(WDM): WAVELENGTH or MEAS WL      WDM : WAVELENGTH or MEAS WL      EDFA-NF: WAVELENGTH      WDM FIL-PK: NOMINAL WAVELENGTH      WDM FIL-BTM: NOMINAL WAVELENGTH</p> <ul style="list-style-type: none"> <li>Data is output in either ASCII or binary form, depending on the setting of :FORMat[:DATA].</li> <li>This is a sequential command.</li> </ul>

### **:CALCulate:DATA:DFBLd?**

Function	Queries the DFB-LD analysis results.
Syntax	:CALCulate:DATA:DFBLd?
Example	:CALCULATE:DATA:DFBLD? ->
Explanation	<ul style="list-style-type: none"> <li>If the :CALCulate:[IMMEDIATE] command has not been executed, a query error occurs.</li> <li>"0" is returned if there is no relevant return value (for example, if the analysis that was executed was not a DFB-LD analysis).</li> <li>This command returns analysis results that are not returned from the ":CALCulate:DATA?" command, such as the OSNR value. The following items are returned. The items are listed here as abbreviations. For the meaning of these abbreviations, see section 7.7.          &lt;peak wl&gt;,&lt;peak lvl&gt;,&lt;center wl&gt;,&lt;spec wd&gt;,&lt;smsr(L)&gt;,&lt;smsr(R)&gt;,&lt;mode ofst(L)&gt;,&lt;mode ofst(R)&gt;,&lt;snr&gt;,&lt;power&gt;,&lt;rms&gt;,&lt;Krms&gt;</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:CALCulate:DATA:NChannels?**

Function	Queries the number of channels of the OSNR(WDM), WDM, EDFA-NF, WDM FIL-PK, or WDM FIL-BTM analysis results.
Syntax	:CALCulate:DATA:NChannels?
Example	:CALCULATE:DATA:NCHANNELS? -> 16

Explanation

- If the analysis function has not been executed, a query error occurs.
- "0" is returned if there is no relevant return value.
- The value is output as ASCII data, regardless of the setting of FORMat[:DATA].
- This is a sequential command.

### **:CALCulate:DATA:OSlope?**

Function	Queries the OUTPUT SLOPE value of the OSNR (WDM) and WDM analysis results.
Syntax	:CALCulate:DATA:OSlope?
Example	Response <NRF> = Output slope value [dB/nm] or [dB/THz]
Explanation	<ul style="list-style-type: none"> <li>A query error will occur if the analysis function is not implemented.</li> <li>"0" is returned if there is no relevant return value (for example, if the analysis that was executed was not a WDM analysis).</li> <li>Analysis results can be queried even if the output of the OUTPUT SLOPE value is set to OFF.</li> <li>ASCII data is returned regardless of the setting specified by the :FORMAT[:DATA] command.</li> <li>This is a sequential command.</li> </ul>

### **:CALCulate:DISPlay**

Function	Sets/queries the display format of analysis results.
Syntax	:CALCulate:DISPlay<wsp>0 1 2 3 4 :CALCulate:DISPlay? 0: TRACE&TABLE 1: TABLE 2: TRACE 3: GRAPH&TABLE 4: GRAPH
Example	:CALCULATE:DISPLAY 1 :CALCULATE:DISPLAY? -> 1
Explanation	<ul style="list-style-type: none"> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:CALCulate:DISPlay:GRAPh:LMARker:Y**

Function	Sets/queries the position of line marker Y1 or Y2 on the graph display of analysis results.
Syntax	:CALCulate:DISPlay:GRAPh:LMARker:Y<wsp>1 2,<NRF>[DB] :CALCulate:DISPlay:GRAPh:LMARker:Y?<wsp>1 2 1: Line marker Y1. 2: Line marker Y2. <NRF>: Line marker position
Example	:CALCULATE:DISPLAY:GRAPH:LMARKER:Y 1,3.4 :CALCULATE:DISPLAY:GRAPH:LMARKER:Y? 1 -> +3.4000000E+000
Explanation	<ul style="list-style-type: none"> <li>This command is valid when the EDFA-NF analysis results are being displayed on a graph.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D.</li> </ul>

**:CALCulate[:IMMediate]**

Function	Executes analysis. Queries the result of whether analysis has been performed.
Syntax	:CALCulate[:IMMediate] :CALCulate[:IMMediate]?
	0: Not performed 1: Performed
Example	:CALCULATE :CALCULATE? -> 1
Explanation	<ul style="list-style-type: none"> <li>• Analysis is performed according to the latest analysis settings.</li> <li>• Analysis is performed on the following occasions:</li> <li>• When CALCulate[:IMMediate] command is executed.</li> <li>• When CALCulatePARameter: command is executed, or parameter settings changed</li> <li>• For the AQ6375, analysis functions included in ANALYSIS2 cannot be executed when in Wavenumber mode. The following parameters cannot be set.</li> <li>• This is a sequential command.</li> </ul>

**:CALCulate[:IMMediate]:AUTO**

Function	Sets/queries the automatic analysis function.
Syntax	:CALCulate[:IMMediate]:AUTO<wsp> OFF ON 0 1 :CALCulate[:IMMediate]:AUTO?
	0: OFF 1: ON
Example	:CALCULATE:AUTO ON :CALCULATE AUTO? -> 1
Explanation	<ul style="list-style-type: none"> <li>• When the automatic analysis function is ON, automatically activates an analysis function that is active after a sweep has ended.</li> <li>• This is a sequential command.</li> </ul>

**:CALCulate:LMARker:AOFF**

Function	Clears all line markers.
Syntax	:CALCulate:LMARker:AOFF
Explanation	This is a sequential command.

**:CALCulate:LMARker:SRANGE**

Function	Sets/queries whether to limit an analytical range to the spacing between line markers L1 and L2.
Syntax	:CALCulate:LMARker:SRANge<wsp>OFF  ON 0 1 :CALCulate:LMARker:SRANge?
	0: OFF 1: ON
Example	:CALCULATE:LMARKER:SRANGE ON :CALCULATE:LMARKER:SRANGE? -> 1
Explanation	This is a sequential command.

**:CALCulate:LMARker:SSPan**

Function	Sets spacing between line markers L1 and L2 for span.
Syntax	:CALCulate:LMARker:SSPan
Example	:CALCULATE:LMARKER:SSPAN
Explanation	This is a sequential command.

**:CALCulate:LMARker:SZSPan**

Function	Sets spacing between line markers L1 and L2 for zoom span.
Syntax	:CALCulate:LMARker:SZSPan
Example	:CALCULATE:LMARKER:SZSPAN
Explanation	This is a sequential command.

**:CALCulate:LMARker:X**

Function	Sets/queries the position of line markers L1 and L2.
Syntax	:CALCulate:LMARker:X<wsp>1 2,<NRf> [M Hz] :CALCulate:LMARker:X?<wsp>1 2 1, 2 = Line marker numbers <NRf> = Position of a line marker
	Response
	<NRf> [m Hz] (AQ6370C, AQ6373, AQ6373B) <NRf> [m Hz m <sup>-1</sup> ] (AQ6375)
Example	:CALCULATE:LMARKER:X 1,1550.000nm :CALCULATE:LMARKER:X? 1 -> +1.5500000E-006
Explanation	<ul style="list-style-type: none"> <li>• If the specified line marker is not located, a query error occurs.</li> <li>• For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value.</li> <li>• This is a sequential command.</li> </ul>

**:CALCulate:LMARker:Y**

Function	Sets/queries the position of line markers L3 and L4.
Syntax	:CALCulate:LMARker:Y<wsp>3 4,<NRf> [DBm DB %] :CALCulate:LMARker:Y?<wsp>3 4 3, 4 = Line marker numbers <NRf> = Position of a line marker
	Response
	<NRf> [dBm DB %]
Example	:CALCULATE:LMARKER:y 3,-10dBm :CALCULATE:LMARKER:y? 3 -> -1.0000000E+001
Explanation	<ul style="list-style-type: none"> <li>• If the specified line marker is not located, a query error occurs.</li> <li>• This is a sequential command.</li> </ul>

**:CALCulate:MARKer:AOFF**

Function	Clears all markers.
Syntax	:CALCulate:MARKer:AOFF
Example	:CALCULATE:MARKER:AOFF
Explanation	This is a sequential command.

## 7.6 Instrument-Specific Commands

### **:CALCulate:MARKer:AUTO**

Function	Sets/queries the auto search function.
Syntax	:CALCulate:MARKer:AUTO<wp> OFF ON 0 1 :CALCulate:MARKer:AUTO? 0 = OFF 1 = ON
Example	:CALCULATE:MARKER:AUTO ON :CALCULATE:MARKER:AUTO? -> 1
Explanation	<ul style="list-style-type: none"> <li>When the auto search function is ON, this instrument automatically performs a peak/bottom search through an active trace after a sweep has ended.</li> <li>This is a sequential command.</li> </ul>

### **:CALCulate:MARKer:FUNCTION:FORMAT**

Function	Sets the format of a difference value displayed in the area marker and queries the format set.
Syntax	:CALCulate:MARKer:FUNCTION:FORMAT<wp>OFFSET SPACing 0 1 :CALCulate:MARKer:FUNCTION:FORMAT? OFFSET = Displays the difference of each marker relative to the moving marker. SPACing = Displays the difference of each marker relative to a neighboring marker. Response 0 = OFFSET, 1 = SPACing
Example	:CALCULATE:MARKER:FUNCTION:FORMAT SPACING :CALCULATE:MARKER:FUNCTION:FORMAT?-> 1
Explanation	This is a sequential command.

### **:CALCulate:MARKer:FUNCTION:UPDATE**

Function	Sets/queries ON/OFF of the automatic update function of fixed markers used when updating an active trace.
Syntax	:CALCulate:MARKer:FUNCTION:UPDATE<wp>OFF ON 0 1 :CALCulate:MARKer:FUNCTION:UPDATE? Response 0 = OFF, 1 = ON
Example	:CALCULATE:MARKER:FUNCTION: UPDATE ON :CALCULATE:MARKER:FUNCTION:UPDATE? -> 1
Explanation	<ul style="list-style-type: none"> <li>When the automatic update function is ON and the active trace is updated, the level positions of fixed markers automatically follow the waveform.</li> <li>This is a sequential command.</li> </ul>

### **:CALCulate:MARKer:MAXimum**

Function	Detects a peak and places the moving marker on that peak.
Syntax	:CALCulate:MARKer:MAXimum
Example	:CALCULATE:MARKER:MAXIMUM

Explanation This is a sequential command.

### **:CALCulate:MARKer:MAXimum:LEFT**

Function	Detects the nearest peak existing on the left side of the current position of the moving marker and places the moving marker on that peak.
Syntax	:CALCulate:MARKer:MAXimum:LEFT
Example	:CALCULATE:MARKER:MAXIMUM:LEFT
Explanation	<ul style="list-style-type: none"> <li>If the moving marker is OFF, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

### **:CALCulate:MARKer:MAXimum:NEXT**

Function	Detects the highest peak that is below the level of the current position of the moving marker and places the moving marker on that peak.
Syntax	:CALCulate:MARKer:MAXimum:NEXT
Example	:CALCULATE:MARKER:MAXIMUM:NEXT

Explanation

- If the moving marker is OFF, an execution error occurs.
- This is a sequential command.

### **:CALCulate:MARKer:MAXimum:RIGHT**

Function	Detects the nearest peak existing on the right side of the current position of the moving marker and places the moving marker on that peak.
Syntax	:CALCulate:MARKer:MAXimum:RIGHT
Example	:CALCULATE:MARKER:MAXIMUM:RIGHT

Explanation

- If the moving marker is OFF, an execution error occurs.
- This is a sequential command.

### **:CALCulate:MARKer:MAXimum:SCENTER**

Function	Detects the peak wavelength and sets it as the measurement center waveform.
Syntax	:CALCulate:MARKer:MAXimum:SCenter
Example	:CALCULATE:MARKER:MAXIMUM:SCENTER

Explanation This is a sequential command.

### **:CALCulate:MARKer:MAXimum:SCENTER:AUTO**

Function	Sets/queries ON/OFF of the function to automatically detect the peak wavelength and set it as the measurement center wavelength.
Syntax	:CALCulate:MARKer:MAXimum:SCenter:AUTO<wp>OFF ON 0 1
Example	:CALCULATE:MARKer:MAXimum:SCenter:AUTO UTO ON :CALCULATE:MARKer:MAXimum:SCenter:AUTO? -> 1
Explanation	<ul style="list-style-type: none"> <li>When this function is ON, this instrument automatically detects the peak wavelength of an active trace wavelength each time a sweep has ended, and sets it as the measurement center wavelength.</li> <li>This is a sequential command.</li> </ul>

<b>:CALCulate:MARKer:MAXimum:SRLevel</b>	
Function	Detects the peak level and sets it for the reference level.
Syntax	:CALCulate:MARKer:MAXimum:SRLevel
Example	:CALCULATE:MARKER:MAXIMUM:SRLEVEL
Explanation	This is a sequential command.
<b>:CALCulate:MARKer:MAXimum:SRLevel:AUTO</b>	
Function	Sets/queries ON/OFF of the function to automatically detect the peak level and sets it as the reference level.
Syntax	:CALCulate:MARKer:MAXimum:SRLevel:AUTO<wsp>OFF ON 0 1 Response 0 = OFF, 1 = ON
Example	:CALCULATE:MARKER:MAXIMUM:SRLEVEL:AUTO ON CALCULATE:MARKER:MAXIMUM:SRLEVEL:AUTO? -> 1
Explanation	<ul style="list-style-type: none"> <li>When this function is ON, the instrument automatically detects the peak level of an active trace wavelength each time a sweep has ended, and sets it as the reference level.</li> <li>This is a sequential command.</li> </ul>
<b>:CALCulate:MARKer:MAXimum:SZCenter</b>	
Function	Detects the peak wavelength and sets it as the display center wavelength.
Syntax	:CALCulate:MARKer:MAXimum:SZCenter
Example	:CALCULATE:MARKER:MAXIMUM:SZCENTER
Explanation	This is a sequential command.
<b>:CALCulate:MARKer:MINimum</b>	
Function	Detects the bottom and places the moving marker on that bottom.
Syntax	:CALCulate:MARKer:MINimum
Example	:CALCULATE:MARKER:MINIMUM
Explanation	This is a sequential command.
<b>:CALCulate:MARKer:MINimum:LEFT</b>	
Function	Detects the nearest bottom existing on the left side of the current position of the moving marker and places the moving marker on that bottom.
Syntax	:CALCulate:MARKer:MINimum:LEFT
Example	:CALCULATE:MARKER:MINIMUM:LEFT
Explanation	<ul style="list-style-type: none"> <li>If the moving marker is OFF, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>
<b>:CALCulate:MARKer:MINimum:NEXT</b>	
Function	Detects the lowest bottom that is above the level of the current position of the moving marker and places the moving marker on that bottom.
Syntax	:CALCulate:MARKer:MINimum:NEXT
Example	:CALCULATE:MARKER:MINIMUM:NEXT
Explanation	<ul style="list-style-type: none"> <li>If the moving marker is OFF, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

<b>:CALCulate:MARKer:MINimum:RIGHT</b>	
Function	Detects the nearest bottom existing on the right side of the current position of the moving marker and places the moving marker on that side.
Syntax	:CALCulate:MARKer:MINimum:RIGHT
Example	:CALCULATE:MARKER:MINIMUM:RIGHT
Explanation	<ul style="list-style-type: none"> <li>If the moving marker is OFF, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>
<b>:CALCulate:MARKer:MSearch</b>	
Function	Sets/queries the type of the search function.
Syntax	:CALCulate:MARKer:MSearch<wsp> OFF ON 0 1 :CALCulate:MARKer:MSearch? OFF 0: Sets the search function to single search. ON 1: Sets the search function to multi search. Response 0 = OFF, 1 = ON
Example	:CALCULATE:MARKER:MSearch on :CALCULATE:MARKER:MSearch? -> 1
Explanation	<ul style="list-style-type: none"> <li>The search is executed as soon as you set the search function.</li> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D.</li> </ul>
<b>:CALCulate:MARKer:MSearch: SORT</b>	
Function	Sets/queries the sort order of the multi search detection list.
Syntax	:CALCulate:MARKer:MSearch: SORT<wsp> WAveLength LEVel 0 1 :CALCulate:MARKer:MSearch: SORT? WAveLength 0: Wavelengths are displayed in order starting from the shortest wavelength. LEVel 1: For the peak search, levels are displayed in order starting from the highest level. For the bottom search, levels are displayed in order starting from the lowest level. Response 0 = OFF, 1 = ON
Example	:CALCULATE:MARKER:MSearch: SORT WAV :CALCULATE:MARKER:MSearch: SORT? -> 0
Explanation	<ul style="list-style-type: none"> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## 7.6 Instrument-Specific Commands

### :CALCulate:MARKer:MSearch:THresh

Function	Sets/queries the multi search threshold.
Syntax	:CALCulate:MARKer:MSearch:THresh<wp> <NRf>[ DB] :CALCulate:MARKer:MSearch:THresh? <NRf>: Threshold (dB)
Example	:CALCULATE:MARKER:MSearch:THRESH 50DB :CALCULATE:MARKER:MSearch? -> +5.0000000E+001
Explanation	<ul style="list-style-type: none"> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### :CALCulate:MARKer:SCenter

Function	Sets the wavelength of the current moving marker as the measurement center waveform.
Syntax	:CALCulate:MARKer:SCenter
Example	:CALCULATE:MARKER:MINIMUM:SCENTER
Explanation	<ul style="list-style-type: none"> <li>If the moving marker is OFF, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:MARKer:SRLevel

Function	Sets the current level of the moving marker for the reference level.
Syntax	:CALCulate:MARKer:SRLevel
Example	:CALCULATE:MARKER:MINIMUM:SRLEVEL
Explanation	<ul style="list-style-type: none"> <li>If the moving marker is OFF, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:MARKer[:STATE]

Function	Specified marker is positioned or deleted in the position of the moving marker. Also, queries the status of the specified marker.
Syntax	:CALCulate:MARKer[:STATE]<wp><marker>,OFF ON 0 1:CALCulate:MARKer[:STATE]?<wp><marker> <marker>: Marker number (0: moving marker) Response 0 = OFF, 1 = ON
Example	:CALCULATE:MARKER:STATE 1,ON :CALCULATE:MARKER:STATE 1 -> 1
Explanation	<ul style="list-style-type: none"> <li>When the moving marker is not active and an attempt is made to set a fixed marker, an execution error occurs.</li> <li>If moving marker is specified, it is placed in the center of measurement display.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:MARKer:SZCenter

Function	Sets the current wavelength of the moving marker for the display center wavelength.
Syntax	:CALCulate:MARKer:SZCenter
Example	:CALCULATE:MARKER:SZCENTER
Explanation	<ul style="list-style-type: none"> <li>If the moving marker is OFF, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:MARKer:UNIT

Function	Sets/queries the units of display for the marker values.
Syntax	:CALCulate:MARKer:UNIT<wp>WAveleng th FREQuency 0 1 :CALCulate:MARKer:UNIT?
Parameter	AQ6370C, AQ6370D, AQ6373, AQ6373B
	WAveLength 0 FREQuency 1 AQ6375 WAveLength 0 FREQuency 1 WNUMber 2
Response	0=Wavelength, 1=FREQuency 2=WNUMber

Example	:CALCULATE:MARKER:UNIT FREQUENCY :CALCULATE:MARKER:UNIT? -> 1
---------	------------------------------------------------------------------

Explanation	<ul style="list-style-type: none"> <li>WNUMber is only valid for the AQ6375.</li> <li>This is a sequential command.</li> </ul>
-------------	--------------------------------------------------------------------------------------------------------------------------------

### :CALCulate:MARKer:X

Function	Places a specified marker in a specified position. Queries the X value of the specified marker.
Syntax	:CALCulate:MARKer:X<wp><marker>,<N Rf>[M HZ] :CALCulate:MARKer:X?<wp><marker>  ALL <marker> = Marker number (0: moving marker) ALL : All assigned markers <NRf>= Marker position
	Response
	<p>&lt;NRf&gt; [m Hz] (AQ6370C, / AQ6370D, AQ6373, AQ6373B)</p> <p>&lt;NRf&gt; [m   Hz]</p> <p>If &lt;marker&gt; is specified</p> <p>&lt;integer&gt;, &lt;NRf&gt;, &lt;NRf&gt;, ..., &lt;NRf&gt; (If ALL is specified)</p> <p>&lt;NRf&gt; [m Hz m<sup>-1</sup>] (AQ6375)</p>
Example	:CALCULATE:MARKER:X 0,1550.000nm :CALCULATE:MARKER:X? 0 -> +1.5500000E-006
Explanation	<ul style="list-style-type: none"> <li>If an already located marker is specified, that marker will be moved to a specified position.</li> <li>If the specified marker is not located, a query error occurs.</li> </ul>

	<ul style="list-style-type: none"> <li>If ALL is specified (e.g., :CALC:MARK:Y? ALL), the Y values of all assigned markers will be returned.</li> </ul> <p>The number of assigned markers will be returned as an integer, and then all the marker values will follow.</p> <ul style="list-style-type: none"> <li>For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value.</li> <li>This is a sequential command.</li> </ul>
	<b>:CALCulate:MARKer:Y?</b>
Function	Queries the Y value of the specified marker.
Syntax	<pre>:CALCulate:MARKer:Y?&lt;wsp&gt;&lt;marker&gt;   ALL &lt;marker&gt; : Marker number (0: moveing marker) ALL = All assigned markers If      &lt;marker&gt; is specified       &lt;NRf&gt;= Marker level If ALL is specified &lt;integer&gt;, &lt;NRf&gt;, &lt;NRf&gt;, ..., &lt;NRf&gt;</pre>
Example	<pre>:CALCULATE:MARKER:Y? 0 -&gt; -1.0000000E+001</pre>
Explanation	<ul style="list-style-type: none"> <li>This unit of the marker level to be queried is dependent on the Y-axis unit of the active trace.</li> <li>If the specified marker is not located, a query error occurs.</li> <li>If ALL is specified (e.g., :CALC:MARK:Y? ALL), the Y values of all assigned markers will be returned.</li> <li>This is a sequential command.</li> </ul>
	<b>:CALCulate:MATH:TRC</b>
Function	Sets/queries the TRACE C calculation function.
Syntax	<pre>:CALCulate:MATH:TRC&lt;wsp&gt;A-B (LOG)   B-A (LOG)   A+B (LOG)   A+B (LIN)   A-B (LIN)   B-A (LIN)   1-K (A/B)   1-K (B/A)   :CALCulate:MATH:TRC?</pre>
Example	<pre>:CALCULATE:MATH:TRC A-B (LOG) :CALCULATE:MATH:TRC? -&gt; A-B (LOG)</pre>
Explanation	<ul style="list-style-type: none"> <li>When the calculation function of trace C is set using this command, the attribute of trace C automatically becomes attribute "CALC".</li> <li>If trace C is not a calculation trace, "NONE" is returned.</li> <li>This is a sequential command.</li> </ul>

	<b>:CALCulate:MATH:TRC:K</b>
Function	Sets/queries parameter K of the TRACE C calculation function.
Syntax	<pre>:CALCulate:MATH:TRC:K&lt;wsp&gt;&lt;NRf&gt; :CALCulate:MATH:TRC:K? &lt;NRf&gt; = Parameter K</pre>
Example	<pre>:CALCULATE:MATH:TRC:K 0.1 :CALCULATE:MATH:TRC:K? -&gt; +1.0000000E-001</pre>
Explanation	This is a sequential command.
	<b>:CALCulate:MATH:TRF</b>
Function	Sets/queries the TRACE F calculation function.
Syntax	<pre>:CALCulate:MATH:TRF&lt;wsp&gt;C-D (LOG)   D-C (LOG)   C+D (LOG)   D-E (LOG)   E-D (LOG)   D+E (LOG)   C+D (LIN)   C-D (LIN)   D-C (LIN)   D+E (LIN)   D-E (LIN)   E-D (LIN)   PWRNBWA   PWRNBWB   PWRNBWC   PWRNBWD   PWRNBWE</pre>
Example	<pre>:CALCULATE:MATH:TRF? :CALCULATE:MATH:TRF C-D (LOG) :CALCULATE:MATH:TRF? -&gt; C-D (LOG)</pre>
Explanation	<ul style="list-style-type: none"> <li>When the calculation function of trace F is set using this command, the attribute of trace F automatically becomes attribute "CALC".</li> <li>If trace F is not a calculation trace, "NONE" is returned.</li> <li>Example calc:math:trf c-d(log) calc:math:trf? -&gt; C-D (LOG)</li> <li>PWRNBWA, PWRNBWB, PWRNBWC, PWRNBWD, and PWRNBWE are valid only for the AQ6370D.</li> <li>This is a sequential command.</li> </ul>
	<b>:CALCulate:MATH:TRF:PNBW:BWIDth   BANDwidth</b>
Function	Sets/queries the normalization bandwidth of the power density trace.
Syntax	<pre>:CALCulate:MATH:TRF:PNBW:BWIDth   BANDwidth&lt;wsp&gt;&lt;NRf&gt; [m] :CALCulate:MATH:TRF:PNBW:BWIDth   BANDwidth? &lt;NRf&gt;=Normalization bandwidth [mm]</pre>
Example	<pre>:CALCULATE:MATH:TRF:PNBW:BAND 0.1nm :CALCULATE:MATH:TRF:PNBW:BAND? -&gt; 1.0000000E-010</pre>
Explanation	<ul style="list-style-type: none"> <li>This command is for the AQ6370D.</li> <li>This is a sequential command.</li> </ul>

## 7.6 Instrument-Specific Commands

### :CALCulate:MATH:TRG

Function Sets/queries the TRACE G calculation function.

Syntax :CALCulate:MATH:TRG<wsp>C-F (LOG) |  
F-C (LOG) | C+F (LOG) | E-F (LOG) |  
F-E (LOG) | E+F (LOG) | C+F (LIN) |  
C-F (LIN) | F-C (LIN) | E+F (LIN) |  
E-F (LIN) | FLIN) | NORMA | NORMB | NORMC |  
CVFTA | CVFTB | CVFTC | MKRFT | PKCVFTA |  
PKCVFTB | PKCVFTC

:CALCulate:MATH:TRG?

Example :CALCULATE:MATH:TRG C-F (LOG)  
:CALCULATE:MATH:TRG? -> C-F (LOG)

Explanation • When the calculation function of trace G is set using this command, the attribute of trace G automatically becomes attribute "CALC".  
• If trace G is not a calculation trace, "NONE" is returned.  
• This is a sequential command.

### :CALCulate:MATH:TRG:CVFT:FALGo

Function Sets/queries the fitting curve function of the TRACE G fitting curve function.

Syntax :CALCulate:MATH:TRG:CVFT:FALGo  
<wsp><algorhythm>  
:CALCulate:MATH:TRG:CVFT:FALGo?  
<algorhythm>  
GAUSSs = GAUSS  
LORENz = LORENZ  
3RD = 3RD POLY  
4TH = 4TH POLY  
5TH = 5TH POLY

Response  
0 = GAUSS            1 = LORENZ,  
2 = 3RD POLY        3 = 4TH POLY  
4 = 5TH POLY

Example :CALCULATE:MATH:TRG:CVFT:  
FALGO GAUSS

Explanation • Setting of calculation area is common to curve fit and peak curve fit.  
• This is a sequential command.

### :CALCulate:MATH:TRG:CVFT:OPARea

Function Sets/queries a calculation area during curve fit and peak curve fit.

Syntax :CALCulate:MATH:TRG:CVFT:OPARea  
<wsp>ALL | INL1-L2 | OUTL1-L2 | 0 | 1 | 2

:CALCulate:MATH:TRG:CVFT:OPARea?

ALL = all of the set wavelength range

INL1-L2 = range surrounding line marker 1 and 2

OUTL1-L2 = range outside line markers 1 and 2

Response 0 = ALL, 1 = INL1-L2, 2 = OUTL1-L2

Example :CALCULATE:MATH:TRG:CVFT:  
OPAREA inl1-l2  
:CALCULATE:MATH:TRG:CVFT:OPAREA?->  
1

Explanation • Setting of calculation area is common to curve fit and peak curve fit.  
• This is a sequential command.

### :CALCulate:MATH:TRG:CVFT:THResh

Function Sets/queries the threshold value for curve fitting.

Syntax :CALCulate:MATH:TRG:CVFT:THResh  
<wsp><integer>[DB]  
:CALCulate:MATH:TRG:CVFT:THResh?  
<NRf> = Threshold level [dB]

Example :CALCULATE:MATH:TRG:CVFT:THRESH  
10db  
:CALCULATE:MATH:TRG:CVFT:THRESH?->  
10

Explanation This is a sequential command.

### :CALCulate:MATH:TRG:PCVFT:THResh

Function Sets/queries the threshold value for peak curve fitting.

Syntax :CALCulate:MATH:TRG:PCVFT:THResh  
<wsp><integer>[DB]  
:CALCulate:MATH:TRG:PCVFT:THResh?  
<NRf> = Threshold level [dB]

Example :CALCULATE:MATH:TRG:PCVFT:  
THRESH 10db  
:CALCULATE:MATH:TRG:PCVFT:THRESH?->  
10

Explanation This is a sequential command.

## 7.6 Instrument-Specific Commands

<b>:CALCulate:PARameter[:CATEgory]:DFB Ld</b>		
Function	Sets/queries parameters for the DFB-LD analysis function.	
Syntax	<pre>:CALCulate:PARameter[:CATEgory]:DFB Ld&lt;wsp&gt;&lt;item&gt;,&lt;parameter&gt;,&lt;data&gt; :CALCulate:PARameter[:CATEgory]:DFB Ld?&lt;wsp&gt;&lt;item&gt;,&lt;parameter&gt; &lt;item&gt; = Analytical item that sets parameter(s) &lt;parameter&gt; = Parameter to be set &lt;data&gt; = Setting data</pre>	
<b>&lt;item&gt; &lt;parameter&gt; &lt;data&gt;</b>		
SWIDth	ALGO	ENVelope THResh RMS  PKRMs
	TH	<NRF>[DB]
	TH2	<NRF>[DB]
	K	<NRF>
	MFIT	OFF ON 0 1
	MDIFF	<NRF>[DB]
SMSR	SMODE	SMSR1 SMSR2 SMSR3  SMSR4
	SMASK	<NRF>[M]
	MDIFF	<NRF>[DB]
RMS	ALGO	RMS PKRMs
	TH	<NRF>[DB]
	K	<NRF>
	MDIFF	<NRF> [DB]
POWer	SPAN	<NRF>[M]
OSNR	MDIFF	<NRF>[DB]
	NALGo	AFIX MFIX ACENTER  MCENTER PIT 0 1 2 3 4
	NARea	<NRF>[M]
	MARea	<NRF>[M]
	FALGo	LINEar GAUSS LORenz  3RD 4TH 5TH 0 1 2 3 4 5
	NBW	<NRF>[M]
	SPOWER	PEAK INTegral 0 1
	IRAnge	<NRF>

Example

```
:CALCULATE:PARAMETER:
DFBLD SWIDTH,ALGO,THRESH
:CALCULATE:PARAMETER:DFBLD? SWIDTH,
ALGO -> THR
:CALCULATE:PARAMETER:DFBLD
SMSR, SMASK, 0.5NM
:CALCULATE:PARAMETER:DFBLD?
SMSR, SMASK -> +5.0000000E-010
```

Explanation

- If a non-existing parameter is used for a combination, an execution error occurs. (such as combinations of SWIDth and SMODE)
- This is a sequential command.

<b>:CALCulate:PARameter[:CATEgory]:FILB tm</b>		
Function	Sets/queries parameters for the FILTER-BTM analysis function.	
Syntax	<pre>:CALCulate:PARameter[:CATEgory]:FIL Btm&lt;wsp&gt;&lt;item&gt;,&lt;parameter&gt;, &lt;data&gt; :CALCulate:PARameter[:CATEgory]:FIL Btm?&lt;wsp&gt;&lt;item&gt;,&lt;parameter&gt; &lt;item&gt; = Analytical item that sets parameter(s) &lt;parameter&gt; = Parameter to be set &lt;data&gt; = Data to be set</pre>	
<b>&lt;item&gt; &lt;parameter&gt; &lt;data&gt;</b>		
BLEVel	SW	OFF ON 0 1
BWAVelength	SW	OFF ON 0 1
CWAVelength	SW	OFF ON 0 1 ALGO PEAK BOTTom
	TH	<NRF>[DB]
	MDIFF	<NRF>[DB]
NWIDth	SW	OFF ON 0 1 ALGO PEAK BOTTom
	TH	<NRF>[DB]
	MDIFF	<NRF>[DB]
XTALK	SW	OFF ON 0 1 ALGO PEAK BOTTom  BLEVel GRID
	TH	<NRF>[DB]
	MDIFF	<NRF>[DB]
	CSPace	<NRF>[M]
	SARea	<NRF>[M]

Example

```
:CALCULATE:PARAMETER:FILBTM
CWAVELENGTH, ALGO, BOTTOM
:CALCULATE:PARAMETER:FILBTM
CWAVELENGTH, ALGO -> BOTT
:CALCULATE:PARAMETER:FILBTM
XTALK, CSPACE, 0.2NM
:CALCULATE:PARAMETER:FILBTM?
XTALK, CSPACEe -> +2.0000000E-010
```

Explanation

- If a non-existing parameter is used for a combination, an execution error occurs (a combination of CWAVelength and SARea, etc.).
- On the AQ6373/AQ6373B, the following data parameter cannot be set. GRID
- This is a sequential command.

## 7.6 Instrument-Specific Commands

:CALCulate:PARameter[:CATEgory]:FIL		
Pk		
Function	Sets/queries parameters for the FILTER PEAK analysis function.	
Syntax	<pre>:CALCulate:PARameter[:CATEgory]:FIL Pk&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt;,&lt;data&gt; :CALCulate:PARameter[:CATEgory]:FIL Pk?&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt; &lt;item&gt; = Analytical item that sets parameter(s) &lt;parameter&gt; = Parameter to be set &lt;data&gt; = Data to be set</pre>	
<item>	<parameter>	<data>
PLEvel	SW	OFF ON 0 1
PWAVelength	SW	OFF ON 0 1
MWAVelength	SW	OFF ON 0 1
	ALGO	THResh RMS
	TH	<NRF>[DB]
	K	<NRF>
	MFIT	OFF ON 0 1
	MDIFF	<NRF>[DB]
SWIDth	SW	OFF ON 0 1
	ALGO	THResh RMS
	TH	<NRF>[DB]
	K	<NRF>
	MFIT	OFF ON 0 1
	MDIFF	<NRF>[DB]
XTALK	SW	OFF ON 0 1
	ALGO	THResh PLEVel GRID
	TH	<NRF>[DB]
	K	<NRF>
	MFIT	OFF ON 0 1
	MDIFF	<NRF>[DB]
	CSPace	<NRF>[M]
	SARea	<NRF>[M]
RWIDth	SW	OFF ON 0 1
	TH	<NRF>[DB]
	MDIFF	<NRF>[DB]

Example	<pre>:CALCULATE:PARAMETER:FILPK SWIDTH,ALGO,THRESH :CALCULATE:PARAMETER:FILPK? SWIDTH,ALGO -&gt; THR :CALCULATE:PARAMETER:FILPK XTALK, CSPACE,0.5NM :CALCULATE:PARAMETER: FILPK? XTALK,CSPACE -&gt; +5.0000000E-010</pre>
Explanation	<ul style="list-style-type: none"> <li>If a non-existing parameter is used for a combination, an execution error occurs (a combination of SWIDth and CSPace, etc.).</li> <li>On the AQ6373, the following data parameter cannot be set. GRID</li> <li>This is a sequential command.</li> </ul>

:CALCulate:PARameter[:CATEgory]:FPLD																																																														
Function	Sets/queries parameters for the FP-LD analysis function.																																																													
Syntax	<pre>:CALCulate:PARameter[:CATEgory]:FPLD D&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt;,&lt;data&gt; :CALCulate:PARameter[:CATEgory]:FPLD D?&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt; &lt;item&gt; = Analytical item that sets parameter(s) &lt;parameter&gt; = Parameter to be set &lt;data&gt; = Setting data</pre>																																																													
	<table border="1"> <thead> <tr> <th>&lt;item&gt;</th><th>&lt;parameter&gt;</th><th>&lt;data&gt;</th></tr> </thead> <tbody> <tr> <td>SWIDth</td><td>ALGO</td><td>ENVelope THResh  RMS PKRMs</td></tr> <tr> <td></td><td>TH</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td></td><td>TH2</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td></td><td>K</td><td>&lt;NRF&gt;</td></tr> <tr> <td></td><td>MFIT</td><td>OFF ON 0 1</td></tr> <tr> <td></td><td>MDIFF</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td>MWAVelength</td><td>ALGO</td><td>ENVelope THResh  RMS PKRMs</td></tr> <tr> <td></td><td>TH</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td></td><td>TH2</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td></td><td>K</td><td>&lt;NRF&gt;</td></tr> <tr> <td></td><td>MFIT</td><td>OFF ON 0 1</td></tr> <tr> <td></td><td>MDIFF</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td>TPOWer</td><td>OFFSET</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td>MNUMber</td><td>ALGO</td><td>ENVelope THResh  RMS PKRMs</td></tr> <tr> <td></td><td>TH</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td></td><td>TH2</td><td>&lt;NRF&gt;[DB]</td></tr> <tr> <td></td><td>K</td><td>&lt;NRF&gt;</td></tr> <tr> <td></td><td>MFIT</td><td>OFF ON 0 11</td></tr> <tr> <td></td><td>MDIFF</td><td>&lt;NRF&gt;[DB]</td></tr> </tbody> </table>		<item>	<parameter>	<data>	SWIDth	ALGO	ENVelope THResh  RMS PKRMs		TH	<NRF>[DB]		TH2	<NRF>[DB]		K	<NRF>		MFIT	OFF ON 0 1		MDIFF	<NRF>[DB]	MWAVelength	ALGO	ENVelope THResh  RMS PKRMs		TH	<NRF>[DB]		TH2	<NRF>[DB]		K	<NRF>		MFIT	OFF ON 0 1		MDIFF	<NRF>[DB]	TPOWer	OFFSET	<NRF>[DB]	MNUMber	ALGO	ENVelope THResh  RMS PKRMs		TH	<NRF>[DB]		TH2	<NRF>[DB]		K	<NRF>		MFIT	OFF ON 0 11		MDIFF	<NRF>[DB]
<item>	<parameter>	<data>																																																												
SWIDth	ALGO	ENVelope THResh  RMS PKRMs																																																												
	TH	<NRF>[DB]																																																												
	TH2	<NRF>[DB]																																																												
	K	<NRF>																																																												
	MFIT	OFF ON 0 1																																																												
	MDIFF	<NRF>[DB]																																																												
MWAVelength	ALGO	ENVelope THResh  RMS PKRMs																																																												
	TH	<NRF>[DB]																																																												
	TH2	<NRF>[DB]																																																												
	K	<NRF>																																																												
	MFIT	OFF ON 0 1																																																												
	MDIFF	<NRF>[DB]																																																												
TPOWer	OFFSET	<NRF>[DB]																																																												
MNUMber	ALGO	ENVelope THResh  RMS PKRMs																																																												
	TH	<NRF>[DB]																																																												
	TH2	<NRF>[DB]																																																												
	K	<NRF>																																																												
	MFIT	OFF ON 0 11																																																												
	MDIFF	<NRF>[DB]																																																												

Example	<pre>:CALCULATE:PARAMETER:FPLD SWIDTH,ALGO,THRESH :CALCULATE:PARAMETER:FPLD? SWIDTH,ALGO -&gt; THR :CALCULATE:PARAMETER:FPLD TPOWER, OFFSET,1.0DB :CALCULATE:PARAMETER: FPLD? TPOWER,OFFSET -&gt; +1.0000000E+000</pre>
Explanation	<ul style="list-style-type: none"> <li>If a non-existing parameter is used for a combination, an execution error occurs (a combination of SWIDth and OFFSET, etc.).</li> <li>This is a sequential command.</li> </ul>

<b>:CALCulate :PARameter [:CATEgory] :LED</b>		
Function	Sets/queries parameters for the LED analysis function.	
Syntax	<pre>:CALCulate:PARameter[:CATEgory]:LED &lt;wsp&gt;&lt;item&gt;,&lt;parameter&gt;,&lt;data&gt; :CALCulate:PARameter[:CATEgory]:LED ?&lt;wsp&gt;&lt;item&gt;,&lt;parameter&gt; &lt;item&gt; = Analytical item that sets parameter(s) &lt;parameter&gt; = Parameter to be set &lt;data&gt; = Setting data</pre>	
<item>	<parameter>	<data>
SWIDth	ALGO	ENVelope THResh  RMS PKRMs TH TH2 K MFIT MDIFF
MWAvavelength	ALGO	ENVelope THResh  RMS PKRMs TH TH2 K MFIT MDIFF
TPOWER	OFFSet	<NRf>[DB]

Example    :CALCULATE:PARAMETER:LED  
SWIDTH, ALGO, THRESHh  
:CALCULATE:PARAMETER:LED?  
SWIDTH, ALGO -> THR  
:CALCULATE:PARAMETER:LED TPOWER,  
OFFSET, 1.0DB :CALCULATE:PARAMETER:  
LED? TPOWER, OFFSET ->  
+1.00000000E+000

Explanation • If a non-existing parameter is used for a combination, an execution error occurs (a combination of SWIDth and OFFSet, etc.).  
• This is a sequential command.

**:CALCulate :PARameter [:CATEgory] :NF:A****ALGo**

Function    Sets/queries the measurement algorithm applied to ASE level measurements made by the NF analysis function.

Syntax    :CALCulate:PARameter[:CATEgory]:NF:
AALGo<wsp><algorhytthm>
:CALCulate:PARameter[:CATEgory]:NF:
AALGo?

<algorhytthm> = Measurement algorithm

AFIX: AUTO FIX

MFIX: MANUAL FIX

ACENTER: AUTO CENTER

MCENTER: MANUAL CENTER

Response 0 = AUTO FIX

1 = MANUAL FIX

2 = AUTO CENTER

3 = MANUAL CENTER

Example    :CALCULATE:PARAMETER:NF:AALGO MFIX
:CALCULATE:PARAMETER:NF:AALGO? -> 1

Explanation • With the AQ6373/AQ6373B, the command is invalid.  
• This is a sequential command.

**:CALCulate :PARameter [:CATEgory] :NF:F****ALGo**

Function    Sets/queries the fitting function during level measurement applied to ASE level measurements made by the NF analysis function.

Syntax    :CALCulate:PARameter[:CATEgory]:NF:
FALGo<wsp><algorhytthm>
:CALCulate:PARameter[:CATEgory]:NF:
FALGo?

<algorhytthm> = Fitting function

LINear: LINEAR

GAUss: GAUSS

LOREnz: LORENZ

3RD: 3RD POLY

4TH: 4YH POLY

5TH: 5TH POLY

Response 0 =LINEAR

1 = GAUSS

2 = LORENZ

3 = 3RD POLY

4 = 4YH POLY

5 = 5TH POLY

Example    :CALCULATE:PARAMETER:NF:FALGO GAUSS
:CALCULATE:PARAMETER:NF:FALGO? -> 1

Explanation • With the AQ6373/AQ6373B, the command is invalid.  
• This is a sequential command.

## 7.6 Instrument-Specific Commands

<b>:CALCulate:PARameter[:CATEgory]:NF:F ARea</b>		<b>:CALCulate:PARameter[:CATEgory]:NF:M DIFF</b>	
Function	Sets/queries the fitting range for level measurement applied to ASE level measurements made by the NF analysis function.	Function	Sets/queries the peak bottom difference of channel detection for the NF analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:NF:F ARea<wsp><NRf>[M] :CALCulate:PARameter[:CATEgory]:NF: FARea? <NRf> = fitting range [m]	Syntax	:CALCulate:PARameter[:CATEgory]:NF: MDIFF<wsp><NRf>[DB] :CALCulate:PARameter[:CATEgory]:NF: MDIFF? <NRf> = Peak bottom difference [dB]
Example	:CALCULATE:PARAMETER:NF: FAREA 0.80NM :CALCULATE:PARAMETER:NF:FAREA? -> +8.0000000E-10	Example	:CALCULATE:PARAMETER:NF: MDIFF 3.00DB :CALCULATE:PARAMETER:NF:MDIFF? -> +3.0000000E+000
Explanation	<ul style="list-style-type: none"> <li>When the fitting range is set to “Between CH” (and ASE measurement algorithm is set to “AUTO-CTR” or “MANUAL-CTR”), then the command returns 0.</li> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>	Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>
<b>:CALCulate:PARameter[:CATEgory]:NF:I OFFset</b>		<b>:CALCulate:PARameter[:CATEgory]:NF:O FFset</b>	
Function	Sets/queries level offset values (signal light) for the NF analysis function.	Function	Sets/queries level offset values (output light) for the NF analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:NF: IOFFset<wsp><NRf>[DB] :CALCulate:PARameter[:CATEgory]:NF: IOFFset? <NRf> = Level offset value of signal light [dB]	Syntax	:CALCulate:PARameter[:CATEgory]:NF: OOFFset<wsp><NRf>[DB] :CALCulate:PARameter[:CATEgory]:NF: OOFFset? <NRf> = Level offset value of output light [dB]
Example	:CALCULATE:PARAMETER:NF: IOFFSET 10.00 :CALCULATE:PARAMETER:NF:IOFFSET? -> +1.0000000E+001	Example	:CALCULATE:PARAMETER:NF: OOFFSET 10.00 :CALCULATE:PARAMETER:NF:OOFFSET? -> +1.0000000E+001
Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>	Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>
<b>:CALCulate:PARameter[:CATEgory]:NF:M ARea</b>		<b>:CALCulate:PARameter[:CATEgory]:NF:P DIStplay</b>	
Function	Sets/queries the mask range for level measurement applied to ASE level measurements made by the NF analysis function.	Function	Sets/queries whether to display data used for fitting of the NF analysis function on the waveform screen.
Syntax	:CALCulate:PARameter[:CATEgory]:NF: MAREa<wsp><NRf>[M] :CALCulate:PARameter[:CATEgory]:NF: MAREa? <NRf> = mask range [m]	Syntax	:CALCulate:PARameter[:CATEgory]:NF: PDISplay<wsp>OFF ON 0 1 :CALCulate:PARameter[:CATEgory]:NF: PDISplay? Response 0 = OFF, 1 = ON
Example	:CALCULATE:PARAMETER:NF: MAREA 0.40NM :CALCULATE:PARAMETER:NF:MAREA? -> +4.0000000E-10	Example	:CALCULATE:PARAMETER:NF:PDISPLAY ON :CALCULATE:PARAMETER:NF:PDISPLAY?-> 1
Explanation	<ul style="list-style-type: none"> <li>When the mask range is set to “---” (and ASE level measurement function is set to “LINEAR”), the command returns 0.</li> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>	Explanation	<ul style="list-style-type: none"> <li>When this set value is 1 (ON), data used for fitting is displayed on the waveform screen.</li> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>

## 7.6 Instrument-Specific Commands

<b>:CALCulate:PARameter[:CATEgory]:NF:TH</b>							
Function	Sets/queries the threshold level of channel detection for the NF analysis function.						
Syntax	:CALCulate:PARameter[:CATEgory]:NF:TH<wsp><NRf> [DB] :CALCulate:PARameter[:CATEgory]:NF:TH? <NRf> = Threshold level [dB]						
Example	:CALCULATE:PARAMETER:NF:TH 20.00DB :CALCULATE:PARAMETER:NF:TH-> +2.0000000E+001						
Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>						
<b>:CALCulate:PARameter[:CATEgory]:NF:RBWidth</b>							
Function	Sets/queries the method for calculating the resolution value of the NF computation.						
Syntax	:CALCulate:PARameter[:CATEgory]:NF:RBWidth<wsp>MEASured CAL 0 1 :CALCulate:PARameter[:CATEgory]:NF:RBWidth?						
Example	<table> <tr> <td>MEASured   0</td><td>Use the value determined from the waveform using THRESH 3dB analysis.</td></tr> <tr> <td>CAL   1</td><td>Use the actual resolution value stored in the instrument.</td></tr> <tr> <td>Response</td><td>0=MEASURED, 1=CAL</td></tr> </table> <pre>:CALCULATE:PARAMETER:NF:RBWIDTH MEASURED :CALCULATE:PARAMETER:NF:RBWIDTH? -&gt; 0</pre>	MEASured   0	Use the value determined from the waveform using THRESH 3dB analysis.	CAL   1	Use the actual resolution value stored in the instrument.	Response	0=MEASURED, 1=CAL
MEASured   0	Use the value determined from the waveform using THRESH 3dB analysis.						
CAL   1	Use the actual resolution value stored in the instrument.						
Response	0=MEASURED, 1=CAL						
Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>						
<b>:CALCulate:PARameter[:CATEgory]:NF:SNoise</b>							
Function	Sets/queries whether Shot Noise is included in the NF computation						
Syntax	:CALCulate:PARameter[:CATEgory]:NF:SNoise<wsp>OFF ON 0 1 :CALCulate:PARameter[:CATEgory]:NF:SNoise?						
Example	<table> <tr> <td>OFF   0</td><td>Shot Noise not included in the NF computation</td></tr> <tr> <td>ON   1</td><td>Shot Noise included in the NF computation</td></tr> <tr> <td>Response</td><td>0=OFF, 1=ON</td></tr> </table> <pre>:CALCULATE:PARAMETER:NF:SNOISE OFF :CALCULATE:PARAMETER:NF:SNOISE?-&gt; 0</pre>	OFF   0	Shot Noise not included in the NF computation	ON   1	Shot Noise included in the NF computation	Response	0=OFF, 1=ON
OFF   0	Shot Noise not included in the NF computation						
ON   1	Shot Noise included in the NF computation						
Response	0=OFF, 1=ON						
Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>This is a sequential command.</li> </ul>						

<b>:CALCulate:PARameter[:CATEgory]:NOTCH:K</b>	
Function	Sets/queries the magnification of the notch width analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:NOTCH:K<wsp><NRf> [DB] :CALCulate:PARameter[:CATEgory]:NOTCH:K? <NRf> = Magnification
Example	:CALCULATE:PARAMETER:NOTCH:K 2.00 :CALCULATE:PARAMETER:NOTCH:K?-> +2.0000000E+000
Explanation	This is a sequential command.
<b>:CALCulate:PARameter[:CATEgory]:NOTCH:TH</b>	
Function	Sets/queries the threshold value for the notch width analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:NOTCH:TH<wsp><NRf> [DB] :CALCulate:PARameter[:CATEgory]:NOTCH:TH? <NRf> = Threshold level [dB]
Example	:CALCULATE:PARAMETER:NOTCH:TH 3.00DB :CALCULATE:PARAMETER:NOTCH:TH?-> +3.0000000E+000
Explanation	This is a sequential command.
<b>:CALCulate:PARameter[:CATEgory]:NOTCH:TYPE</b>	
Function	Sets/queries the analysis direction of the notch width analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:NOTCH:TYPE<wsp>PEAK BOTTOM 0 1 :CALCulate:PARameter[:CATEgory]:NOTCH:TYPE? PEAK: Performs analysis using the peak level of a waveform as a reference. BOTTOM: Performs analysis using the bottom level of a waveform as a reference.
Example	:CALCULATE:PARAMETER:NOTCH:TYPE BOTTOM :CALCULATE:PARAMETER:NOTCH:TYPE? -> 1
Explanation	This is a sequential command.
<b>:CALCulate:PARameter[:CATEgory]:PMD:TH</b>	
Function	Sets/queries the threshold value for the PMD analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:PMD:TH<wsp><NRf> [DB] :CALCulate:PARameter[:CATEgory]:PMD:TH? <NRf> = Threshold level [dB]
Explanation	:CALCULATE:PARAMETER:PMD:TH 10.00DB :CALCULATE:PARAMETER:PMD:TH?-> +1.0000000E+001

## 7.6 Instrument-Specific Commands

### :CALCulate:PARameter[:CATEgory]:POWe r:OFFSet

**Function** Sets/queries the offset value for the POWER analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:POWER:OFFSet<wsp><NRf>[DB]  
:CALCulate:PARameter[:CATEgory]:POWER:OFFSet?  
<NRf> = Offset value [dB]

**Example** :CALCULATE:PARAMETER:POWER:  
OFFSET 1.00DB  
:CALCULATE:PARAMETER:POWER:OFFSET?->  
+1.0000000E+000

### :CALCulate:PARameter[:CATEgory]:SMSR

#### :MASK

**Function** Sets/queries the mask value for the SMSR analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SMSR:MASK<wsp><NRf>[M]  
:CALCulate:PARameter[:CATEgory]:SMSR:MASK?  
<NRf> = Mask value [m]

**Example** :CALCULATE:PARAMETER:SMSR:  
MASK 2.0nm  
:CALCULATE:PARAMETER:SMSR:MASK ?->  
+2.0000000E-009

### :CALCulate:PARameter[:CATEgory]:SMSR

#### :MODE

**Function** Sets/queries the analysis mode for the SMSR analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SMSR:MODE<wsp>SMSR1|SMSR2|SMSR3|SMSR4  
:CALCulate:PARameter[:CATEgory]:SMSR:MODE?  
<NRf> = Mode

**Example** :CALCULATE:PARAMETER:SMSR:  
MODE SMSR1  
:CALCULATE:PARAMETER:SMSR:MODE?->  
SMSR1

### :CALCulate:PARameter[:CATEgory]:SWEN velope:K

**Function** Sets/queries the magnification of the ENVELOPE method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWENvelope:K  
:CALCulate:PARameter[:CATEgory]:SWENvelope:K?  
<NRf> = Magnification

**Example** :CALCULATE:PARAMETER:SWENVELOPE:  
K 2.00  
:CALCULATE:PARAMETER:SWENVELOPE:K?  
-> +2.0000000E+000

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWEN velope:TH1

**Function** Sets/queries the search threshold level of the ENVELOPE method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWENvelope:TH1<wsp><NRf>[DB]  
:CALCulate:PARameter[:CATEgory]:SWENvelope:TH1?  
<NRf> = Search threshold level [dB]

**Example** :CALCULATE:PARAMETER:SWENVELOPE:  
TH1 3.00  
:CALCULATE:PARAMETER:SWENVELOPE:  
TH1?-> +3.0000000E+000

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWEN velope:TH2

**Function** Sets/queries the threshold level of the ENVELOPE method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWENvelope:TH2<wsp><NRf>[DB]  
:CALCulate:PARameter[:CATEgory]:SWENvelope:TH2?  
<NRf> = Threshold level [dB]

**Example** :CALCULATE:PARAMETER:SWENVELOPE:  
TH2 10.00db  
:CALCULATE:PARAMETER:SWENVELOPE:  
TH2?-> +1.0000000E+001

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWPK rms:K

**Function** Sets/queries the magnification of the PEAK-RMS method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWPKrms:K<wsp><NRf>[DB]  
:CALCulate:PARameter[:CATEgory]:SWPKrms:K?  
<NRf> = Magnification

**Example** :CALCULATE:PARAMETER:SWPKRMS:K 2.00  
:CALCULATE:PARAMETER:SWPKRMS:K?->  
+2.0000000E+000

**Explanation** This is a sequential command.

## 7.6 Instrument-Specific Commands

### :CALCulate:PARameter[:CATEgory]:SWPK rms:TH

**Function** Sets/queries the threshold level of the PEAK-RMS method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWP  
Krms:TH<wsp><NRF>[DB]  
:CALCulate:PARameter[:CATEgory]:SWP  
Krms:TH?  
<NRF> = Threshold level [dB]

**Example** :CALCULATE:PARAMETER:SWPKRMS:  
TH 3.00db  
:CALCULATE:PARAMETER:SWPKRMS:TH?->  
+3.0000000E+000

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWRM s:K

**Function** Sets/queries the magnification of the RMS method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWR  
MS:K<wsp><NRF>[DB]  
:CALCulate:PARameter[:CATEgory]:SWR  
MS:K?  
<NRF> = Magnification

**Example** :CALCULATE:PARAMETER:SWRMS:K2.00  
:CALCULATE:PARAMETER:SWRMS:K? ->  
+2.0000000E+000

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWRM s:TH

**Function** Sets/queries the threshold level of the RMS method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWR  
MS:TH<wsp><NRF>[DB]  
:CALCulate:PARameter[:CATEgory]:SWR  
MS:TH?  
<NRF> = Threshold level [dB]

**Example** :CALCULATE:PARAMETER:SWRMS:  
TH 3.00db  
:CALCULATE:PARAMETER:SWRMS:TH?->  
+3.0000000E+000

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWTH

#### Resh:K

**Function** Sets/queries the magnification of the THRESH method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWT  
HResh:K<wsp><NRF>  
:CALCulate:PARameter[:CATEgory]:SWT  
HResh:K?  
<NRF> = Magnification

**Example** :CALCULATE:PARAMETER:SWTHRESH:  
K 2.00  
:CALCULATE:PARAMETER:SWTHRESH:K?->  
+2.0000000E+000

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWTH resh:MFIT

**Function** Sets/queries whether to enable the mode fit of the THRESH method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWT  
Hresh:MFIT<wsp>OFF|ON|0|1  
:CALCulate:PARameter[:CATEgory]:SWT  
Hresh:MFIT?  
Response 0 = OFF, 1 = ON

**Example** :CALCULATE:PARAMETER:SWTHRESH:  
MFIT ON  
:CALCULATE:PARAMETER:SWTHRESH:MF  
IT?-> 1

**Explanation** This is a sequential command.

### :CALCulate:PARameter[:CATEgory]:SWTH resh:TH

**Function** Sets/queries the threshold level of the THRESH method-based spectrum width analysis function.

**Syntax** :CALCulate:PARameter[:CATEgory]:SWT  
Hresh:TH<wsp><NRF>[DB]  
:CALCulate:PARameter[:CATEgory]:SWT  
Hresh:TH?  
<NRF> = Threshold level [dB]  
Response ex. Same as above

**Example** :CALCULATE:PARAMETER:SWTHRESH:  
TH 3.00DB  
:CALCULATE:PARAMETER:SWTHRESH:TH?->  
+3.0000000E+000

**Explanation** This is a sequential command.

## 7.6 Instrument-Specific Commands

<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>DMASK</b>	<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>
Function	Sets/queries the channel mask threshold level for the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :DMASK<wsp><NRf>[DB] :CALCulate:PARameter[:CATEgory]:WDM :DMASK? <NRf> = Threshold level [dB] (-999: Mask OFF)
Example	:CALCULATE:PARAMETER:WDM:DMASK -999 :CALCULATE:PARAMETER:WDM:DMASK? -> -9.9900000E+002
Explanation	<ul style="list-style-type: none"> <li>• Channels the level of which are below this parameter will not be detected as a channel.</li> <li>• To turn off the channel mask function, set the threshold level to -999.</li> <li>• This is a sequential command.</li> </ul>
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>DTYPE</b>	<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>
Function	Sets/queries the displayed waveforms of the analysis results for the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :DTPe<wsp><display type> :CALCulate:PARameter[:CATEgory]:WDM :DTPe? <display type>=Type of display ABSolute = Absolute value display RELative = Relative value display MDRift = Drift value display based on the past measurement wavelength GDRift = Drift value display based on the grid wavelength
Response	<ul style="list-style-type: none"> <li>0 = Absolute value display</li> <li>1 = Relative value display</li> <li>2 = Display drift value using previously measured waveforms as a reference</li> <li>3 = Display drift value using grid wavelength as a reference</li> </ul>
Example	:CALCULATE:PARAMETER:WDM:DTYPE:ABSO LUTE :CALCULATE:PARAMETER:WDM:DTYPE:ABSO LUTE? -> 0
Explanation	<ul style="list-style-type: none"> <li>• On the AQ6373/AQ6373B, the following display types cannot be set. GDRift, RELative</li> <li>• This is a sequential command.</li> </ul>
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>DUAL</b>	<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>
Function	Sets/queries the SNR calculation mode for the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :DUAL<wsp>OFF ON 0 1 :CALCulate:PARameter[:CATEgory]:WDM :DUAL? Response 0 = OFF, 1 = ON
Example	:CALCULATE:PARAMETER:WDM:DUAL ON :CALCULATE:PARAMETER:WDM:DUAL ON? -> 1
Explanation	<ul style="list-style-type: none"> <li>• When this set value is 1 (ON), SNR calculation uses both traces A and B data.</li> <li>• When this set value is 0 (OFF), SNR calculation uses active trace data.</li> <li>• This is a sequential command.</li> </ul>
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>FALGo</b>	<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>
Function	Sets/queries the fitting function during level measurement applied to noise level measurements made by the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :FALGo<wsp><algorhythm> :CALCulate:PARameter[:CATEgory]:WDM :FALGo? LINEar = LINEAR GAUSSs = GAUSS LOREnz = LORENZ 3RD = 3RD POLY 4TH = 4YH POLY 5TH = 5TH POLY Response 0 = LINEAR 1 = GAUSS 2 = LORENZ 3 = 3RD POLY 4 = 4YH POLY 5 = 5TH POLY
Example	CALCULATE:PARAMETER:WDM:FALGO GAUSS :CALCULATE:PARAMETER:WDM:FALGO? -> 1
Explanation	This is a sequential command.

## 7.6 Instrument-Specific Commands

<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>IRANge</b>	
Function	Sets/queries the integral frequency range during signal light power calculation by the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :IRANge<wsp><NRf> :CALCulate:PARameter[:CATEgory]:WDM :IRANge? <NRf> Integral frequency range [GHz]
Example	calc:par:wdm:iran 40 calc:par:wdm:iran? -> +4.0000000E+001
Explanation	<ul style="list-style-type: none"> <li>With the AQ6375, the command is invalid.</li> <li>This is a sequential command.</li> </ul>
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>MARea</b>	
Function	Sets/queries the mask range during level measurement applied to noise level measurements made by the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :MARea<wsp><NRf>[M] :CALCulate:PARameter[:CATEgory]:WDM :MARea?
Example	:CALCULATE:PARAMETER:WDM: MAREA 0.40NM :CALCULATE:PARAMETER:WDM:MAREA? -> +4.0000000E-10
Explanation	This is a sequential command.
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>MDIFF</b>	
Function	Sets/queries the peak bottom difference of channel detection for the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :MDIFF<wsp><NRf>[DB] :CALCulate:PARameter[:CATEgory]:WDM :MDIFF? <NRf> = Peak bottom difference [dB]
Example	:CALCULATE:PARAMETER:WDM: MDIFF 3.00DB :CALCULATE:PARAMETER:WDM:MDIFF
Explanation	This is a sequential command.
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>MMReset</b>	
Function	Resets the maximum and minimum of the drift values of the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :MMReset
Example	:CALCULATE:PARAMETER:WDM:MMRESET
Explanation	<ul style="list-style-type: none"> <li>When "DISPLAY TYPE" (set by the :CALCu late:PARameter[:CATEgory]:WDM:DTYPE command is set to other than "DRIFT", an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>NALGo</b>	
Function	Sets/queries the measurement algorithm applied to noise level measurements made by the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :NALGo<wsp><algorhythm> :CALCulate:PARameter[:CATEgory]:WDM :NALGo? AFIX 0 = AUTO FIX MFIX 1 = MANUAL FIX ACENTER 2 = AUTO CENTER MCENTER 3 = MANUAL CENTER PIT 4 = PIT
Response	0 = AUTO FIX 1 = MANUAL FIX 2 = AUTO CENTER 3 = MANUAL CENTER 4 = PIT
Example	:CALCULATE:PARAMETER:WDM: NALGO ACENTER :CALCULATE:PARAMETER:WDM:NALGO?-> 2
Explanation	This is a sequential command.
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>NARea</b>	
Function	Sets/queries the measuring range applied to noise level measurements made by the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :NARea<wsp><NRf>[M] :CALCulate:PARameter[:CATEgory]:WDM :NARea? <NRf> = NOISE AREA [m]
Example	:CALCULATE:PARAMETER:WDM: NAREA 0.80NM :CALCULATE:PARAMETER:WDM:NAREA? -> +8.0000000E-10
Explanation	This is a sequential command.
<b>:CALCulate:PARameter[:CATEgory]:WDM:</b>	
<b>NBW</b>	
Function	Sets/queries the noise bandwidth for the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM :NBW<wsp><NRf>[M] :CALCulate:PARameter[:CATEgory]:WDM :NBW? <NRf> = Noise bandwidth [m]
Example	:CALCULATE:PARAMETER:WDM:NBW 0.10NM :CALCULATE:PARAMETER:WDM:NBW?-> +1.0000000E-010
Explanation	This is a sequential command.

## 7.6 Instrument-Specific Commands

### :CALCulate:PARameter[:CATEgory]:WDM:

#### OSlope

Function	Sets/queries whether to enable the function of obtaining the least square approximation line in the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM: :OSlope<wsp>OFF ON 0 1 :CALCulate:PARameter[:CATEgory]:WDM: :OSlope? Response 0 = OFF, 1 = ON
Example	:CALCULATE:PARAMETER:WDM:OSLOP ON :CALCULATE:PARAMETER:WDM:OSLOP? -> 1
Explanation	<ul style="list-style-type: none"> <li>When this set value is 1 (ON), this instrument calculates the least square approximation line of the peak of each channel and draws it on the waveform screen.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:PARameter[:CATEgory]:WDM:

#### PDISplay

Function	Sets/queries whether to display data used for fitting of the WDM analysis function on the waveform screen.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM: :PDISplay<wsp>OFF ON 0 1 :CALCulate:PARameter[:CATEgory]:WDM: :PDISplay? Response 0 = OFF, 1 = ON
Example	:CALCULATE:PARAMETER:WDM: PDISPLAY ON :CALCULATE:PARAMETER:WDM:PDISPLAY?-> 1
Explanation	<ul style="list-style-type: none"> <li>When this set value is 1 (ON), data used for fitting is displayed on the waveform screen.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:PARameter[:CATEgory]:WDM:

#### RCH

Function	Sets/queries the reference channel used in calculating the offset wavelength/level of the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM: :RCH<wsp><integer> :CALCulate:PARameter[:CATEgory]:WDM: :RCH? <integer> = Reference channel number (0: channel with the highest level)
Example	:CALCULATE:PARAMETER:RCH 10 :CALCULATE:PARAMETER:RCH? -> 10
Explanation	<ul style="list-style-type: none"> <li>When this set value is "0," the channel with the highest level is regarded as the reference channel.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:PARameter[:CATEgory]:WDM:

#### RELation

Function	Sets/queries the display format of the wavelength/level relative values for the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM: :RELation<wsp>OFFSET SPACing 0 1 :CALCulate:PARameter[:CATEgory]:WDM: :RELation? OFFSET 0 = Displays an offset value based on any channel. SPACing 1 = Displays an offset value relative to a neighboring channel.
Example	Response 0 = OFFSET, 1 = SPACING :CALCULATE:PARAMETER:WDM: RELATION SPACING :CALCULATE:PARAMETER:WDM:RELATION?-> 1
Explanation	<ul style="list-style-type: none"> <li>When "DISPLAY TYPE" (set by the :CALCulate:PARameter[:CATEgory]:WDM:DTYPE command) is set to other than "ABSOLUTE", an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:PARameter[:CATEgory]:WDM:

#### SPower

Function	Sets/queries the signal light power calculation method of the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM: :SPOWer<wsp>PEAK INTEGRal 0 1 :CALCulate:PARameter[:CATEgory]:WDM: :SPOWer? PEAK 0 = Sets the mode peak to the signal light power INTEGRal 1 = Sets the power that integrates the spectrum to the signal light power
Example	:CALCULATE:PARAMETER:WDM:SPOWer PEAK :CALCULATE:PARAMETER:WDM:SPOWer? -> 0
Explanation	<ul style="list-style-type: none"> <li>With the AQ6375, the command is invalid.</li> <li>This is a sequential command.</li> </ul>

### :CALCulate:PARameter[:CATEgory]:WDM:

#### TH

Function	Sets/queries the threshold level of channel detection for the WDM analysis function.
Syntax	:CALCulate:PARameter[:CATEgory]:WDM: :TH<wsp><NRf>[dB] :CALCulate:PARameter[:CATEgory]:WDM: :TH? <NRf> = Threshold level [dB]
Example	:CALCULATE:PARAMETER:WDM:TH 20.00db :CALCULATE:PARAMETER:WDM:TH-> +2.0000000E+001
Explanation	This is a sequential command.

## 7.6 Instrument-Specific Commands

<b>:CALCulate:PARameter[:CATEgory]:WFBottom</b>		
Function	Sets/queries parameters for the WDM FILTER-BTM analysis function.	
Syntax	<pre>:CALCulate:PARameter[:CATEgory]:WFBottom&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt;,&lt;data&gt; :CALCulate:PARameter[:CATEgory]:WFBottom?&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt;</pre> <p>&lt;item&gt; = Analytical item that sets parameter(s)      &lt;parameter&gt; = Parameter to be set      &lt;data&gt; = Data to be set</p>	
<b>&lt;item&gt; &lt;parameter&gt; &lt;data&gt;</b>		
NWAveLength	ALGO	BOTtom NPEak  NBOTtom  GFIT GRID MDIFF TH TBAND
BWAveLength	SW	OFF ON 0 1
CWAveLength	SW	OFF ON 0 1 ALGO TH
SBAND	SW	OFF ON 0 1 TH
EBAND	SW	OFF ON 0 1 TH TBAND
RIPPLe	SW	OFF ON 0 1 TBAND
XTALK	SW	OFF ON 0 1 SPACing TBAND

**Example**

```
:CALCULATE:PARAMETER:WFBOTTOM
NWAY, ALGO, NPEAK
:CALCULATE:PARAMETER:WFBOTTOM?
NWAY, ALGO -> NPE:CALCULATE:
PARAMETER:WFBOTTOM BWAVELENGTH, SW,
OFF
:CALCULATE:PARAMETER:WFBOTTOM?
BWAVELENGTH, SW -> 0
```

**Explanation**

- If a non-existing parameter is used for a combination, an execution error occurs (a combination of NWAveLength and SPACing, etc.).
- With the AQ6373/AQ6373B, the command is invalid.
- This is a sequential command.

<b>:CALCulate:PARameter[:CATEgory]:WFPeak</b>		
Function	Sets/queries parameters for the WDM FILTER-PEAK analysis function.	
Syntax	<pre>:CALCulate:PARameter[:CATEgory]:WFPeak&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt;,&lt;data&gt; :CALCulate:PARameter[:CATEgory]:WFPeak?&lt;wsp&gt;&lt;item&gt;,&lt;paramater&gt;</pre> <p>&lt;item&gt; = Analytical item that sets parameter(s)      &lt;parameter&gt; = Parameter to be set      &lt;data&gt; = Data to be set</p>	
<b>&lt;item&gt; &lt;parameter&gt; &lt;data&gt;</b>		
NWAveLength	ALGO	PEAK MEAN GFIT  GRID MDIFF TH TBAND
BWAveLength	SW	OFF ON 0 1
CWAveLength	SW	OFF ON 0 1 TH
SBAND	SW	OFF ON 0 1 TH
PBAND	SW	OFF ON 0 1 TH TBAND
RIPPLe	SW	OFF ON 0 1 TBAND
XTALK	SW	OFF ON 0 1 SPACing TBAND

**Example**

```
:CALCULATE:PARAMETER:WFPEAK
NWAY, ALGO, PEAK
:CALCULATE:PARAMETER:WFPEAK?
NWAY, ALGO -> PEAK
:CALCULATE:PARAMETER:WFPEAK
BWAVELENGTH, SW, OFF
:CALCULATE:PARAMETER:WFPEAK?
BWAVELENGTH, S -> 0
```

**Explanation**

- If a non-existing parameter is used for a combination, an execution error occurs (a combination of NWAveLength and SPACing, etc.).
- With the AQ6373/AQ6373B, the command is invalid.
- This is a sequential command.

### **:CALCulate:PARameter:COMMON:MDIFF**

**Function**

Sets/queries the peak-bottom difference parameter of channel detection used in the analysis function.

**Syntax**

```
:CALCulate:PARameter:COMMON:MDIFF<wsp><NRF>[DB]
```

**Example**

```
:CALCULATE:PARAMETER:COMMON:
```

MDIFF 3.00DB

```
:CALCULATE:PARAMETER:COMMON:MDIFF->
+3.0000000E+000
```

**Explanation**

This is a sequential command.

## 7.6 Instrument-Specific Commands

### CALibration Sub System Command

#### :CALibration:ALIGN[:IMMEDIATE]

Function Executes optical axis adjustment of the monochromator using the internal reference light source.  
Syntax :CALibration:ALIGN[:IMMEDIATE]  
Example :CALIBRATION:ALIGN  
Explanation This is an overlapable command.

#### :CALibration:ALIGN:EXTernal[:IMMEDIATE]

Function Executes optical axis adjustment of the monochromator using an external light source.  
Syntax :CALibration:ALIGN:EXTernal[:IMMEDIATE]  
Example :CALIBRATION:ALIGN:EXTERNAL  
Description • This is an overlappable command.  
• This command can be used on the AQ6370D without the reference light source (-L0).

#### :CALibration:ALIGN:INTERNAL[:IMMEDIATE]

Function Executes optical axis adjustment of the monochromator using the internal reference light source.  
Syntax :CALibration:ALIGN:INTERNAL[:IMMEDIATE]  
Example :CALIBRATION:ALIGN:INTERNAL  
Description • This is an overlappable command.  
• This command can be used on the AQ6370C/AQ6370D.

#### :CALibration:BANDwidth|:BWIDth[:IMMEDIATE]

Function Executes an resolution calibration.  
Syntax :CALibration:BANDwidth|:BWIDth[:IMMEDIATE]  
Example :CALIBRATION:BANDWIDTH:IMMEDIATE  
Description • When the resolution calibration finishes, bit 3 (Cal/Alignment) of the operation status register is set to 1.  
For details, see section 6.4.  
• This is an overlappable command.  
• This command can be used on the AQ6370C/AQ6370D.

#### :CALibration:BANDwidth|:BWIDth:INITIalize

Function Clears the rms resolution calibration value.  
Syntax :CALibration:BANDwidth|:BWIDth:INITIALIZE  
Example :CALIBRATION:BANDWIDTH:INITIALIZE  
Description • This is a sequential command.  
• This command can be used on the AQ6370C/AQ6370D.

#### :CALibration:BANDwidth|:BWIDth:WAVelength?

Function Queries the wavelength of the light source used to perform resolution calibration.  
Syntax :CALibration:BANDwidth|:BWIDth:WAVElength?  
Response <NRf> = Light source wavelength in meters  
Example :CALIBRATION:BANDWIDTH:WAVELLENGTH?  
-> 1.5500000E-006  
Description • If resolution calibration has not been executed, this command returns 0.  
• This is a sequential command.  
• This command can be used on the AQ6370C/AQ6370D.

#### :CALibration:POWer:OFFSet:TABLE

Function Sets/queries the level offset table.  
Syntax :CALibration:POWer:OFFSet:TABLE<wsp><integer>,<NRf> [dB]  
:CALibration:POWer:OFFSet:TABLE?<wp><integer>  
<integer> = wavelength [nm]  
<NRf> = Level offset value [dB]  
Example :CALIBRATION:POWER:OFFSET:  
TABLE 1550,-0.1DB  
:CALIBRATION:POWER:OFFSET:TABLE?  
1550 -> -1.0000000E-001  
Explanation • Of the level offset table, the command sets or queries the offset value of a wavelength specified by <integer>.  
• This is a sequential command.

## 7.6 Instrument-Specific Commands

### **:CALibration:WAVelength:EXTernal[:IM Mediate]**

Function	Performs wavelength calibration using an external reference light source.
Syntax	:CALibration:WAVelength:EXTernal[:IM Mediate]
Example	:CALIBRATION:WAVELENGTH:EXTERNAL
Explanation	<ul style="list-style-type: none"> <li>• The type of the external reference light source to be used for calibration is set using the CALibration:WAVelength:EXTernal:SOURce command.</li> <li>• The wavelength of the external reference light source to be used for calibration is set using the CALibration:WAVelength:EXTernal:WAVelength command.</li> <li>• This is an overlapable command.</li> </ul>

### **:CALibration:WAVelength:EXTernal:SOU Rce**

Function	Sets/queries the type of the light source used for external reference light source-based wavelength calibration.
Syntax	:CALibration:WAVelength:EXTernal :SOURce<wsp>LASer GASCell EMISSION 0 1 2 :CALibration:WAVelength:EXTernal:SO URce?
	LASer = An external reference light source is used for the laser
	GASCell = A gas cell is used as the external reference light source.
	EMISSION = An emission light is used as the external reference light source.
Response	0 = Laser, 1 = Gas cell, 2 = Emission light
Example	:CALIBRATION:WAVELENGTH:EXTERNAL:S OURCE LASER :CALIBRATION:WAVELENGTH:EXTERNAL:S OURCEe? -> 0
Explanation	<ul style="list-style-type: none"> <li>• Of the level offset table, the command sets or queries the offset value of a wavelength specified by &lt;integer&gt;.</li> <li>• On the AQ6373/AQ6373B, the following parameter cannot be set. GASCell , 1</li> <li>• This is a sequential command.</li> </ul>

### **:CALibration:WAVelength:EXTernal:WA Vlength**

Function	Sets/queries the wavelength of the light source used for external reference light source-based wavelength calibration.
Syntax	:CALibration:WAVelength:EXTernal:WA Vlength<wsp><NRf>[M] :CALibration:WAVelength:EXTernal:WA Vlength? <NRf> = Wavelength of the external reference light source [nm]
Example	:CALIBRATION:WAVELENGTH:EXTERNAL:W AVELENGTH 1550.000NM :CALIBRATION:WAVELENGTH:EXTERNAL:W AVELENGTH? -> +1.5500000E-006
Explanation	This is a sequential command.

### **:CALibration:WAVelength:INTernal[:IM Mediate]**

Function	Performs wavelength calibration using an internal reference light source.
Syntax	:CALibration:WAVelength:INTernal[:IM Mediate]
Example	:CALIBRATION:WAVELENGTH:INTERNAL
Explanation	<ul style="list-style-type: none"> <li>• With the AQ6373/AQ6373B, the command is invalid.</li> <li>• This is an overlapable command.</li> </ul>

### **:CALibration:WAVelength:OFFSet:TABLE**

Function	Sets/queries the wavelength offset table.
Syntax	:CALibration:POWer:OFFSet:TABLE<wsp ><integer>,<NRf> :CALibration:POWer:OFFSet:TABLE?<ws p><integer> <integer> = wavelength (specified in nm) <NRf> = Wavelength offset value (specified in nm)
Example	:CALIBRATION:WAVELENGTH:OFFSET:TAB LE 1550,-0.1 :CALIBRATION:WAVELENGTH:OFFSET:TAB LE? 1550 -> -1.0000000E-001
Explanation	<ul style="list-style-type: none"> <li>• Of the wavelength offset table, the command sets or queries the offset value of a wavelength specified by &lt;integer&gt;.</li> <li>• This is a sequential command.</li> </ul>

## 7.6 Instrument-Specific Commands

### **:CALibration:ZERO[:AUTO]**

Function	Sets/queries whether to enable the auto offset function of the level.
Syntax	:CALibration:ZERO[:AUTO]<wp>OFF ON 0 1 ONCE :CALibration:ZERO[:AUTO]?
Example	Response 0 = OFF, 1 = ON :CALIBRATION:ZERO ONCE :CALIBRATION:ZERO? -> 1
Explanation	<ul style="list-style-type: none"> <li>• If you send this command with the parameter "ONCE" when the sweep is stopped, offset adjustment is performed once. In this case, ON/OFF of this setting does not change.</li> <li>• On the AQ6370C/AQ6370D/AQ6373B, the operation of this command is complete at the instant the offset adjustment starts. Therefore, the AQ6370C/AQ6370D/AQ6373B can execute the next command even while offset adjustment is being performed. You can use :CALibration:ZERO[:AUTO]:STATus? to query the execution status of the offset adjustment.</li> <li>• This is a sequential command.</li> </ul>

### **:CALibration:ZERO[:AUTO]:INTerval**

Function	Sets/queries the time interval for executing the Auto Offset function for the level.
Syntax	:CALibration:ZERO[:AUTO]:INTerval<wp><integer> :CALibration:ZERO[:AUTO]:INTerval?<integer>= Interval of execution (specified in units of minutes)
Example	:CALIBRATION:ZERO:INTERVAL 20 :CALIBRATION:ZERO:INTERVAL? -> 20
Explanation	<ul style="list-style-type: none"> <li>• When a time is set for this parameter, the auto offset adjustment is performed at the specified time interval starting from the moment of execution.</li> <li>• This command only valid for the AQ6373/AQ6373B.</li> <li>• This is a sequential command.</li> </ul>

### **:CALibration:ZERO[:AUTO]:STATus?**

Function	Queries the offset adjustment status.
Syntax	:CALibration:ZERO[:AUTO]:STATus?
	0: The offset adjustment is not being executed. 1: The offset adjustment is being executed.
Example	:CALIBRATION:ZERO:STATUS? -> 1
Explanation	<ul style="list-style-type: none"> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

## DISPlay Sub System Command

### **:DISPlay:COLOR**

Function	Sets/queries the screen color mode.
Syntax	:DISPlay:COLOR<wp><mode> :DISPlay:COLOR? 0 = Black and white mode 1–5 = Modes 1–5
Example	:DISPLAY:COLOR 1 :DISPLAY:COLOR? -> 1
Explanation	This is a sequential command.

### **:DISPlay[:WINDOW]**

Function	Sets/queries whether the display is enabled.
Syntax	:DISPlay[:WINDow]<wp>OFF ON 0 1 :DISPlay[:WINDow]?
Example	Response 0 = OFF, 1 = ON :DISPLAY OFF :DISPLAY? -> 0
Explanation	<ul style="list-style-type: none"> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

### **:DISPlay[:WINDOW]:OVIew:POSITION**

Function	Sets/queries the ON/OFF and position of the OVERVIEW display shown during zoom operation.
Syntax	:DISPlay[:WINDow]:OVIew:POSition<wp>OFF LEFT RIGHT 0 1 2 :DISPlay[:WINDow]:OVIew:POSition? OFF = Display OFF LEFT = The overview display is on the left of the screen. RIGHT = The overview display is on the right of the screen.
Example	Response 0 = OFF, 1 = LEFT, 2 = RIGHT :DISPLAY:OVIEW:POSITION RIGHT :DISPLAY:OVIEW:POSITION? -> 2
Explanation	This is a sequential command.

### **:DISPlay[:WINDOW]:OVIew:SIZE**

Function	Sets/queries the size of the OVERVIEW display shown during zoom operation.
Syntax	:DISPlay[:WINDow]:OVIew:SIZE<wp>LA RG SMALL 0 1 :DISPlay[:WINDow]:OVIew:SIZE? LARGE = Larger OVERVIEW size SMALL = Smaller OVERVIEW size Response 0 = LARGE, 1 = SMALL
Example	:DISPLAY:OVIEW:SIZE LARGE :DISPLAY:OVIEW:SIZE? -> 0
Explanation	This is a sequential command.

**:DISPlay[:WINDOW]:SPLIT**

**Function** Sets/queries whether to split the screen display into two parts.

**Syntax** :DISPlay[:WINDOW]:SPLIT<wsp>OFF|ON|0|1  
:DISPlay[:WINDOW]:SPLIT?  
Response 0 = OFF, 1 = ON

**Example** :DISPLAY:SPLIT ON  
:DISPLAY:SPLIT? -> 1

**Explanation** This is a sequential command.

**:DISPlay[:WINDOW]:SPLIT:HOLD:LOWER**

**Function** Sets/queries whether to fix a trace assigned to the lower area when the screen is in the upper/lower 2-split display mode.

**Syntax** :DISPlay[:WINDOW]:SPLIT:HOLD:LOWER<wsp>OFF|ON|0|1  
:DISPlay[:WINDOW]:SPLIT:HOLD:LOWER?  
Response 0 = OFF, 1 = ON

**Example** :DISPLAY:SPLIT:HOLD:LOWER ON  
:DISPLAY:SPLIT:HOLD:LOWER? -> 1

**Explanation** If not in 2-split screen display mode, an execution error occurs.

**:DISPlay[:WINDOW]:SPLIT:HOLD:UPPER**

**Function** Sets/queries whether to fix a trace assigned to the upper area when the screen is in the upper/lower 2-split display mode.

**Syntax** :DISPlay[:WINDOW]:SPLIT:HOLD:UPPER<wsp>OFF|ON|0|1  
:DISPlay[:WINDOW]:SPLIT:HOLD:UPPER?  
Response 0 = OFF, 1 = ON

**Example** :DISPLAY:SPLIT:HOLD:UPPER ON  
:DISPLAY:SPLIT:HOLD:UPPER? -> 1

**Explanation** • If not in 2-split screen display mode, an execution error occurs.  
• This is a sequential command.

**:DISPlay[:WINDOW]:SPLIT:POSITION**

**Function** Sets/queries whichever display area, upper or lower, is used to display a trace when the screen is in the upper/lower 2-split display mode.

**Syntax** :DISPlay[:WINDOW]:SPLIT:POSITION<wsp><trace name>,UP|LOW|0|1  
:DISPlay[:WINDOW]:SPLIT:POSITION?  
<wsp><trace name>  
<trace name> = trace name  
(TRA,TRB,TRC,TRD,TRE,TRF,TRG)  
UP = Trace is displayed in the upper area.  
LOW = Trace is displayed on the lower area.  
Response 0 = UP, 1 = LOW

**Example** :DISPLAY:SPLIT:POSITION TRA,UP  
:DISPLAY:SPLIT:POSITION? TRA -> 0

**Explanation** This is a sequential command.

**:DISPlay[:WINDOW]:TEXT:CLEar**

**Function** Clears labels.

**Syntax** :DISPlay[:WINDOW]:TEXT:CLEar

**Example** :DISPLAY:TEXT:CLEAR

**Explanation** This is a sequential command.

**:DISPlay[:WINDOW]:TEXT:DATA**

**Function** Sets/queries the labels.

**Syntax** :DISPlay[:WINDOW]:TEXT:DATA<wsp><string>  
:DISPlay[:WINDOW]:TEXT:DATA?  
<string> = Label character string (56 characters max.)

**Example** :DISPLAY:TEXT:  
DATA "Optical Spectrum Analyzer"  
:DISPLAY:TEXT:DATA?->  
Optical Spectrum Analyzer

**Explanation** • A label character string has a maximum length of 56 characters. If a label of more than 56 characters is specified, characters from and exceeding the 57th will be ignored.  
• If there is no label, one space character is returned.  
• This is a sequential command.

**:DISPlay[:WINDOW]:TRACe:X[:SCALE]:CENTer**

**Function** Sets/queries the center wavelength of the X-axis of the display scale.

**Syntax** :DISPlay[:WINDOW]:TRACe:X[:SCALE]:CENTer<wsp><NRF>[M|HZ]  
:DISPlay[:WINDOW]:TRACe:X[:SCALE]:CENTer?  
<NRF> = Center wavelength [m|Hz]

**Response**  
<NRF>[m|Hz] (AQ6370C/AQ6370D/  
AQ6373B)  
<NRF>[m|Hz|m<sup>-1</sup>] (AQ6375)

**Example** :DISPLAY:TRACE:X:CENTER 1550.000NM  
:DISPLAY:TRACE:X:CENTER?->  
+1.5500000E-006

**Explanation** • For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value.  
• This is a sequential command.

**:DISPlay[:WINDOW]:TRACe:X[:SCALE]:INITialize**

**Function** Initializes the X-axis parameters of the display scale.

**Syntax** :DISPlay[:WINDOW]:TRACe:X[:SCALE]:INITialize

**Example** :DISPLAY:TRACE:X:INITIALIZE

**Explanation** • The following parameters are initialized based on the measurement scale after this command has been executed.  
ZOOM CENTER, ZOOM SPAN, ZOOM START, ZOOM STOP  
• This is a sequential command.

## 7.6 Instrument-Specific Commands

### :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:SM Scale

Function	Sets parameters of the current display scale to the measurement scale.
Syntax	:DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S MScale
Example	:DISPLAY:TRACE:X:SMSCALE
Explanation	<ul style="list-style-type: none"> <li>The following parameters are initialized based on the display scale after this command has been executed.</li> <li>CENTER, SPAN, START, STOP</li> <li>This is a sequential command.</li> </ul>

### :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:SP AN

Function	Sets/queries the span of the X-axis of the display scale.
Syntax	:DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S PAN<wsp><NRf>[M HZ] :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S PAN? <NRf> = Span [m Hz]
Response	<NRf>[m Hz] (AQ6370C/AQ6370D/ AQ6373B) <NRf>[m Hz m <sup>-1</sup> ] (AQ6375)
Example	:DISPLAY:TRACE:X:SPAN 20.0NM :DISPLAY:TRACE:X:SPAN? -> +2.0000000E-008
Explanation	<ul style="list-style-type: none"> <li>For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value.</li> <li>This is a sequential command.</li> </ul>

### :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:SR ANGE

Function	Sets/queries whether to limit an analytical range to the display scale range.
Syntax	:DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S RANGE<wsp>OFF ON 0 1 :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S RANGE?
Response	0 = OFF, 1 = ON
Example	:DISPLAY:TRACE:X:SRANGE on :DISPLAY:TRACE:X:SRANGE? -> 1

Explanation This is a sequential command.

### :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:START

Function	Sets/queries the start wavelength of the X-axis of the display scale.
Syntax	:DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S TART<wsp><NRf>[M HZ] :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S TART? <NRf> = Start wavelength [m Hz]
Response	<NRf>[m Hz] (AQ6370C/AQ6370D/ AQ6373B) <NRf>[m Hz m <sup>-1</sup> ] (AQ6375)

Example	:DISPLAY:TRACE:X:START 1540.000NM :DISPLAY:TRACE:X:START?-> +1.5400000E-006
Explanation	<ul style="list-style-type: none"> <li>For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value.</li> <li>This is a sequential command.</li> </ul>

### :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:STOP

Function	Sets/queries the stop wavelength of the X-axis of the display scale.
Syntax	:DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S TOP<wsp><NRf>[M HZ] :DISPLAY[:WINDOW]:TRACe:X[:SCALE]:S TOP? <NRf> = Stop wavelength [m Hz]
Response	<NRf>[m Hz] (AQ6370C/AQ6370D/ AQ6373B) <NRf>[m Hz m <sup>-1</sup> ] (AQ6375)

Example	:DISPLAY:TRACE:X:STOP 1560.000NM :DISPLAY:TRACE:X:STOP?-> +1.5600000E-006
Explanation	<ul style="list-style-type: none"> <li>For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value.</li> <li>This is a sequential command.</li> </ul>

### :DISPLAY[:WINDOW]:TRACe:Y:NMask

Function	Sets whether to mask the display of waveforms the level of which is at or below a set threshold level or queries the condition of whether the relevant waveform display is masked.
Syntax	:DISPLAY[:WINDOW]:TRACe:Y:NMask<wsp><NRf>[dB] :DISPLAY[:WINDOW]:TRACe:Y:NMask? <NRf> = Threshold level [dB] (-999: Masking function OFF)

Example	:DISPLAY:TRACE:Y:MASK -999 :DISPLAY:TRACE:Y:MASK? -> -9.9900000E+002
Explanation	<ul style="list-style-type: none"> <li>The display of waveforms the level of which is at or below this parameter will be masked. To turn off the mask function, set the threshold level to -999.</li> <li>This is a sequential command.</li> </ul>

## 7.6 Instrument-Specific Commands

### **:DISPlay[:WINDOW]:TRACe:Y:NMASK:TYPE**

Function	Sets/queries the display method when a waveform display at or below a threshold level is masked.
Syntax	:DISPlay[:WINDOW]:TRACe:Y:NMASK:TYPE E<wsp>VERTical HORizontal 0 1 :DISPlay[:WINDOW]:TRACe:Y:NMASK:TY PE? VERTical = Waveform display with zero as the mask value or lower HORizontal = Waveform display with the mask value as the mask value or lower Response 0 = VERTical, 1 = HORizontal
Example	:DISPLAY:TRACE:Y:MASK:TYPE VERTICAL :DISPLAY:TRACE:Y:MASK:TYPE? -> 0
Explanation	This is a sequential command.

### **:DISPlay[:WINDOW]:TRACe:Y[:SCALe]:DN UMber**

Function	Sets/queries the number of display divisions of the level axis.
Syntax	:DISPlay[:WINDOW]:TRACe:Y[:SCALe]:D NUMber<wsp>8 10 12 :DISPlay[:WINDOW]:TRACe:Y[:SCALe]:D NUMber? 8, 10, 12 = Number of display divisions
Example	:DISPLAY:TRACE:Y:DNUMBER 10 :DISPLAY:TRACE:Y:DNUMBER? -> 10
Explanation	This is a sequential command.

### **:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]:B LEVel**

Function	Sets/queries the base level applied when the main scale of the level axis is linear.
Syntax	:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: BLEVel<wsp><NRf>[W] :DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: BLEVel? <NRf> = Base level value [W]
Example	:DISPLAY:TRACE:Y1:BLEVEL 1.0MW :DISPLAY:TRACE:Y1:BLEVEL?-> +1.0000000E-003
Explanation	• If a instrument other than W is specified, an execution error occurs. • This is a sequential command.

### **:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]:P DIVision**

Function	Sets/queries the main scale of the level axis.
Syntax	:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: PDIVision<wsp><NRf>[DB] :DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: PDIVision? <NRf> = Level scale [dB]
Example	:DISPLAY:TRACE:Y1:PDIV 5.0DB :DISPLAY:TRACE:Y1:PDIV?-> +5.0000000E+000
Explanation	• If a instrument other than dB is specified, an execution error occurs. • This is a sequential command.

### **:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]:R LEVel**

Function	Sets/queries the reference level of the main scale of the level axis.
Syntax	:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: RLEVel<wsp><NRf>[DBM W] :DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: RLEVel? <NRf> = Reference level [dB W]
Example	:DISPLAY:TRACE:Y1:RLEVEL -30dbm :DISPLAY:TRACE:Y1:RLEVEL?-> -3.0000000E+001
Explanation	• When the unit is omitted in the parameter, the reference level is set in dBm if the main scale of the level axis is in the LOG mode or is set in W if it is in the linear mode. • If the setting condition of the LOG/linear mode of the level axis' main scale does not match the unit specified in the parameter of the command, the parameter of this command is translated matching the LOG/linear mode of the main scale. For example, when the main scale is LOG and you set the reference level to 1m with this command, the reference level is set to 0 dB. • This is a sequential command.

## 7.6 Instrument-Specific Commands

<b>:DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:RPOSITION</b>		<b>:DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:AUTO</b>	
Function	Sets/queries the position of the reference level of the main scale of the level axis.	Function	Sets/queries the automatic setting function of the sub scale of the level axis.
Syntax	:DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:RPOSITION<wp><integer>[DIV] :DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:RPOSITION? <integer> = Position of the reference level	Syntax	:DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:AUTO<wp>OFF ON 0 1 :DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:AUTO? Response 0 = OFF, 1 = ON
Example	:DISPLAY:TRACE:Y1:RPOSITION 10DIV :DISPLAY:TRACE:Y1:RPOSITION? -> 10	Example	:DISPLAY:TRACE:Y2:AUTO ON :DISPLAY:TRACE:Y2:AUTO? -> 1
Explanation	<ul style="list-style-type: none"> <li>If a value greater than the number of display divisions of the level axis is specified for the position of the reference level, the position of this level is treated as the top of the scale.</li> <li>This is a sequential command.</li> </ul>	Explanation	This is a sequential command.
<b>:DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:SPACING</b>		<b>:DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:LENGTH</b>	
Function	Sets/queries the scale mode of the main scale of the level axis.	Function	Sets/queries the parameter of the optical fiber length used when the unit of the subscale of the level axis is dB/km.
Syntax	:DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:SPACING<wp>LOGarithmic LINEar 0 1 :DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:SPACING? LOGarithmic = LOG scale LINEar = Linear scale Response 0 = LOGarithmic, 1 = LINEar	Syntax	:DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:LENGTH<wp><NRf>[KM] :DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:LENGTH? <NRf> = Length of optical fiber [km]
Example	:DISPLAY:TRACE:Y1:SPACING LINIER :DISPLAY:TRACE:Y1:SPACING? -> 1	Example	:DISPLAY:TRACE:Y2:LENGTH 99.999KM :DISPLAY:TRACE:Y2:LENGTH?-> +9.9999000E+001
Explanation	This is a sequential command.	Explanation	<ul style="list-style-type: none"> <li>When the unit of the subscale is set to other than "dB/km", an execution error occurs.</li> <li>This is a sequential command.</li> </ul>
<b>:DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:UNIT</b>		<b>:DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:OLEVEL</b>	
Function	Sets/queries the units of the main scale of the level axis.	Function	Sets/queries the offset level of the sub scale of the level axis.
Syntax	:DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:UNIT<wp><unit> :DISPLAY[:WINDOW]:TRACe:Y1[:SCALE]:UNIT? DBM = dBm W = W DBM/NM = dBm/nm or dBm/THz W/NM = W/nm or W/THz Response 0 = dBm 1 = W 2 = DBM/NM 3 = W/NM	Syntax	:DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:OLEVEL<wp><NRf>[DB DB/KM] :DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:OLEVEL? <NRf> = Offset level [dB dB/km]
Example	:DISPLAY:TRACE:Y1:UNIT DBM/NM :DISPLAY:TRACE:Y1:UNIT? -> 2	Example	:DISPLAY:TRACE:Y2:OLEVEL 10DB/KM :DISPLAY:TRACE:Y2:OLEVEL? -> +1.0000000E+001
Explanation	<ul style="list-style-type: none"> <li>For the AQ6375, the parameters cannot be set when in Wavenumber mode. Query commands function even when in Wavenumber mode.</li> <li>This is a sequential command.</li> </ul>	Explanation	<ul style="list-style-type: none"> <li>When the unit of the subscale is set to other than "dB" or "dB/km", an execution error occurs.</li> <li>If the unit is not specified in the parameter, dB is set if the subscale of the level axis is in the dB mode or dB/km is set if it is in the dB/km mode.</li> <li>If a unit different from the current set unit (:DISPLAY[:WINDOW]:TRACe:Y2[:SCALE]:UNIT) of the subscale is specified, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

<b>:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:PDIVision</b>	
Function	Sets/queries the sub scale of the level axis.
Syntax	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:PDIVision<wsp><NRf>[DB DB/KM   %] :DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:PDIVision? <NRf> = Level scale [dB   dB/km   %]
Example	:DISPLAY:TRACE:Y2:PDIVISION 5.0% :DISPLAY:TRACE:Y2:PDIVISION? -> +5.0000000E+000
Explanation	<ul style="list-style-type: none"> <li>If the unit is not specified in the parameter, the set unit of the subscale of the level axis is used as the set unit of this parameter.</li> <li>If a unit different from the current set unit (:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:UNIT) of the subscale is specified, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>

<b>:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:RPOSITION</b>	
Function	Sets/queries the position of the reference level of the sub scale of the level axis.
Syntax	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:RPOSITION<wsp><integer>[DIV] :DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:RPOSITION? <integer> = Position of the reference level
Example	:DISPLAY:TRACE:Y2:RPOSITION 10DIV :DISPLAY:TRACE:Y2:RPOSITION? -> 10
Explanation	<ul style="list-style-type: none"> <li>If a value greater than the number of display divisions of the level axis is specified for the position of the reference level, the position of this level is treated as the top of the scale.</li> <li>This is a sequential command.</li> </ul>

<b>:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:SMINimum</b>	
Function	Sets/queries the value of the bottom of the scale applied when the subscale of the level axis is set to the linear or % mode.
Syntax	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:SMINimum<wsp><NRf>[%] :DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:SMINimum? <NRf> = Value of the bottom of the scale [%]
Example	:DISPLAY:TRACE:Y2:SMINIMUM 0% :DISPLAY:TRACE:Y2:SMINIMUM? -> 0
Explanation	<ul style="list-style-type: none"> <li>If the unit is not specified in the parameter, the set unit of the subscale of the level axis is used as the set unit of this parameter.</li> <li>If a unit different from the current set unit (:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:UNIT) of the subscale is specified, an execution error occurs.</li> <li>This is a sequential command.</li> </ul>
<b>:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:UNIT</b>	
Function	Sets/queries the units of the sub scale of the level axis.
Syntax	:DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:UNIT<wsp><unit> :DISPlay[:WINDOW]:TRACe:Y2[:SCALE]:UNIT? <unit> = Units DB = dB display LINEar = Linear display DB/KM = dB/km display % = % display
Response	0 = DB 1 = LINEar 2 = DB/KM 3 = %
Example	:DISPLAY:TRACE:Y2:UNIT DB/KM :DISPLAY:TRACE:Y2:UNIT? -> 2
Explanation	This is a sequential command.

## 7.6 Instrument-Specific Commands

### FORMAT Sub System Command

#### :FORMAT [:DATA]

Function Sets/queries the format used for data transfer via GP-IB.

Syntax :FORMAT[:DATA]<wsp>REAL[,64|,32]|ASCII  
:FORMAT[:DATA]?  
ASCII = ASCII format (default)  
REAL[.64] = REAL format (64bits)  
REAL,32 = REAL format (32bits)

Example FORMAT:DATA REAL,64  
FORMAT:DATA? -> REAL,64  
FORMAT:DATA REAL,32 FORMAT:DATA? ->  
REAL,32  
FORMAT:DATA ASCII  
FORMAT:DATA? -> ASCII

- Explanation
- When the format is set to REAL (binary) using this command, the output data of the following commands are produced in the REAL format.  
:CALCulate:DATA:CGAin?  
:CALCulate:DATA:CNF?  
:CALCulate:DATA:CPOWers?  
:CALCulate:DATA:CSNR?  
:CALCulate:DATA:CWAveLengths?  
:TRACe[:DATA]:X?  
:TRACe[:DATA]:Y?
  - The default is ASCII mode.
  - When the \*RST command is executed, the format is reset to the ASCII mode.
  - The ASCII format outputs a list of numerics each of which is delimited by a comma (,). Example: 12345,12345,....
  - By default, the REAL format outputs data in fixed length blocks of 64 bits, floating-point binary numerics.
  - If "REAL,32" is specified in the parameter, data is output in the 32-bit, floating-point binary form.
  - The fixed length block is defined by IEEE 488.2 and consists of "#" (ASCII), one numeric (ASCII) indicating the number of bytes that specifies the length after #, length designation (ASCII), and binary data of a specified length in this order. Binary data consists of a floating-point data string of 8 bytes (64 bits) or 4 bytes (32 bits). Floating-point data consists of lower-order bytes to higher-order bytes.  
E.g.: #18 [eight <byte data>]  
#280[80 <byte data>]  
#48008[8008 <byte data>]
  - For data output in the 32-bit floating-point binary form, cancellation of significant digits is more likely to occur in comparison with transfer of data in the 64-bit, floating-point binary form.
  - This is a sequential command.

### HCOPY Sub System Command

#### :HCOPY:DESTination

Function Sets/queries the print output destination.

Syntax :HCOPY:DESTination<wsp>INTernal|FILE|0|2  
:HCOPY:DESTination?  
INTernal = Internal Printer  
FILE = File  
Response 0 = INTernal  
2 = FILE

Example :HCOPY:DESTINATION FILE  
:HCOPY:DESTINATION? -> 2

Explanation

- This is a sequential command.
- The INTernal parameter cannot be used on the AQ6370D/AQ6373B.

#### :HCOPY[:IMMEDIATE]

Function Makes a hard copy of the screen display.

Syntax :HCOPY[:IMMEDIATE]

Example :HCOPY

Explanation This is an overlapable command.

#### :HCOPY[:IMMEDIATE]:FEED

Function Feeds printer paper to the internal printer.

Syntax :HCOPY[:IMMEDIATE]:FEED<wsp>[<integer>]  
<integer> = Specify the amount of feed in 1–10 (unit: × 5 mm)

Example :HCOPY:FEED

Explanation

- If <integer> is not specified, printer paper is fed by approximately 5 mm.
- This is a sequential command.
- This command cannot be used on the AQ6370D/AQ6373B.

#### :HCOPY[:IMMEDIATE]:FUNCTION:CALCULATE:LIST

Function Prints the results of the execution of an analysis function.

Syntax :HCOPY[:IMMEDIATE]:FUNCTION:CALCULATE:LIST

Example :HCOPY:FUNCTION:CALCULATE:LIST

Explanation

- If the analysis function is not executed, an execution error occurs.
- This is an overlapable command.

#### :HCOPY[:IMMEDIATE]:FUNCTION:MARKER:LIST

Function Prints a marker list.

Syntax :HCOPY[:IMMEDIATE]:FUNCTION:MARKER:LIST

Example :HCOPY:FUNCTION:MARKER:LIST

Explanation

- No execution error occurs even if a marker does not exist.
- This is an overlapable command.

**INITiate Sub System Command****:INITiate[ :IMMediate]**

Function Makes a sweep.  
 Syntax :INITiate[:IMMediate]  
 Example :INITIATE  
 Explanation • You can stop sweep with the :ABORT command.  
 • The sweep mode (AUTO, SINGLE, REPEAT, or SEGMENT MEASURE) is set using the :INITiate:SMODE command.  
 • If this command is executed while the sweep mode is in REPEAT (:INITiate:SMODE REPeat), the operation of the command is complete at the instant a sweep starts. In this case, this command is regarded as a sequential command.  
 • If this command is executed while the sweep mode is one of AUTO, SINGLE, and SEGMENT MEASURE, the operation of the command is complete at the instant a sweep ends. In this case, this command is regarded as a command subject to overlapping.

**:INITiate:SMODE**

Function Sets/queries the sweep mode.  
 Syntax :INITiate:SMODE<wsp><sweep mode>  
 :INITiate:SMODE?  
 <sweep mode> = Sweep mode  
 SINGle = SINGLE sweep mode  
 REPeat = REPEAT sweep mode  
 AUTO = AUTO sweep mode  
 SEGment = SEGMENT  
 Response 1 = SINGle  
 2 = REPeat  
 3 = AUTO  
 4 = SEGment  
 Example :INITIATE:SMODE REPEAT  
 :INITIATE:SMODE? -> 2  
 Explanation This is a sequential command.

**MEMory Sub System Command****:MEMory:CLEar**

Function Clears the contents of a specified waveform memory.  
 Syntax :MEMory:CLEar<wsp><integer>  
 <integer> = Memory number  
 Example :MEMORY:CLEAR 10  
 Explanation • No execution error occurs even if a specified waveform memory has already been cleared.  
 • This is a sequential command.

**:MEMory:EMPTY?**

Function Queries the condition of whether a waveform has been specified in a specified waveform memory.  
 Syntax :MEMory:EMPTY?<wsp><integer>  
 <integer> = Memory number  
 Example :MEMORY:EMPTY? 10 -> 1  
 Explanation This is a sequential command.

**:MEMory:LOAD**

Function Loads a waveform from a specified waveform memory into a specified trace.  
 Syntax :MEMory:LOAD<wsp><integer>,<trace name>  
 <integer> = Memory number  
 <trace name> = trace  
 (TRA,TRB,TRC,TRD,TRE,TRF,TRG)  
 Example :MEMORY:LOAD 10,TRA  
 Explanation • When a waveform is not registered in the specified waveform memory, a warning message appears.  
 • This is a sequential command.

**:MEMory:STORE**

Function Stores the waveform of a specified trace into a specified waveform memory.  
 Syntax :MEMory:STORe<wsp><integer>,<trace name>  
 <integer> = Memory number  
 <trace name>= trace  
 (TRA,TRB,TRC,TRD,TRE,TRF,TRG)  
 Example :MEMORY:STORE 10,TRA  
 Explanation • When waveform data do not exist in the specified trace, a warning message appears.  
 • This is a sequential command.

## 7.6 Instrument-Specific Commands

### MMEMemory Sub System Command

- Common Items
- To include a directory name in <"filename">, specify the path in the following manner.
  - Specification of an absolute path  
When the head of <"file name"> is character "\\", specify the absolute path.
  - Relative path specification  
When the head of <"file name"> is any character other than "\", specify the the relative path from the current directory. The current directory is specified using the :MMEMemory:CDIRectory command.
  - If INTernal|EXTernal is not specified, access is made to the current drive.  
The current drive is specified using the :MMEMemory:CDRive command.
  - If a file name extension is omitted when storing a file, an extension corresponding to the data type will be appended to the file name.
  - When loading a file, the file name extension can be omitted.

#### :MMEMemory:ANAMe

- Function Sets or queries the naming rule for automatic file names.
- Syntax :MMEMemory:ANAMe<wsp>NUMBER|DATE|0|1  
:MMEMemory:ANAMe?  
NUMBER|0 Number  
DATE|1 Timestamp
- Example :MMEMemory:ANAMe DATE  
:MMEMemory:ANAMe? -> 1
- Description • This command is for the AQ6370D.  
• This is a sequential command.

#### :MMEMemory:CATalog?

- Function Queries a list of all files in the current directory.
- Syntax :MMEMemory:CATalog?<wsp>[INTernal|EXTernal] [, <directory name>]  
INTernal = Acquires a file list in the current directory of the internal memory.  
EXTernal = Acquires a file list in the current directory of the external USB storage.  
directory name = Default name  
Response  
<free size>,<file number>,<file name>,<file name>,...,<file name>  
<free size> = <NRF> Disk's free size [KB] (1KB=1024 bytes)  
<file number> = <integer> number of files  
<file name> = File name
- Example :MMEMemory:CATALOG? INTERNAL, "\TEST\SAMPLE"  
-> +1.91176800E+006,2,test0001.wv6,test0002.wv6
- Explanation This is a sequential command.

#### :MMEMemory:CDIRectory

- Function Sets/queries the current directory.
- Syntax :MMEMemory:CDIRectory<wsp><directory name>  
:MMEMemory:CDIRectory?  
<directory name> = Directory name to be changed
- Example :MMEMemory:CDIRECTORY "\test\sample"  
:MMEMemory:CDIRECTORY? ->  
\test\sample

Explanation This is a sequential command.

#### :MMEMemory:CDRive

- Function Sets/queries the current drive.
- Syntax :MMEMemory:CDRive<wsp>INTernal|EXTernal  
:MMEMemory:CDRive?  
INTernal = Makes the current drive the internal memory.  
EXTernal = Makes the current drive the external USB storage.
- Example :MMEMemory:CDRIVE INTERNAL  
:MMEMemory:CDRIVE -> INT

Explanation This is a sequential command.

#### :MMEMemory:COPY

- Function Copies a specified file.
- Syntax :MMEMemory:COPY<wsp><"source file name">,[INTernal|EXTernal],<"destination file name">[,INTernal|EXTernal]  
<"source file name"> = File name at the copy source  
<"destination file name"> = File name at the copy destination
- Example :MMEMemory:COPY "test001.wv6",, "test002.wv6"

Explanation This is a sequential command.

#### :MMEMemory:DATA?

- Function Queries the data in the specified file.
- Syntax :MMEMemory:DATA?<wsp><"file name">[,INTernal|EXTernal]  
<"file name"> = Name of the file to be read  
Response  
The data that was read (binary block data of fixed length starting with "#")
- Example :MMEMemory:DATA? "test.csv",internal  
-> #18ABCDEFGH

Explanation • Maximum file size that can be sent is 1 MB.  
• For the data format of the fixed length blocks, see :FORMAT Command.  
• This is a sequential command.

#### :MMEMemory:DELetE

- Function Deletes a specified file.
- Syntax :MMEMemory:DELetE<wsp><"file name">[,INTernal|EXTernal]  
<"file name"> = Name of a file to be deleted
- Example :MMEMemory:DELETE "test002.wv6",internal

Explanation This is a sequential command.

**:MMEMORY:LOAD:ATRACE**

**Function** Loads the specified waveform files (all traces) into traces.

**Syntax** :MMEMORY:LOAD:ATRACE<wsp><"file name"> [,INTernal|EXTernal]  
<"file name"> = Name of file to load  
INTernal|EXTernal = Source drive for loading

**Example:** MMEMORY:LOAD:ATRACE "test001.csv",internal

**Explanation** This is a sequential command.

**:MMEMORY:LOAD:DLOGging**

**Function** Loads the specified data logging file.

**Syntax** :MMEMORY:LOAD:DLOGging<wsp><"filename"> [,INTernal|EXTernal]  
<"filename"> = Name of the file to load  
INTernal|EXTernal = Source drive to load from

**Example** :MMEMORY:LOAD:DLOGGING "test001.LG8", INTERNAL

**Description**

- This command is invalid when data logging is in progress.
- This is a sequential command.
- This command can be used on the AQ6370C/AQ6370D/AQ6373B.

**:MMEMORY:LOAD:MEMORY**

**Function** Loads a specified waveform file into a specified memory.

**Syntax** :MMEMORY:LOAD:MEMORY<wsp><integer>, <"file name"> [,INTernal|EXTernal]  
<integer> = Number of the memory into which a file is loaded  
<"file name"> = Name of file to be loaded  
INTernal|EXTernal = Drive of source file to load

**Example** :MMEMORY:LOAD:MEMORY 1,"test001.wv6" INTERNAL

**Explanation** This is a sequential command.

**:MMEMORY:LOAD:PROGRAM**

**Function** Loads a specified program file into a specified program number.

**Syntax** :MMEMORY:LOAD:PROGRAM<wsp><integer>, <"file name"> [,INTernal|EXTernal]  
<trace name> = Number of the program into which a file is loaded  
<"file name"> = Name of a file to be loaded  
INTernal|EXTernal = Drive of source file to be loaded

**Example** MMEMORY:LOAD:PROGRAM 1,"test001.prg", INTERNAL

**Explanation** This is a sequential command.

**:MMEMORY:LOAD:SETTING**

**Function** Loads a specified setting file.

**Syntax** :MMEMORY:LOAD:SETTING<wsp><"file name"> [,INTernal|EXTernal]  
<"file name"> = Name of a file to be loaded  
INTernal|LOPpy = Drive of source file to be loaded

**Example** MMEMORY:LOAD:SETTING "test001.st6", INTERNAL

**Explanation** This is a sequential command.

**:MMEMORY:LOAD:TEMPLATE**

**Function** Loads a specified template file.

**Syntax** :MMEMORY:LOAD:TEMPLATE<wsp><template>, <"file name"> [,INTernal|EXTernal]  
<template> = Template at the loading destination (UPPER|LOWER|TARGET)  
<"file name"> = Name of a file to be loaded  
INTernal|EXTernal = Drive at the loading source

**Example** :MMEMORY:LOAD:SETTING UPPER,"test001.csv", INTERNAL

**Explanation** This is a sequential command.

**:MMEMORY:LOAD:TRACe**

**Function** Loads a specified waveform file into a specified trace.

**Syntax** :MMEMORY:LOAD:TRACe<wsp><trace name>, <"file name"> [,INTernal|EXTernal]  
<trace name> = Trace to be loaded  
<"file name"> = Name of file to be loaded  
INTernal|EXTernal = Drive of source file to load

**Example** :MMEMORY:LOAD:TRACE TRA,"test001.wv6", INTERNAL

**Explanation** This is a sequential command.

**:MMEMORY:MDIRECTory**

**Function** Creates a new directory.

**Syntax** :MMEMORY:MDIRECTory<wsp><"directory name"> [,INTernal|EXTernal]  
<directory name> = Directory name to be created  
INTernal|EXTernal = Destination drive for created directory

**Example** :MMEMORY:MDIRECTORY "sample2", INTERNAL

**Explanation** This is a sequential command.

**:MMEMORY:REMove**

**Function** Readies the USB storage media for removal or queries the readiness status.

**Syntax** :MMEMORY:REMove  
:MMEMORY:REMove?  
Response 0 = Ready for removal  
1 = Not ready

**Example** :MMEMORY:REMOVE  
:MMEMORY:REMOVE -> 1

## 7.6 Instrument-Specific Commands

### :MMEMORY:RENAME

Function	Renames a specified file.
Syntax	:MMEMORY:RENAME<wsp><"new file name">,<"old file name">[, INTernal EXTernal] <"new file name">= Name of new file <"old file name">= Name of old file INTernal EXTernal = Target drive
Example	:MMEMORY:RENAME "test001.wv6","test002.wv6",INTERNAL
Explanation	This is a sequential command.

### :MMEMORY:STORE:ARESULT

Function	Stores a variety of analysis results to a specified file.
Syntax	:MMEMORY:STORE:ARESULT<wsp><"file name">[, INTernal EXTernal] <"file name"> = Name of a file to be saved INTernal EXTernal = Save destination drive
Example	:MMEMORY:STORE:ARESULT "test001",INTERNAL
Explanation	This is a sequential command.

### :MMEMORY:STORE:ATRACE

Function	Stores the specified waveform files (all traces) into traces.
Syntax	:MMEMORY:STORE:ATRACE<wsp> <"file name"> [,INTernal EXTernal] <"file name"> = Name of file be saved INTernal EXTernal = Save destination drive
Example:	MMEMORY:STORE:ATRACE "test001.csv",internal
Explanation	This is a sequential command.

### :MMEMORY:STORE:DATA

Function	Stores a variety of data to a specified file.
Syntax	:MMEMORY:STORE:DATA<wsp><"file name">[, INTernal EXTernal] <"file name"> = Name of a file to be saved INTernal EXTernal = Save destination drive
Example	:MMEMORY:STORE:DATA "test001",INTERNAL
Explanation	<ul style="list-style-type: none"> <li>• The type of data to be stored is specified using the :MMEMORY:STORE:DATA:ITEM command.</li> <li>• Whether to insert data into or overwrite the file with it when storing it is specified using the :MMEMORY:STORE:DATA:MODE command.</li> <li>• This is a sequential command.</li> </ul>

### :MMEMORY:STORE:DATA:ITEM

Function	Sets/queries an item to be used when storing data.
Syntax	:MMEMORY:STORE:DATA:ITEM<wsp> <item>,OFF ON 0 1 :MMEMORY:STORE:DATA:ITEM?<wsp> <item>
	<item> DATE = Date/time at the time of storage
	LABEL = Label
	DATA = DATA area data
	CONDITION = Setting conditions
	OWNDOW = OUTPUT WINDOW
	TRACe = Waveform data

Example	OFF = Do not save ON = Save Response 0 = OFF, 1 = ON
Explanation	:MMEMORY:STORE:DATA:ITEM TRACE,OFF :MMEMORY:STORE:DATA:ITEM? TRACE -> 0
Explanation	This is a sequential command.

### :MMEMORY:STORE:DATA:MODE

Function	Sets whether to insert data into or overwrite an existing file with the data when storing it or queries the condition of whether data is inserted or overwritten.
Syntax	:MMEMORY:STORE:DATA:MODE<wsp>ADD   OVER   0   1 :MMEMORY:STORE:DATA:MODE? ADD = Insert mode OVER = Overwrite mode
	Response 0 = ADD, 1 = OVER
Example	:MMEMORY:STORE:DATA:MODE OVER :MMEMORY:STORE:DATA:MODE? -> 1
Explanation	This is a sequential command.

### :MMEMORY:STORE:DATA:TYPE

Function	Sets/queries a file format to be used when storing data.
Syntax	:MMEMORY:STORE:DATA:TYPE<wsp>CSV   DT   0   1 :MMEMORY:STORE:DATA:TYPE? CSV = CSV storage format DT = DT6 storage format DT= Instrument-specific data type
	The AQ6370C uses DT8 format
	The AQ6373/AQ6373B uses DT9 format
	The AQ6375 uses DT7 format
Example	Response 0 = CSV, 1 = DT7 to DT9 :MMEMORY:STORE:DATA:TYPE DT8 :MMEMORY:STORE:DATA:TYPE? -> 1
Explanation	This is a sequential command.

**:MMEMory : STORe : DLOGging**

Function	Saves the data logging results to a specified file.
Syntax	:MMEMory:STORe:DLOGging<wsp><"file name">[,INTernal EXTernal] <"file name"> = Name of the file to save to INTernal EXTernal = Drive to save to
Example	:MMEMORY:STORE:DLOGGING "test001",INTERNAL
Description	<ul style="list-style-type: none"> <li>• This command is invalid when data logging is in progress.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

**:MMEMory : STORe : DLOGging : CSAVe**

Function	Sets or queries whether data logging results will be saved to a file in CSV format.
Syntax	:MMEMory:STORe:DLOGging:CSAVe<wsp>O FF ON 0 1 :MMEMory:STORe:DLOGging:CSAVe? OFF = Data will not be saved to CSV format. ON = Data will be saved to CSV format.
Response	0 = Off, 1 = On
Example	:MMEMORY:STORE:DLOGGING:CSAVE ON :MMEMORY:STORE:DLOGGING:CSAVE? -> 1
Description	<ul style="list-style-type: none"> <li>• This command is invalid when data logging is in progress.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

**:MMEMory : STORe : DLOGging : TSAVE**

Function	Sets or queries whether temporary saved waveform files will be saved when data logging results is saved.
Syntax	:MMEMory:STORe:DLOGging:TSAve<wsp>O FF ON 0 1 :MMEMory:STORe:DLOGging:TSAve? OFF: Will not be saved ON: Will be saved
Response	0 = Off, 1 = On
Example	:MMEMORY:STORE:DLOGGING:TSAVE ON :MMEMORY:STORE:DLOGGING:TSAVE? -> 1
Description	<ul style="list-style-type: none"> <li>• This command is invalid when data logging is in progress.</li> <li>• This is a sequential command.</li> <li>• This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>

**:MMEMory : STORe : GRAPhics**

Function	Stores a waveform screen to a specified graphic file.
Syntax	:MMEMory:STORe:GRAPhics<wsp>B&W COLOR PCOLOR,BMP TIFF,<"file name">[,INTernal EXTernal] B&W COLOR PCOLOR = Color mode when saving B&W = Black and white mode COLOR = Color mode PCOLOR = Preset color (waveforms in color, background in black & white)
	BMP TIFF = Saved format BMP = BMP format TIFF = TIFF format
	<"file name"> = Name of a file to be saved INTernal EXTernal = Save destination drive
Example	:MMEMORY:STORE:GRAPHICS COLOR,BMP, "test001",INTERNAL

Explanation	This is a sequential command.
-------------	-------------------------------

**:MMEMory : STORe : MEMemory**

Function	Stores a specified memory to a specified waveform file.
Syntax	:MMEMory:STORe:MEMemory<wsp><integer>,BIN CSV,<"file name">[,INTernal EXTernal] <integer> = Number of a memory whose contents are stored BIN CSV = Sav format BIN = Binary format CSV = Text format
	<"file name"> = Name of file to be saved INTernal EXTernal = Save destination drive
Example	:MMEMORY:STORE:MEMORY 1,CSV, "test001",INTERNAL
Explanation	This is a sequential command.

**:MMEMory : STORe : PROGram**

Function	Stores a specified program to a specified file.
Syntax	:MMEMory:STORe:PROGRAM<wsp><integer>,<"file name">[,INTernal EXTernal] <integer> = Number of a program whose contents are stored <"file name"> = Name of a file to be saved INTernal EXTernal = Save destination drive
Example	:MMEMORY:STORE:PRORAM 1,"test001", INTERNAL
Explanation	This is a sequential command.

## 7.6 Instrument-Specific Commands

### :MMEMORY:STORE:SETTING

Function Stores setting information to a specified file.  
Syntax :MMEMORY:STORE:SETTING<wsp><"file name">[, INTernal|EXTernal]  
<"file name"> = Name of a file to be saved  
INTernal|EXTernal = Save destination drive  
Example :MMEMORY:STORE:SETTING "test001",  
INTERNAL  
Explanation This is a sequential command.

### :MMEMORY:STORE:TEMPPlate

Function Stores specified template data to a specified file  
Syntax :MMEMORY:STORE:TEMPPlate  
<wsp><template>,<"file name">[, INTernal|EXTernal]  
<template> = Template to be saved.  
(UPPER|LOWER|TARGET)  
<"file name"> = Name of a file to be saved  
INTernal|EXTernal = Save destination drive  
Example :MMEMORY:STORE:TEMPLATE UPPER,  
"test001", INTERNAL  
Explanation This is a sequential command.

### :MMEMORY:STORE:TRACe

Function Stores a specified trace to a specified waveform file.  
Syntax :MMEMORY:STORE:TRACe<wsp><trace name>, BIN|CSV,<"file name">[, INTernal|EXTernal]  
<trace name> = Trace to be saved  
BIN|CSV = Save format  
BIN = Binary format  
CSV = Text format)  
<"file name"> = Name of file to be saved  
INTernal|EXTernal = Save destination drive  
Example :MMEMORY:STORE:TRACE TRA,CSV,  
"test001", INTERNAL  
Explanation This is a sequential command.

## PROGram Sub System Command

### :PROGRAM:EXECute

Function This key is used to execute a program that has been specified.  
Syntax :PROGRAM:EXECute<wsp><integer>  
<integer> = Number of a program to execute  
Example :PROGRAM:EXECUTE 1  
Explanation This is an overlappable command.

**SENSe Sub System Command****:SENSe:AVERage:COUNT**

Function Sets/queries the number of times averaging for each measured point.

Syntax :SENSe:AVERage:COUNT<wsp><integer>  
:SENSe:AVERage:COUNT?  
<integer> = Number of times averaging

Example: :SENSe:AVERage:COUNT 100  
:SENSe:AVERage:COUNT? -> 100

Explanation This is a sequential command.

**:SENSe:BANDwidth|:BWIDth[:RESoluti  
on]**

Function Sets/queries the measurement resolution.

Syntax :SENSe:BANDwidth|:BWIDth[:RESolutio  
n]<wsp><NRf>[M|Hz]  
:SENSe:BANDwidth|:BWIDth  
[:RESolution]?  
<NRf> = Measurement resolution [m|Hz]

Response  
    <NRf> [m|Hz] (AQ6370C/AQ6370D/  
AQ6373B/AQ6373)  
    <NRf> [m|Hz|m<sup>-1</sup>] (AQ6375)

Example :SENSe:BANDWIDTH:RESOLUTION 20PM  
:SENSe:BANDWIDTH? -> +2.0000000E-012

Explanation • For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value.  
• This is a sequential command.

**:SENSe:CHOPper**

Function Sets/queries chopper mode.

Syntax :SENSe:CHOPper<wsp>OFF|SWITCH|0|2  
:SENSe:CHOPper?

Response 0 = OFF,  
2 = SWITCH

Example :SENSe:CHOPPER SWITCH  
:SENSe:CHOPPER? -> 2

Explanation • When the measurement sensitivity setting (:SENSe:SENSe command) is NORMAL HOLD or NORMAL AUTO, Chopper does not function even if chopper mode is turned on with this command.  
• With the AQ6375, the command is invalid.  
• This is a sequential command.

**:SENSe:CORRection:LEVel:SHIFT**

Function Sets/queries the offset value for the level.

Syntax :SENSe:CORRection:LEVel:SHIFT<wsp><  
NRf>[DB]  
:SENSe:CORRection:LEVel:SHIFT?  
<NRf> = Level offset value [dB]

Example :SENSe:CORRECTION:LEVEL:SHIFT 0.2DB  
:SENSe:CORRECTION:LEVEL:SHIFT?->  
+2.0000000E-001

Explanation This is a sequential command.

**:SENSe:CORRection:RVELocity:MEedium**

Function Sets/queries whether air or vacuum is used as the wavelength reference.

Syntax :SENSe:CORRection:RVELocity:MEedium  
<wsp>AIR|VACuum|0|1  
:SENSe:CORRection:RVELocity:MEedium?  
AIR = Air is assumed to be the reference.  
VACuum = Vacuum is assumed to be the reference.  
Response 0 = AIR  
1 = VACuum

Example :SENSe:CORRECTION:RVELOCITY:  
MEDIUM VACUUM  
:SENSe:CORRECTION:RVELOCITY:MEDI  
UM?-> 1

Explanation This is a sequential command.

**:SENSe:CORRection:WAVelength:SHIFT**

Function Sets/queries the offset value for the levelwavelength.

Syntax :SENSe:CORRection:WAVelength:SHIFT<  
wsp><NRf>[M]  
:SENSe:CORRection:WAVelength:SHIFT?  
<NRf> = Wavelength offset value [m]

Example :SENSe:CORRECTION:WANELENGTH:  
SHIFT 0.05NM  
:SENSe:CORRECTION:WANELENGTH:SHI  
FT?-> +5.0000000E-011

Explanation This is a sequential command.

**:SENSe:SENSe**

Function Sets/queries the measurement sensitivity.

Syntax :SENSe:SENSe<wsp><sense>  
:SENSe:SENSe?  
<sense>= Sensitivity setting parameters

NHLD = NORMAL HOLD  
NAUT = NORMAL AUTO  
NORMAl = NORMAL  
MID = MID  
HIGH1 = HIGH1 or HIGH1/CHOP  
HIGH2 = HIGH2 or HIGH2/CHOP  
HIGH3 = HIGH3 or HIGH3/CHOP

Response 0 = NHLD  
1 = NAUT  
2 = MID  
3 = HIGH1  
4 = HIGH2  
5 = HIGH3  
6 = NORMAL

Example :SENSe:SENSE MID  
:SENSe:SENSE? -> 2

Explanation This is a sequential command.

## 7.6 Instrument-Specific Commands

### **:SENSe:SETTING:CORRection**

Function	Sets/queries the resolution correction function.
Syntax	:SENSe:SETTING:CORRection<wsp>OFF   ON 0 1 :SENSe:SETTING:CORRection? Response 0 = OFF, 1 = ON
Example	:SENSe:SETTING:CORRECTION ON :SENSe:SETTING:CORRECTION? -> 1
Explanation	• With the AQ6375, the command is invalid. • This is a sequential command.

### **:SENSe:SETTING:FCONnetcor**

Function	Sets/queries the fiber connector mode.
Syntax	:SENSe:SETTING:FCONnectoR<wsp> NORMAL ANGLeD 0 1 :SENSe:SETTING:FCONnectoR? NORMAL = Standard mode ANGLeD = Angle lap fiber mode Response 0 = NORMAL, 1 = ANGLeD
Example	:SENSe:SETTING:FCONNECTOR ANGLEd :SENSe:SETTING:FCONNECTOR? -> 1
Explanation	This is a sequential command.

### **:SENSe:SETTING:FIBer**

Function	Sets/queries the fiber core size mode.
Syntax	:SENSe:SETTING:FIBer<wsp>SMALL   LARGE 0 1 :SENSe:SETTING:FIBer? SMALL= Standard mode LARGE= Large core size fiber mode Response 0 = SMALL, 1 = LARGE
Example	:SENSe:SETTING:FIBER LARGE :SENSe:SETTING:FIBER? -> 1
Explanation	• This is a sequential command. • This command only valid for the AQ6373/AQ6373B.

### **:SENSe:SETTING:SMOoothing**

Function	Sets/queries the Smoothing function.
Syntax	:SENSe:SETTING:SMOoothing<wsp>OFF   ON 0 1 :SENSe:SETTING:SMOoothing? Response 0 = OFF, 1 = ON
Example	:SENSe:SETTING:SMOoothing ON :SENSe:SETTING:SMOoothing? -> 1
Explanation	• This is a sequential command. • This command only valid for the AQ6373/AQ6373B.

### **:SENSe:SWEep:POInTs**

Function	Sets/queries the number of samples measured.
Syntax	:SENSe:SWEep:POInTs<wsp><integer> :SENSe:SWEep:POInTs? <integer> = The number of samples to be measured
Example	:SENSe:SWEeP:POINTS 20001 :SENSe:SWEeP:POINTS? -> 20001
Explanation	• When the function of automatically setting the sampling number to be measured (SENSe:SWEep:POInTs:AUTO command) is ON, the sampling number to be measured that has been set can be queried. • When the function of automatically setting the sampling number to be measured (SENSe:SWEep:POInTs:AUTO command) is ON, this command will be automatically set to OFF. • When the sampling number to be measured is set using this command, the sampling intervals for measurements (SENSe:SWEep:STEP) will be automatically set. • With the AQ6375, if you set HIGH1–HIGH3, it becomes HIGH1/CHOP–HIGH3/CHOP. • This is a sequential command.

### **:SENSe:SWEep:POInTs:AUTO**

Function	Sets/queries the function of automatically setting the sampling number to be measured.
Syntax	:SENSe:SWEep:POInTs:AUTO<wsp>OFF   ON 0 1 :SENSe:SWEep:POInTs:AUTO? Response 0 = OFF, 1 = ON
Example	:SENSe:SWEeP:POINTS:AUTO ON :SENSe:SWEeP:POINTS:AUTO? -> 1
Explanation	• When the capability to automatically set the sampling number to be measured is set to ON using this command, the sampling number to be measured and the sampling intervals for measurements (SENSe:SWEep:STEP) will be automatically set. • This is a sequential command.

### **:SENSe:SWEep:SEGMeNT:POInTs**

Function	Sets/queries the number of sampling points to be measured at one time when performing SEGMENT MEASURE.
Syntax	:SENSe:SWEep:SEGMeNT:POInTs<wsp> <integer> :SENSe:SWEep:SEGMeNT:POInTs? <integer> = The number of samples measured
Example	:SENSe:SWEeP:SEGMENT:POINTS 100 :SENSe:SWEeP:SEGMENT:POINTS? -> 100
Explanation	This is a sequential command.

<b>:SENSe:SWEep:SPEED</b>	<b>:SENSe:SWEep:TLSSync</b>
Function Sets/queries the sweep speed.	Function Sets/queries the synchronous sweep function.
Syntax :SENSe:SWEep:SPEED<wsp>1x 2x 0 1 :SENSe:SETting:FCONnector? 1x 0: Standard 2x 1: Twice as fast as standard Response 0 = 1x, 1 = 2x	Syntax :SENSe:SWEep:TLSSync<wsp>OFF ON 0 1 :SENSe:SWEep:TLSSync? Response 0 = OFF, 1 = ON
Example :SENSe:SWEEP:SPEED 2x	Example :SENSe:SWEEP:TLSSYNC ON
Explanation • This is a sequential command. • This command can be used on the AQ6370C/AQ6370D/AQ6373B.	Explanation This is a sequential command. With the AQ6373/AQ6373B, the command is invalid.
<b>:SENSe:SWEep:STEP</b>	<b>:SENSe:WAVelength:CENTER</b>
Function Sets/queries the sampling interval for measurements.	Function Sets/queries the measurement condition center wavelength.
Syntax :SENSe:SWEep:STEP<wsp><NRf>[M] :SENSe:SWEep:STEP? <NRf> = The sampling interval for measurement [m]	Syntax :SENSe:WAVelength:CENTER<wsp><NRf>[M Hz] :SENSe:WAVelength:CENTER? <NRf> = Measurement center wavelength [m]
Example :SENSe:SWEEP:STEP 1PM	Response <NRf>[m Hz] (AQ6370C/AQ6370D/AQ6373/AQ6373B) <NRf>[m Hz m <sup>-1</sup> ] (AQ6375)
Explanation • When the function of automatically setting the sampling interval for measurement (SENSe:SWEep:POINTS:AUTO command) is ON, the sampling number to be measured that has been set can be queried. • When the function of automatically setting the sampling number to be measured (SENSe:SWEep:POINTS:AUTO command) is ON, this command will be automatically set to OFF. • When the sampling interval for measurement is set using this command, the sampling intervals for measurements (SENSe:SWEep:POINTS) will be automatically set. • This is a sequential command.	Example :SENSe:WAVELENGTH:CENTER 1550.000NM :SENSe:WAVELENGTH:CENTER?-> +1.55000000E-006
<b>:SENSe:SWEep:TIME:0NM</b>	Explanation • For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value. • This is a sequential command.
Function Sets/queries the time taken from the start to the end of measurements when measurement is made in the 0-nm sweep mode.	<b>:SENSe:WAVelength:SPAN</b>
Syntax :SENSe:SWEep:TIME:0NM<wsp><integer>[SEC] :SENSe:SWEep:TIME:0NM? <integer> = Measurement time [sec] (0 = MINIMUM)	Function Sets/queries the measurement condition measurement span.
Example :SENSe:SWEEP:TIME:0NM 10SEC	Syntax :SENSe:WAVelengthSPAN<wsp><NRf>[M Hz] :SENSe:WAVelength:SPAN? <NRf> = Measurement span [m]
Explanation • This is a sequential command.	Response <NRf>[m Hz] (AQ6370C) <NRf>[m Hz m <sup>-1</sup> ] (AQ6375)
<b>:SENSe:SWEep:TIME:INTerval</b>	Example :SENSe:WAVELENGTH:SPAN 20.0NM :SENSe:WAVELENGTH:SPAN?-> +2.00000000E-008
Function Sets/queries the time taken from the start of a sweep to that of the next sweep when repeat sweeps are made.	Explanation • For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value. • This is a sequential command.
Syntax :SENSe:SWEep:TIME:INTerval<wsp><integer>[SEC] :SENSe:SWEep:TIME:INTerval? <integer> = Measurement time [sec] (0 = MINIMUM)	
Example :SENSe:SWEEP:TIME:INTERVAL 100sec	
Explanation • This is a sequential command.	

## 7.6 Instrument-Specific Commands

### :SENSe:WAVelength:SRAnge

Function	Sets/queries whether to limit a sweep range to the spacing between line markers L1 and L2.
Syntax	:SENSe:WAVelength:SRAnge<wsp>OFF ON 0 1 :SENSe:WAVelength:SRAnge? Response 0 = OFF, 1 = ON
Example	:SENSe:WAVELENGTH:SRANGE ON :SENSe:WAVELENGTH:SRANGE? -> 1
Explanation	This is a sequential command.

### :SENSe:WAVelength:START

Function	Sets/queries the measurement condition measurement start wavelength.
Syntax	:SENSe:WAVelength:START<wsp><NRf> [M HZ] :SENSe:WAVelength:START? <NRf>=Measurement center wavelength [m] Response <NRf> [m Hz] (AQ6370C/AQ6370D/ AQ6373/AQ6373B) <NRf> [m Hz m <sup>-1</sup> ] (AQ6375)
Example	:SENSe:WAVELENGTH:START 1540.000NM :SENSe:WAVELENGTH:START?-> +1.5400000E-006
Explanation	• For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value. • This is a sequential command.

### :SENSe:WAVelength:STOP

Function	Sets/queries the measurement condition measurement stop wavelength.
Syntax	:SENSe:WAVelengthSTOP<wsp><NRf> [M HZ] :SENSe:WAVelength:STOP? <NRf> = Measurement stop wavelength [m] Response <NRf> [m Hz] (AQ6370C/AQ6370D/ AQ6373/AQ6373B) <NRf> [m Hz m <sup>-1</sup> ] (AQ6375)
Example	:SENSe:WAVELENGTH:STOP 1560.000NM :SENSe:WAVELENGTH:STOP?-> +1.5600000E-006
Explanation	• For the AQ6375, to set using the wavenumber, do not add any units when in Wavenumber mode, and just enter the numerical value. • This is a sequential command.

## STATUS Sub System Command

### :STATus:OPERation:CONDition?

Function	Queries the contents of the operation status condition register.
Syntax	:STATus:OPERation:CONDiton?
Example	:STATus:OPERATION:CONDITION? -> 1
Explanation	This is a sequential command.

### :STATus:OPERation:ENABLE

Function	Queries the contents of the operation status Enable register.
Syntax	:STATus:OPERation:ENABLE<wsp> <integer> :STATus:OPERation:ENABLE? <integer> = Contents of the operation status enable register
Example	:STATus:OPERATION:ENABLE 8 :STATus:OPERATION:ENABLE? -> 8
Explanation	This is a sequential command.

### :STATus:OPERation[:EVENT]?

Function	Queries the contents of the operation status Event register.
Syntax	:STATus:OPERation[:EVENT]?
Example	:STATus:OPERATION? -> 1

Explanation This is a sequential command.

### :STATus:PRESet

Function	Clears the event register and sets all bits of the enable register.
Syntax	:STATus:PRESet
Example	:STATus:PRESET
Explanation	• When this command is executed, the registers will be affected as follows. • The operation status event register is cleared to “0.” • All bits of the operation status enable register are set to “0.” • The questionable status event register is cleared to “0.” • All bits of the questionable status enable register are set to “0.” • Even when this command is executed, the standard event status register and standard event status enable register do not change. • This is a sequential command.

<b>:STATus:QUESTIONable:CONDition?</b>	
Function	Queries the contents of the questionable status condition register.
Syntax	:STATus:QUESTIONable:CONDiton?
Example	:STATUS:QUESTIONABLE:CONDITION? -> 1
Explanation	This is a sequential command.
<b>:STATus:QUESTIONable:ENABLE</b>	
Function	Reads the contents of the questionable status enable register or writes data to this register.
Syntax	:STATus:QUESTIONable:ENABLE<wp><integer> :STATus:QUESTIONable:ENABLE? <integer> = Contents of the questionable status enable register
Example	:STATUS:QUESTIONABLE:ENABLE 8 :STATUS:QUESTIONABLE:ENABLE? -> 8
Explanation	This is a sequential command.
<b>:STATus:QUESTIONable[:EVENT]?</b>	
Function	Reads the contents of the questionable status event register.
Syntax	:STATus:QUESTIONable[:EVENT]?
Example	:STATUS:QUESTIONABLE:? -> 1
Explanation	This is a sequential command.

## SYStem Sub System Command

### :SYSTem:BUZZer:CLICK

Function	Sets/queries whether to sound the buzzer when clicked the key.
Syntax	:SYSTem:BUZZer:CLICK<wp>OFF ON 0 1
	:SYSTem:BUZZer:CLICK?
	Response 0 = OFF, 1 = ON
Example	:SYSTEM:BUZZER:CLICK ON
	:SYSTEM:BUZZER:CLICK? -> 1
Explanation	This is a sequential command.

### :SYSTem:BUZZer:WARNING

Function	Sets/queries whether to sound the buzzer during an alarm.
Syntax	:SYSTem:BUZZer:WARNING<wp>OFF ON 0 1
	:SYSTem:BUZZer:WARNING?
	Response 0 = OFF, 1 = ON
Example	:SYSTEM:BUZZER:WARNING ON
	:SYSTEM:BUZZER:WARNING? -> 1
Explanation	This is a sequential command.

### :SYSTem:COMMUnicate:CFORmat

Function	Sets/queries the GP-IB command format of this unit.
Syntax	:SYSTem:COMMUnicate:CFORmat<wp><mode> :SYSTem: COMMUnicate:CFORmat? <mode> = GP-IB command format
	For AQ6370C AQ6317 = AQ6317 compatible mode
	AQ6370 = AQ6370C mode
	AQ6370C = AQ6370C mode
	For AQ6370D AQ6317 = AQ6317 compatible mode AQ6370D = AQ6370D mode
	For AQ6373 AQ6317 = AQ6317 compatible mode AQ6373 = AQ6373 mode
	For AQ6373B AQ6317 = AQ6317 compatible mode AQ6373B = AQ6373B mode
	For AQ6375 AQ6317 = AQ6317 compatible mode AQ6375 = AQ6375 mode
Response	0 = AQ6317, 1 = AQ6370C (For AQ6370C) 0 = AQ6317, 1 = AQ6373 (For AQ6373) 0 = AQ6317, 1 = AQ6370D (For AQ637D) 0 = AQ6317, 1 = AQ6375 (For AQ6375)
Example	:SYSTEM:COMMUNICATE:CFORMAT AQ6370C syst:comm:cformat? -> 1
Explanation	• This command is valid when in AQ6370C/AQ6373/AQ6373B/AQ6375 mode. This command results in an error when in AQ6317 compatible mode.

## 7.6 Instrument-Specific Commands

- To set the GP-IB command format while this unit is in the AQ6317-compatible mode, use the following commands.
 

Control command  
CFORM\* (\*: 0 = AQ6317 compatible mode, 1 = AQ6370C/AQ6373/AQ6373B/AQ6375 mode)

Query command  
CFORM? (return value: 0 = AQ6317-compatible mode, 1 = AQ6370C/AQ6373/AQ6373B/AQ6375 mode)
- To use a GP-IB command to place this unit into the AQ6317-compatible mode, regardless of the status during execution of the command, execute the following command. Note that if this unit has already been in the AQ6317-compatible mode at the time of executing this command, a command error occurs, but you can ignore it.  
:SYSTem:COMMUnicatE:CFORmat<wsp>AQ6317
- To use a GP-IB command to place this unit into the AQ6370C, AQ6373, AQ6373B or AQ6375 mode, regardless of the status during execution of the command, execute the following command. Note that if this unit has already been in the AQ6370C, AQ6370D, AQ6373, AQ6373B or AQ6375 mode at the time of executing this command, a command error occurs, but you can ignore it.  
CFORM1  
• This is a sequential command.

### :SYSTem:COMMUnicatE:GP-IB2:ADDReSS

- Function Sets/queries the GP-IB address of the instrument's GP-IB2 port.
- Syntax :SYSTem:COMMUnicatE:GP-IB2:ADDReSS <wsp><integer>  
:SYSTem:COMMUnicatE:GP-IB2:ADDReSS?
- Example :SYSTEM:COMMUNICATE:GP-IB2:  
ADDRESS 2  
:SYSTEM:COMMUNICATE:GP-  
IB2:ADDRESS?-> 2
- Explanation • This is a sequential command.  
• With the AQ6370D/AQ6373B, the command is invalid.

### :SYSTem:COMMUnicatE:GPIB2:SConTroller

- Function Sets/queries whether the system controller function of the instrument's GP-IB2 port is enabled.
- Syntax :SYSTem:COMMUnicatE:GPIB2:SConTroller<wsp>OFF|ON|0|1  
:SYSTem:COMMUnicatE:GPIB2:SConTroller?  
OFF|0: Disables the system controller function  
ON|1: Enables the system controller function
- Example :SYSTEM:COMMUNICATE:GPIB2:SCon ON  
:SYSTEM:COMMUNICATE:GPIB2:SCon? ->  
1
- Explanation • To use the instrument's GP-IB2 port as a system controller in performing a synchronous sweep with a variable wavelength light source, enable this setting.  
• This is a sequential command.  
• With the AQ6370D/AQ6373B, the command is invalid.

### :SYSTem:COMMUnicatE:GP-IB2:TLS:ADDReSS

- Function Sets/queries the GP-IB address of the turnable laser source connected to the instrument's GP-IB2 port.
- Syntax :SYSTem:COMMUnicatE:GP-  
IB2:TLS:ADDReSS<wsp><integer>  
:SYSTem:COMMUnicatE:GP-  
IB2:TLS:ADDReSS?  
<integer> = GP-IB address of the turnable laser source
- Example :SYSTEM:COMMUNICATE:GP-  
IB2:TLS:ADDRESS 20  
:SYSTEM:COMMUNICATE:GP-  
IB2:TLS:ADDRESS? -> 20
- Explanation • Sets the address of the Tunable Laser Source.  
• This is a sequential command.  
• With the AQ6373 or AQ6370D, the command is invalid.

### :SYSTem:COMMUnicatE:LOCKout

- Function Sets/cancels local lockout.
- Syntax :SYSTem:COMMUnicatE:LOCKout<wsp>  
OFF|ON|0|1  
:SYSTem:COMMUnicatE:LOCKout?  
OFF|0: Cancels local lockout  
ON|1: Sets local lockout
- Example :SYSTEM:COMMUNICATE:LOCKOUT OFF  
:SYSTEM:COMMUNICATE:LOCKOUT? -> 0
- Explanation • This command is valid when the remote interface is the Ethernet interface. An interface message is available for the GP-IB interface.  
• During local lockout, if the Ethernet connection is lost, the instrument switches to local mode, regardless of the local lockout status.  
• This is a sequential command.  
• This command can be used on the AQ6370C.

<b>:SYSTem:COMMUnicAtE:RMONitor</b>	
Function	Sets/queries whether the remote monitor function is enabled.
Syntax	:SYSTem:COMMUnicAtE:RMONitor<wsp> OFF ON 0 1 :SYSTem:COMMUnicAtE:RMONitor? OFF 0: Disables the remote monitor function ON 1: Enables the remote monitor function
Example	:SYSTEM:COMMUNICATE:RMONITOR OFF :SYSTEM:COMMUNICATE:RMONITOR? -> 0
Explanation	<ul style="list-style-type: none"> <li>This is a sequential command.</li> <li>This command can be used on the AQ6370C/AQ6370D/AQ6373B.</li> </ul>
<b>:SYSTem:DATE</b>	
Function	Sets/queries the system data.
Syntax	:SYSTem:DATE<wsp><year>,<month>,<day> :SYSTem:DATE? <year> = Year <month> = Month <day> = Day
Example	:SYSTEM:DATE 2006,03,01 :SYSTEM:DATE? -> 2006,03,01
Explanation	This is a sequential command.
<b>:SYSTem:DISPlay:TRANspArent</b>	
Function	Sets/queries whether to make the Interrupt Window and OVERVIEW Window of the measurement screen semi-transparent.
Syntax	:SYSTem:DISPlay:TRANspArent<wsp>OFF ON 0 1 :SYSTem:DISPlay:TRANspArent? Response 0 = OFF, 1 = ON
Example	:SYSTEM:DISPLAY:TRANSPARENT OFF :SYSTEM:DISPLAY:TRANSPARENT? -> 0
Explanation	This is a sequential command.
<b>:SYSTem:DISPlay:UNCal</b>	
Function	Sets/queries whether to display an alarm message in the event of UNCAL.
Syntax	:SYSTem:DISPlay:UNCal<wsp>OFF ON 0 1 :SYSTem:DISPlay:UNCal? Response 0 = OFF, 1 = ON
Example	:SYSTEM:DISPLAY:UNCAL OFF :SYSTEM:DISPLAY:UNCAL? -> 0
Explanation	This is a sequential command.
<b>:SYSTem:ERRor[:NEXT]?</b>	
Function	Queries data in an error queue and deletes it from the queue.
Syntax	:SYSTem:ERRor[:NEXT]? <integer> = Error number
Example	:SYSTEM:ERROR? -> 100
Explanation	This is a sequential command.

<b>:SYSTem:GRID</b>	
Function	Sets/queries the instrument's grid setting.
Syntax	:SYSTem:GRID<wsp><grid> :SYSTem:GRID? <grid> = Grid setting 12.5 GHZ = 12.5 GHz Spacing 25 GHZ = 25 GHz Spacing 50 GHZ = 50 GHz Spacing 100 GHZ = 100 GHz Spacing 200 GHZ = 200 GHz Spacing CUSTom = User setting
Response	0 = 12.5GHz 1 = 25GHz 2 = 50GHz 3 = 100GHz 4 = 200GHz 5 = CUSTom
Example	:SYSTEM:GRID 50GHZ :SYSTEM:GRID? -> 2
Explanation	<ul style="list-style-type: none"> <li>This is a sequential command.</li> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>For the AQ6375, cannot be executed when in Wavenumber mode.</li> </ul>
<b>:SYSTem:GRID:CUSTOM:CLEar:ALL</b>	
Function	Clears the user-specified custom grid and returns it to the default value.
Syntax	:SYSTem:GRID:CUSTOM:CLEar:ALL
Example	:SYSTEM:GRID:CUSTOM:CLEar:ALL
Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>For the AQ6375, cannot be executed when in Wavenumber mode.</li> <li>This is a sequential command.</li> </ul>
<b>:SYSTem:GRID:CUSTOM:DElete</b>	
Function	Deletes the specified grid of the custom grid.
Syntax	:SYSTem:GRID:CUSTOM:DElete<wsp><integer> <integer> = Number of a grid to be deleted
Example	:SYSTEM:GRID:CUSTOM:DELETE 10
Explanation	<ul style="list-style-type: none"> <li>With the AQ6373/AQ6373B, the command is invalid.</li> <li>For the AQ6375, cannot be executed when in Wavenumber mode.</li> <li>This is a sequential command.</li> </ul>

## 7.6 Instrument-Specific Commands

### **:SYSTem:GRID:CUSTom:INSeRt**

**Function** Inserts a new grid when the grid setting is in the custom grid.

**Syntax** :SYSTem:GRID:CUSTom:INSeRt<wsp><NRf> [M|HZ]  
<NRf> = Grid wavelength/frequency to be inserted [m|Hz]

**Example** :SYSTem:GRID:CUSTom:INSERT  
1550.123NM

**Explanation** • When :SYSTem:GRID is CUSTom, an execution error occurs.  
• With the AQ6373/AQ6373B, the command is invalid.  
• For the AQ6375, cannot be executed when in Wavenumber mode.  
• This is a sequential command.

### **:SYSTem:GRID:CUSTom:SPACing**

**Function** Sets/queries the grid spacing of the custom grid.

**Syntax** :SYSTem:GRID:CUSTom:SPACing<wsp><NRf>[GHZ]  
:SYSTem:GRID:CUSTom:SPACing?  
<NRf> = Grid spacing [GHz]

**Example** :SYSTem:GRID:CUSTom:SPACING 12.5  
:SYSTem:GRID:CUSTom:SPACING?->  
+1.25000000E+001

**Explanation** • When :SYSTem:GRID is CUSTom, an execution error occurs.  
• With the AQ6373/AQ6373B, the command is invalid.  
• For the AQ6375, cannot be executed when in Wavenumber mode.  
• This is a sequential command.

### **:SYSTem:GRID:CUSTom:STARt**

**Function** Sets/queries the custom grid start wavelength.

**Syntax** :SYSTem:GRID:CUSTom:STARt<wsp><NRf> [M|HZ]  
:SYSTem:GRID:CUSTom:STARt?  
<NRf> = Grid start wavelength [m|Hz]

**Example** :SYSTem:GRID:CUSTom:STARt  
1550.000NM  
:SYSTem:GRID:CUSTom:STARt?->  
+1.55000000E-006

**Explanation** • When :SYSTem:GRID is CUSTom, an execution error occurs.  
• With the AQ6373/AQ6373B, the command is invalid.  
• For the AQ6375, cannot be executed when in Wavenumber mode.  
• This is a sequential command.

### **:SYSTem:GRID:CUSTom:STOP**

**Function** Sets/queries the custom grid stop wavelength.

**Syntax** :SYSTem:GRID:CUSTom:STOP<wsp><NRf> [M|HZ]  
:SYSTem:GRID:CUSTom:STOP?  
<NRf> = Grid stop wavelength [m|Hz]

**Example** :SYSTem:GRID:CUSTom:STOP 1560.000NM  
:SYSTem:GRID:CUSTom:STOP?->  
+1.56000000E-006

**Explanation** • When :SYSTem:GRID is something other than CUSTom, an execution error occurs.  
• With the AQ6373/AQ6373B, the command is invalid.  
• For the AQ6375, cannot be executed when in Wavenumber mode.  
• This is a sequential command.

### **:SYSTem:GRID:REFerence**

**Function** Sets/queries the reference frequency of the instrument's grid setting.

**Syntax** :SYSTem:GRID:REFerence<wsp><NRf> [HZ]  
:SYSTem:GRID:REFerence?  
<NRf> = Grid's reference frequency [Hz]

**Example** :SYSTem:GRID:REFERENCE 193.1000HZ  
:SYSTem:GRID:REFERENCE ?->  
+1.93000000E+014

**Explanation** • With the AQ6373/AQ6373B, the command is invalid.  
• For the AQ6375, cannot be executed when in Wavenumber mode.  
• This is a sequential command.

### **:SYSTem:INformation?**

**Function** Queries model-specific information (the model code and special code)

**Syntax** :SYSTem:INformation?<wsp><integer>  
<integer> = The type of instrument specific information to obtain  
0 = MODEL code  
1 = SPECIAL code

**Example** :SYSTEM:INFORMATION? 0 ->  
AQ6370C-M/  
FC/RFC/B5

**Example** :SYSTEM:INFORMATION? 1 ->  
AQ6370C-M/

**Explanation** • Outputs model-specific information (the model code and special code)  
• If no SPECIAL mode is present, "NONE" is returned.  
• This is a sequential command.

**:SYSTem:PRESet**

Function   Initializes the unit status.  
 Syntax   :SYSTem:PRESet  
 Example   :SYSTEM:PRESET  
 Explanation This is a sequential command.

**:SYSTem:TIME**

Function   Sets/queries the system time.  
 Syntax   :SYSTem:TIME<wsp><hour>,<minute>,<second>  
           :SYSTem:TIME?  
           <hour> = Hour  
           <minute> = Minute  
           <second> = Second  
 Example   :SYSTEM:TIME 22,10,01  
           :SYSTEM:TIME? -> 22,10,1  
 Explanation This is a sequential command.

**:SYSTem:VERSion?**

Function   Queries the SCPI compatibility version of this unit.  
 Syntax   :SYSTem:VERSion?  
 Example   :SYSTEM:VERSION? -> 1999.0  
 Explanation This is a sequential command.

**TRACe Sub System Command****:TRACe:ACTive**

Function   Sets/queries the active trace.  
 Syntax   :TRACe:ACTive<wsp><trace name>  
           :TRACe:ACTIVE?  
           <trace name> = Active trace  
           (TRA|TRB|TRC|TRD|TRE|TRF|TRG)  
 Example   :TRACE:ACTIVE TRA  
           :TRACE:ACTIVE? -> TRA  
 Explanation This is a sequential command.

**:TRACe:ATTRibute[:<trace name>]**

Function   Sets/queries the attributes of the specified trace.  
 Syntax   :TRACe:ATTRibute[:<trace name>]  
           <wsp><attribute>  
           :TRACe:ATTRibute[:<trace name>]?  
           <trace name> = trace  
           (TRA|TRB|TRC|TRD|TRE|TRF|TRG)  
           <attribute> = Attribute  
             WRITe = WRITE  
             FIX = FIX  
             MAX = MAX HOLD  
             MIN = MIN HOLD  
             RAVG = ROLL AVG  
             CALC = CALC  
 Response 0 = WRITe  
           1 = FIX  
           2 = MAX  
           3 = MIN  
           4 = RAVG  
           5 = CALC

Example   :TRACE:ATTRIBUTE:TRA WRITE  
           :TRACE:ATTRIBUTE:TRA? -> 0

Explanation • If <trace name> is omitted, the command is executed with respect to the active trace.  
 • If <trace name> is specified, the specified trace is set as the active trace after the command is executed.  
 • When the attribute is set to a CALC trace, the expression is set using the :CALCulate:MATH command.  
 • This is a sequential command.

## 7.6 Instrument-Specific Commands

### :TRACe:ATTRibute:RAVG[:<trace name>]

Function	Sets/queries the number of times for averaging of the specified trace.
Syntax	:TRACe:ATTRibute:RAVG[:<trace name>]<wsp><integer> :TRACe:ATTRibute:RAVG[:<trace name>]? <trace name> = trace (TRA TRB TRC TRD TRE TRF TRG) <integer> = Number of times averaging of ROLL AVG
Example	:TRACE:ATTRIBUTE:RAVG:TRA 10 :TRACE:ATTRIBUTE:RAVG:TRA? -> 10
Explanation	<ul style="list-style-type: none"> <li>When this command is executed, the attribute of the set trace goes to ROLL AVG.</li> <li>If &lt;trace name&gt; is omitted, the command is executed with respect to the active trace.</li> <li>If &lt;trace name&gt; is specified, the specified trace is set as the active trace after the command is executed.</li> <li>This is a sequential command.</li> </ul>

### :TRACe:COPY

Function	Copies the data of a specified trace to another trace.
Syntax	:TRACe:COPY<wsp><source trace name>,<destination trace name> <source trace name> = Copy source trace <destination trace name> = Copy trace destination
Example	:TRACE:COPY TRA,TRB
Explanation	This is a sequential command.

### :TRACe[:DATA]:SNUMBER?

Function	Sets/queries the number of data sampled of the specified trace.
Syntax	:TRACe[:DATA]:SNUMBER?<wsp><trace name> <trace name> = Trace from which to acquire data
Example	:TRACE:DATA:SNUMBER? -> 50001
Explanation	<ul style="list-style-type: none"> <li>If a specified trace has no data, "0" is returned.</li> <li>This is a sequential command.</li> </ul>

### :TRACe[:DATA]:X?

Function	Queries the wavelength axis data of the specified trace.
Syntax	:TRACe[:DATA]:X?<wsp><trace name> <start point>,<stop point> <trace name> = Trace to be transferred (TRA TRB TRC TRD TRE TRF TRG) <start point> = A range of samples to be transferred (starting point) (1 to 50001) <stop point> = A range of samples to be transferred (stopping point) (1 to 50001)
Example	:TRACE:X? TRA -> +1.5500000E-006,+1.55001000E-006,+1.55002000E-006,.....
Explanation	<ul style="list-style-type: none"> <li>Data is output in the unit of wavelength value (m), regardless of whether this unit is in the wavelength mode or in the frequency mode.</li> <li>If the parameter &lt;start point&gt; or &lt;stop point&gt; is omitted, all sampling data of a specified trace will be output.</li> </ul> <p>The number of output data can be acquired by executing :TRACe[:DATA]:SNUMBER?.</p> <ul style="list-style-type: none"> <li>Data is output in either ASCII or binary form, depending on the setting of :FORMAT[:DATA].</li> <li>This is a sequential command.</li> </ul>

### :TRACe[:DATA]:Y?

Function	Queries the level axis data of specified trace.
Syntax	:TRACe[:DATA]:Y?<wsp><trace name> <start point>,<stop point> <trace name> = Trace to be transferred (TRA TRB TRC TRD TRE TRF TRG) <start point> = A range of samples to be transferred (starting point) (1 to 50001) <stop point> = A range of samples to be transferred (stopping point) (1 to 50001)
Example	Response For ASCII data: <NRF>,<NRF>,...<NRF> For BINARY data: '#<integer><byte num><data byte>
Explanation	<ul style="list-style-type: none"> <li>The data is output in order of its wavelength from the shortest level to the longest, irrespective of the wavelength/frequency mode.</li> <li>When the level scale is LOG, data is output in LOG values.</li> <li>When the level scale is Linear, data is output in linear values.</li> <li>If the parameter &lt;start point&gt; or &lt;stop point&gt; is omitted, all sampling data of a specified trace will be output.</li> </ul> <p>The number of output data can be acquired by executing :TRACe[:DATA]:SNUMBER?.</p> <ul style="list-style-type: none"> <li>Data is output in either ASCII or binary form, depending on the setting of :FORMAT[:DATA].</li> <li>This is a sequential command.</li> </ul>

**:TRACe[:DATA]:Y:PDENsity?**

Function	Queries the power density trace data.
Syntax	:TRACe[:DATA]:Y:PDENsity? <wsp><trace name>,<NRf>[m] [, <start point>,<stop point> <trace name> = Computation source trace <NRf> = Normalization bandwidth [m] <start point> = Sample range to transfer (start point) (1 to 50001) <stop point> = Sample range to transfer (stop point) (1 to 50001)
Example	:trac:y:pden? tra,0.1nm -> -5.36017335E+001, -5.36143380E+001, -5.34441639E+001,....
Description	<ul style="list-style-type: none"> <li>• When the level scale is set to LOG, LOG values will be output.</li> <li>• When the level scale is set to linear, linear values will be output.</li> <li>• If the &lt;start point&gt; and &lt;stop point&gt; parameters are omitted, the entire sample data of the specified trace will be output.</li> <li>• The data is output in ASCII or BINARY format according to the :FORMat[:DATA] setting.</li> <li>• This command is for the AQ6370D.</li> <li>• This is a sequential command.</li> </ul>

**:TRACe:DElete**

Function	Deletes the data of a specified trace.
Syntax	:TRACe:DElete<wsp><trace name> <trace name> = Trace to be transferred (TRA TRB TRC TRD TRE TRF TRG)
Example	:TRACE:DELETE TRA
Explanation	This is a sequential command.

**:TRACe:DElete:ALL**

Function	Clears the data for all traces.
Syntax	:TRACE:DELETE:ALL
Example	:TRACE:DELETE:ALL
Explanation	This is a sequential command.

**:TRACe:STATe[:<trace name>]**

Function	Sets/queries the display status of the specified trace.
Syntax	:TRACe:STATe[:<trace name>]<wsp>OFF ON 0 1 :TRACe:ACTive? <trace name> = Trace to be transferred (TRA TRB TRC TRD TRE TRF TRG) OFF = Hide trace (BLANK) ON = Makes trace visible (DISP). Response 0 = OFF, 1 = ON
Example	:TRACE:STATE OFF :TRACE:STATE OFF? -> 0
Explanation	<ul style="list-style-type: none"> <li>• If &lt;trace name&gt; is omitted, the command is executed with respect to the active trace.</li> <li>• If &lt;trace name&gt; is specified, the specified trace is set as the active trace after the command is executed.</li> <li>• This is a sequential command.</li> </ul>

**TRACe:TEMPLe:DATA**

Function	Adds data to the specified template or queries the data.
Syntax	:TRACe:TEMPLe:DATA<wsp><template>,<wavelength>[M],<level>[dB] :TRACe:TEMPLe:DATA?<wsp><template> <template> = Template (UPPer LOWer TARGet) <wavelength> = Wavelength of template data to be added [nm] <level> = Lvl. of template data added [dB] Response <integer>,<wavelength>,<level>,<wavelength>,<level>, ... ,<level> <integer> = Number of data points <wavelength> = wavelength value [m] <level> = Level value [dB]
Example	:TRACE:TEMPLe:DATA TARGET,1550NM,-10dbm :TRACE:TEMPLe:DATA? TARGET -> 3,+1.54000000E-006,-1.00000000E+001,+1.54500000E-006,-5.00000000E+000,+1.55000000E-006,-1.00000000E+001
Explanation	<ul style="list-style-type: none"> <li>• Adds data to a specified template.</li> <li>• After data has been added, it will be sorted by wavelength.</li> <li>• If data exceeding the maximum number of template data is added, an execution error occurs.</li> <li>• This is a sequential command.</li> </ul>

## 7.6 Instrument-Specific Commands

### **:TRACe:TEMPLeT:DATA:ADElete**

Function Deletes all data of a specified template.  
 Syntax :TRACe:TEMPLeT:DATA:ADElete<wsp><template>  
           <template> = Template  
                  (UPPer|LOWer|TARGET)  
 Example :TRACE:TEMPLATE:DATA:ADELETE TARGET  
 Explanation • Deletes all data of a specified template.  
 • This is a sequential command.

### **:TRACe:TEMPLeT:DATA:ETYPe**

Function Sets/queries the extrapolation mode of the specified template.  
 Syntax :TRACe:TEMPLeT:DATA:ETYPe<wsp><template>, <type>  
           <template> = Template (UPPer | LOWER | TARGET)  
           <type> = Extrapolation type  
                  A = Extrapolation type A  
                  B = Extrapolation type B  
                  NONE = No extrapolation  
 Response 0 = NONE, 1 = A, 2 = B  
 Example :TRACE:TEMPLATE:DATA:ETYPe  
           TARGET, NONE  
           :TRACE:TEMPLATE:DATA:ETYPe? target  
           -> NONE  
 Explanation This is a sequential command.  
 Parameter: Response ex. Same as the above

### **:TRACe:TEMPLeT:DATA:MODE**

Function Sets/queries the absolute value mode/relative value mode of the specified template.  
 Syntax :TRACe:TEMPLeT:DATA:MODE<wsp><template>, <mode>  
           <template> = Template  
                  (UPPer|LOWer|TARGET)  
           <mode> = Mode (ABSolute | RELative)  
                  ABSolute = Absolute value mode  
                  RELative = Relative value mode  
 Response 0 = ABSolute, 1 = RELative  
 Example :TRACE:TEMPLATE:DATA:MODE  
           TARGET, RELATIVE  
           :TRACE:TEMPLATE:DATA:MODE? TARGET  
           -> REL  
 Explanation This is a sequential command.

### **:TRACe:TEMPLeT:DISPlay**

Function Sets/queries display ON/OFF for the specified template.  
 Syntax :TRACe:TEMPLeT:DISPlay<wsp><template>, OFF|ON|0|1  
           :TRACe:TEMPLeT:DISPlay?<wsp><template>  
           <template> = Template  
                  (UPPer|LOWer|TARGET)  
           OFF = Display OFF  
           ON = Display ON  
 Response 0 = OFF, 1 = ON  
 Example :TRACE:TEMPLATE:DISPLAY TARGET, OFF  
           :TRACE:TEMPLATE:DISPLAY? TARGET-> 0  
 Explanation This is a sequential command.

### **:TRACe:TEMPLeT:GONoGo**

Function Sets or acquires ON/OFF of the go/no-go decision function of the template function.  
 Syntax :TRACe:TEMPLeT:GONoGo<wsp>OFF|ON|0|1  
           :TRACe:TEMPLeT:GONoGo?  
           OFF = Judgement function OFF  
           ON = Judgment function ON  
 Response 0 = OFF, 1 = ON  
 Example :TRACE:TEMPLATE:GONOGo OFF  
           :TRACE:TEMPLATE:GONOGo? -> 0  
 Explanation This is a sequential command.

### **:TRACe:TEMPLeT:LEVel:SHIfT**

Function Sets/queries the amount of level shift for the template.  
 Syntax :TRACe:TEMPLeT:LEVel:SHIfT<wsp><NRf>[dB]  
           :TRACe:TEMPLeT:LEVel:SHIfT?  
           <NRf> = Level shift amount [dB]  
 Example :TRACE:TEMPLATE:LEVEL:SHIFT -1db  
           :TRACE:TEMPLATE:LEVEL:SHIFT?->  
           -1.0000000E+000  
 Explanation This is a sequential command.

### **:TRACe:TEMPLeT:REsult?**

Function Queries the results of go/no-go decision of the template function.  
 Syntax :TRACe:TEMPLeT:REsult?  
           Response 0= No go, 1= Go  
 Example :TRACE:TEMPLATE:RESULT? -> 1  
 Explanation This is a sequential command.

**:TRACe :TEMPplate:TTYPE**

**Function** Sets/queries judgement type of the go/no-go decision function of the template function.

**Syntax** :TRACe :TEMPplate:TTYPE<wsp><type>  
:TRACe :TEMPplate:TTYPE?  
<type>=Judgement type  
    UPPer = Judge Upper line only  
    LOWer = Judge Lower line only  
    U&L = Judge both Upper and LOWER line  
Response 0 = UPPer, 1 = LOWer, 2 = U&L

**Example** :TRACE:TEMPLATE:TTYPE U&L  
:TRACE:TEMPLATE:TTYPE? -> 2

**Explanation** This is a sequential command.

**:TRACe :TEMPplate:WAVelength:SHIFT**

**Function** Sets/queries the amount of wavelength shift for the template.

**Syntax** :TRACe :TEMPplate:WAVelength:SHIFT<wsp><NRf>[M]  
:TRACe :TEMPplate:WAVelength:SHIFT?  
<NRf> = Amount of a wavelength shift [m]

**Example** :TRACE:TEMPLATE:WAVELENGTH:  
SHIFT -5NM  
:TRACE:TEMPLATE:WAVELENGTH:SHIFT?  
-> -5.0000000E-009

**Explanation** This is a sequential command.

**TRIGger Sub System Command****:TRIGger [:SEQUence] :DELay**

**Function** Sets/queries the trigger delay.

**Syntax** :TRIGger[:SEQUence]:DELay<wsp><NRf>[S]  
:TRIGger[:SEQUence]:DELay?  
<NRf> = delay [sec]

**Example** :TRIGER:DELAY 100.0US  
:TRIGER:DELAY? -> +1.0000000E-004

**Explanation** • When this command is executed, the external trigger mode becomes enabled.  
• (TRIGger[:SEQUence]:STATe ON)  
• This is a sequential command.

**:TRIGger [:SEQUence] :GATE:ITIMe**

**Function** Sets or queries sampling interval for gate sampling.

**Syntax** :TRIGger[:SEQUence]:GATE:ITIMe<wsp><NRf>[S]  
:TRIGger[:SEQUence]:GATE:ITIMe?  
<NRf> = Sampling interval

**Example** :TRIGGER:SEQUENCE:GATE:ITIME 100ms  
:TRIGGER:SEQUENCE:GATE:ITIME? ->  
+1.0000000E-001

**Description** • This is a sequential command.  
• This command can be used on the AQ6370C/AQ6370D/AQ6373B.

**:TRIGger [:SEQUence] :GATE:LOGic**

**Function** Sets or queries the gate signal logic of gate sampling.

**Syntax** :TRIGger[:SEQUence]:GATE:LOGic<wsp>POSI|NEGA|0|1  
:TRIGger[:SEQUence]:GATE:LOGic?  
POSI = Sampling is performed when the gate signal is at high level  
NEGA = Sampling is performed when the gate signal is at low level

**Response** 0 = POSI, 1 = NEGA

**Example** :TRIGGER:SEQUENCE:GATE:LOGIC POSI  
:TRIGGER:SEQUENCE:GATE:LOGIC? -> 0

**Description** • This is a sequential command.  
• This command can be used on the AQ6370C/AQ6370D/AQ6373B.

## 7.6 Instrument-Specific Commands

### :TRIGger [:SEQUence] :SLOPe

Function	Sets/queries the trigger edge.
Syntax	:TRIGger[:SEQUence]:SLOPe<wsp>RISE FALL 0 1 :TRIGger[:SEQUence]:SLOPe? RISE = RISE FALL = FALL Response 0 = RISE, 1 = FALL
Example	:TRIGER:SLOPE RISE :TRIGER:SLOPE? -> 0
Explanation	<ul style="list-style-type: none"><li>When this command is executed, the external trigger mode becomes enabled.</li><li>This is a sequential command.</li></ul>

### :TRIGger [:SEQUence] :STATE

Function	Sets/queries the external trigger mode.
Syntax	:TRIGger[:SEQUence]:STATE<wsp>OFF ON PHOLD 0 1 2 :TRIGger[:SEQUence]:STATE? OFF: External Trigger OFF ON: External trigger mode PHOLD: Peak hold mode GATE: Gate sampling Response 0 = OFF, 1 = ON, 2 = PHOLD, 3 = GATE
Example	:TRIGER:STATE ON :TRIGER:STATE? -> 1
Explanation	<ul style="list-style-type: none"><li>This is a sequential command.</li><li>Gate sampling can be used on the AQ6370C / AQ6370D / AQ6373B.</li></ul>

### :TRIGger [:SEQUence] :INPut

Function	Sets/queries the signal of the input trigger.
Syntax	:TRIGger[:SEQUence]:INPut<wsp>ETRigger STRigger SENable 0 1 2 :TRIGger[:SEQUence]:INPut? ETRigger 0: Sampling trigger STRigger 1: Sweep trigger SENable 2: Sample enable
Example	:TRIGER:INPUT STRIGGER :TRIGER:INPUT? -> 1
Explanation	This is a sequential command.

### :TRIGger [:SEQUence] :OUTPut

Function	Sets/queries the signal of the output trigger.
Syntax	:TRIGger[:SEQUence]:OUTPut<wsp>OFF SSTatus 0 1 :TRIGger[:SEQUence]:OUTPut? OFF: OFF SSTatus: Sweep status Response 0 = OFF, 1 = SSTatus
Example	:TRIGER:OUTPUT SSTATUS :TRIGER:OUTPUT? -> 1
Explanation	This is a sequential command.

### :TRIGger [:SEQUence] :PHOLd:HTIMe

Function	Sets/queries the hold time of peak hold mode.
Syntax	:TRIGger[:SEQUence]:PHOLd:HTIMe<wsp><NRf>[s] :TRIGger[:SEQUence]:PHOLd:HTIMe? <NRf> = Hold time [s]
Example	:TRIGER:PHOLD:HTIME 100MS :TRIGER:PHOLD:HTIME? -> +1.0000000E-1
Explanation	This is a sequential command.

## UNIT Sub System Command

### :UNIT:POWER:DIGIT

Function Sets/queries the number of decimal places displayed for the level value.

Syntax :UNIT:POWER:DIGIT<wp>1|2|3  
          :UNIT:POWER:DIGIT?  
          1, 2, 3 = Number of displayed digits

Example :UNIT:POWER:DIGIT 3  
          :UNIT:POWER:DIGIT? -> 3

Explanation This is a sequential command.

### :UNIT:X

Function Sets/queries the units for the X axis.

Syntax :UNIT:X<wp>WAVelocity|FREQuency|  
          WNUmber|0|1|2:UNIT:X?  
          Response  
          For AQ6370C, AQ6373 or AQ6373B  
          WAVelocity = Wavelength  
          FREQuency = Frequency  
          For AQ6375  
          WAVelocity = Wavelength  
          FREQuency = Frequency  
          WNUmber = Wavenumber  
          Response 0 = WAVelocity, 1 = FREQuency,  
                  2=WNUmber

Example :UNIT:X FREQUENCY  
          :UNIT:X? -> 1

Explanation This is a sequential command.

## 7.7 Output Format for Analysis Results

### Output of Analysis Results

The analysis results of analysis functions are collectively output using the CALCulate:DATA? command. If analysis has been not performed, a query error occurs.

### Output Data Format for Each Analysis Function

The output data format of each analysis function is as shown below.

For information on abbreviations such as <center wl>, see “List of Abbreviations of Data Output using the CALCulate:DATA? Command.”

#### THRESH , ENVELOPE, PK-RMS

<center wl>,<spec wd>,<mode num>

#### RMS

<center wl>,<spec wd>

#### NOTCH

<center wl>,<notch wd>

#### SMSR

- SMSR1, SMSR2

<peak wl>,<peak lvl>,<2nd peak wl>,<2nd peak lvl>,<delta wl>,<delta lvl>

- SMSR3, SMSR4

<peak wl>,<peak lvl>,<2nd peak wl(L)>,<2nd peak lvl(L)>,<delta wl(L)>,<delta lvl(L)>,<2nd peak wl(R)>,<2nd peak lvl(R)>,<delta wl(R)>,<delta lvl(R)>

#### POWER

<total pow>

#### DFB-LD

<spec wd>,<peak wl>,<peak lvl>,<mode ofst>,<smsr>

#### FP-LD

<spec wd>,<peak wl>,<peak lvl>,<center wl>,<total pow>,<mode num>

#### LED

<spec wd>,<peak wl>,<peak lvl>,<center wl>,<total pow>

#### PMD

<left mode peak>,<right mode peak>,<pmd>

#### WDM

- ABSOLUTE, CH RELATION = OFFSET

<ch num>,<center wl>,<peak lvl>,<offset wl>,<offset lvl>,<noise>,<snr>,...

- ABSOLUTE, CH RELATION = SPACING

<ch num>,<center wl>,<peak lvl>,<spacing>,<lvl diff>,<noise>,<snr>,...

- RELATIVE

<ch num>,<grid wl>,<center wl>,<rel wl>,<peak lvl>,<noise>,<snr>,...

- DRIFT (MEAS)

<ch num>,<grid wl>,<center wl>,<wl diff max>,<wl diff min>,<ref lvl>,<peak lvl>,<lvl diff max>,<lvl diff min>,...

- **DRIFT (GRID)**

<ch num>, <ref wl>, <center wl>, <wl diff max>, <wl diff min>, <ref lvl>, <peak lvl>, <lvl diff max>, <lvl diff min>, ...

### **EDFA-NF**

<ch num>, <center wl>, <input lvl>, <output lvl>, <ase lvl>, <resoln>, <gain>, <nf>, ...

### **FILTER-PK**

<peak wl>, <peak lvl>, <center wl>, <spec wd>, <l-xtalk>, <r-xtalk>, <ripple>

### **FILTER-BTM**

<btm wl>, <btm lvl>, <center wl>, <notch wd>, <l-xtalk>, <r-xtalk>

### **WDM FIL-PK**

<ch num>, <nominal wl>, <peak wl>, <peak lvl>, <xdb wd>, <center wl>, <xdb sb>, <xdb pb>, <ripple>, <l-xtalk>, <r-xtalk>, ...

\* Items with SW set to OFF are also output.

### **WDM FIL-BTM**

<ch num>, <nominal wl>, <btm wl>, <btm lvl>, <xdb ntwd>, <center wl>, <xdb sb>, <xdb eb>, <ripple>, <l-xtalk>, <r-xtalk>, ...

\* Items with SW set to OFF are also output.

### **COLOR**

<dominant wl>, <x col>, <y col>, <z col>

## 7.7 Output Format for Analysis Results

---

### List of Abbreviations of Data Output Using the CALCulate:DATA? Command

Abbreviation	Description	Format	Output Unit
<center wl>	Center wavelength	<NRF>	m / Hz
<spec wd>	Spectrum width	<NRF>	m / Hz
<mode num>	Mode number	<integer>	
<notch wd>	Notch width	<NRF>	m / Hz
<peak wl>	Peak wavelength	<NRF>	m / Hz
<peak lvl>	Peak level	<NRF>	dBm
<2nd peak wl>	2nd peak wavelength	<NRF>	m / Hz
<2nd peak lvl>	2nd peak level	<NRF>	dB
<delta wl>	Wavelength difference	<NRF>	m / Hz
<delta lvl>	Level difference	<NRF>	dB
<mode ofst>	Mode offset	<NRF>	m / Hz
<smsr>	SMSR value	<NRF>	dB
<smsr(L)>	SMSR value (shorter wavelength side)	<NRF>	dB
<smsr(R)>	SMSR value (longer wavelength side)	<NRF>	dB
<mode ofst(L)>	Mode offset (shorter wavelength side)	<NRF>	m/Hz
<mode ofst(R)>	Mode offset (longer wavelength side)	<NRF>	m/Hz
<2nd peak wl(L)>	Second peak wavelength (shorter wavelength side)	<NRF>	m/Hz
<2nd peak wl(R)>	Second peak wavelength (longer wavelength side)	<NRF>	m/Hz
<2nd peak lvl(L)>	Second peak level (shorter wavelength side)	<NRF>	dB
<2nd peak lvl(R)>	Second peak level (longer wavelength side)	<NRF>	dB
<delta wl(L)>	Wavelength difference (shorter wavelength side)	<NRF>	m/Hz
<delta wl(R)>	Wavelength difference (longer wavelength side)	<NRF>	m/Hz
<delta lvl(L)>	Level difference (shorter wavelength side)	<NRF>	dB
<delta lvl(R)>	Level difference (longer wavelength side)	<NRF>	dB
<power>	Power value	<NRF>	dB/W
<total pow>	Total power value	<NRF>	dB / W
<mode num>	Mode number	<integer>	
<left mode peak>	Mode peak frequency (left)	<NRF>	Hz
<right mode peak>	Mode peak frequency (right)	<NRF>	Hz
<pmd>	PMD value	<NRF>	ps
<ch num>	Channel number	<integer>	
<offset wl>	Offset wavelength	<NRF>	m / Hz
<offset lvl>	Offset level	<NRF>	dB
<noise>	Noise level	<NRF>	dBm / NBW
<snr>	SNR value	<NRF>	dB
<grid wl>	Grid wavelength	<NRF>	m / Hz
<rel wl>	Relative wavelength	<NRF>	m / Hz
<wl diff max>	Wavelength difference (max.)	<NRF>	m / Hz
<wl diff min>	Wavelength difference (min.)	<NRF>	m / Hz
<ref lvl>	Relative level	<NRF>	dB
<lvl diff max>	Level difference (max.)	<NRF>	dB
<lvl diff min>	Level difference (min.)	<NRF>	dB
<input lvl>	Input level	<NRF>	dBm
<output lvl>	Output level	<NRF>	dBm
<ase lvl>	ASE level	<NRF>	dBm / RES
<resoln>	Measurement resolution	<NRF>	m
<gain>	Gain	<NRF>	dB
<nf>	NF value	<NRF>	dB
<l-xtalk>	Crosstalk value (left)	<NRF>	dB
<r-xtalk>	Crosstalk value (right)	<NRF>	dB
<ripple>	Ripple width	<NRF>	m / Hz

## 7.7 Output Format for Analysis Results

Abbreviation	Description	Format	Output Unit
<nominal wl>	Reference wavelength	<NRF>	m / Hz
<xdb wd>	Xdb width	<NRF>	m / Hz
<xdb sb>	XdB stop-band	<NRF>	m / Hz
<xdb pb>	XdB passband	<NRF>	m / Hz
<xdb eb>	XdB elimination band	<NRF>	m / Hz
<dominant wl>	Dominant wavelength	<NRF>	m / Hz
<x col>	Chromaticity coordinates (x)	<NRF>	
<y col>	Chromaticity coordinates (y)	<NRF>	
<z col>	Chromaticity coordinates (z)	<NRF>	

## 8.1 Editing a Program

To use the program functions, a program must be pre-registered in the instrument.

### Procedure

**1.** Press **PROGRAM**.


The program menu is displayed.

**2.** Press the **PROGRAM EDIT** soft key. The program registration screen appears.

**Note**


- Thirty-two program names are displayed on a single screen.
  - The US column includes an asterisk (\*) if a program has already been registered in the corresponding program number.
  - The EXECUTE NO. column shows the registered program numbers for programs that have been registered to the <EXECUTE 1> to <EXECUTE 21> keys.
- See section 8.2, "Executing Programs" for information on registering programs to the EXECUTE1–EXECUTE21 soft keys.

**3.** Select a registration number using the **rotary knob** or the **arrow keys**.

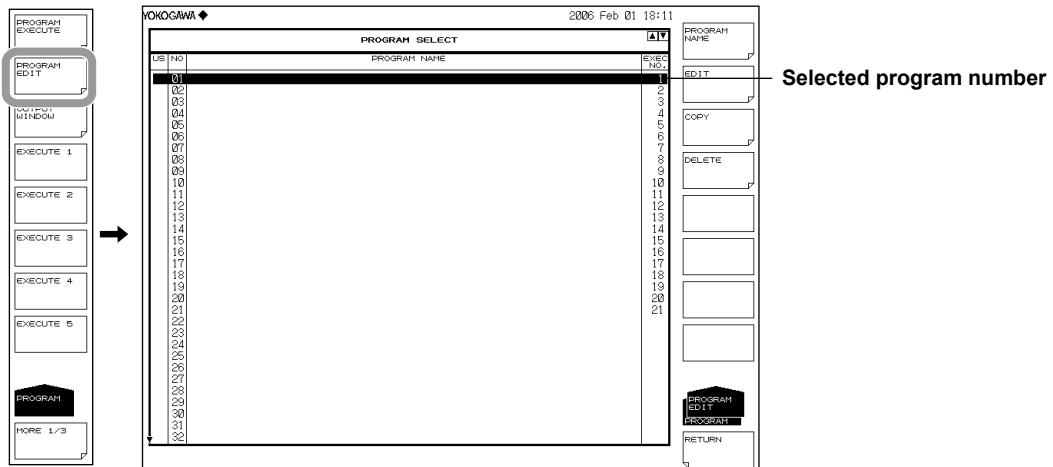

## Entering a Program Name

4. Press the **PROGRAM NAME** soft key.
- The program name input screen appears.
5. Enter a program name using the **rotary knob** and soft keys.
6. After entering a name, press the **DONE** soft key. The program name is finalized, the instrument returns to the program registration screen. The entered program name is displayed in the program registration screen.

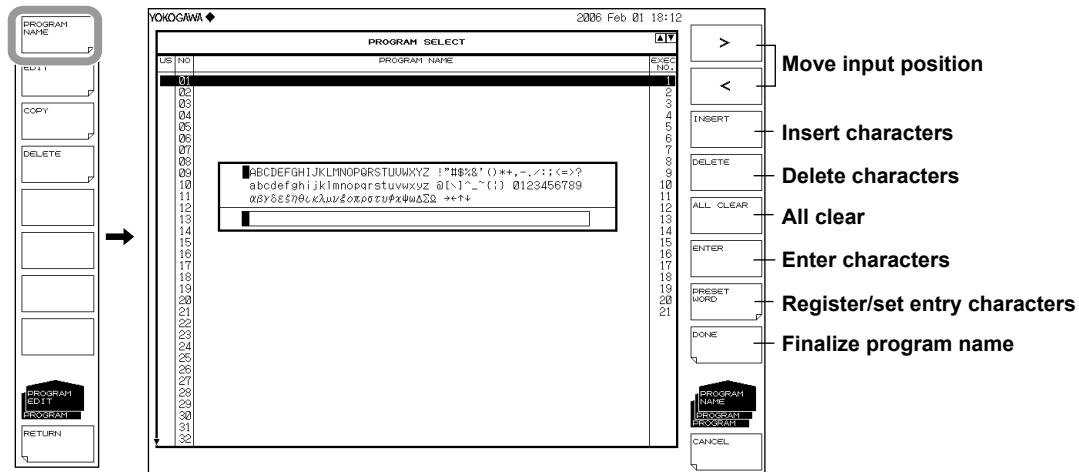

### Note

To register and reuse an entered string, or to use a previously entered string, press the PRESET WORD soft key.

#### Registering Strings

After a string has been entered in the program name entry screen, press the PRESET WORD soft key.

Select a registration number and press the SAVE soft key. The entered string is registered in the program name input screen.


#### Using Registered Strings

Press the PRESET WORD soft key.

Select the number of the string you wish to use and press the RECALL soft key. The selected string is entered as a program name.

## Editing a Program

7. Select a program to edit in the program registration screen and press the **EDIT** soft key. The program edit screen appears.

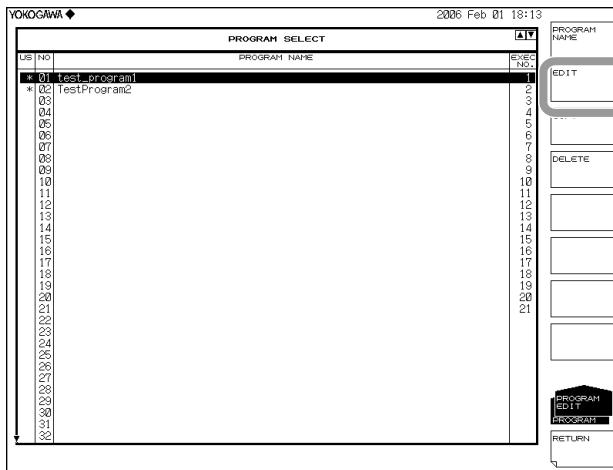

8. Select a line to edit using the **rotary knob** or the **arrow keys**. When a line of a specified command parameter is selected, the **PARAMETER EDIT** soft key is enabled.
9. Edit the program using the soft keys. For the settings associated with each soft key, see pages 8-6 and 8-7.
10. When finished editing the program, press the **RETURN** soft key.


**Line number**

- Function command
- Edit parameters
- Enter the input values
- Special commands
- Copy/delete line
- List print  
(On the AQ6370C, AQ6373 or AQ6375)

## 8.1 Editing a Program

### Copying/Merging (Combining) Programs

11. Select the program to copy in the program registration screen in step 2.
12. Press the **COPY** soft key.

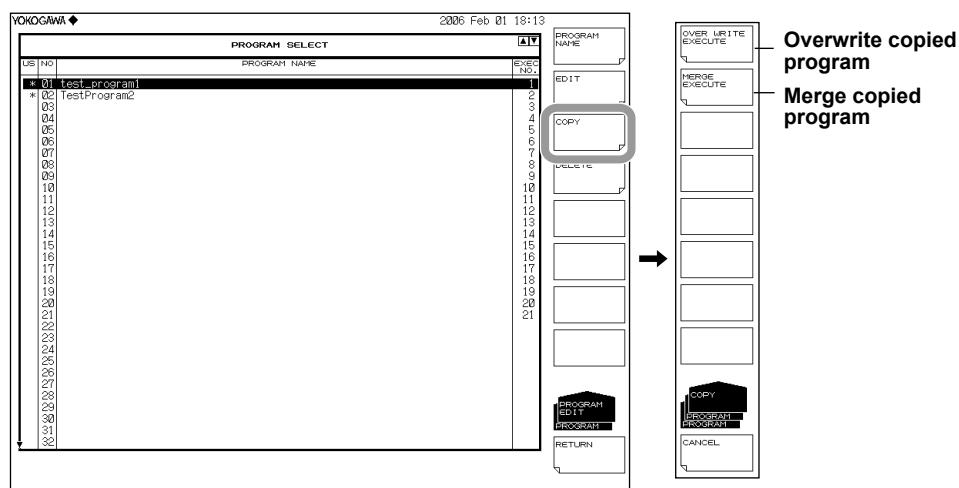

#### Overwriting a Copied Program


13. Select a copy destination program and press the **OVER WRITE EXECUTE** soft key. The copied program overwrites the selected destination program.

#### Merging a Copied Program

14. After performing step 12, select a copy destination program and press the **MERGE EXECUTE** soft key. The contents of the copied program are pasted onto the end of the copy destination program (making one large program).

### Deleting a Program

15. Select the program to delete in the program registration screen in step 2.
16. Press the **DELETE** soft key. A confirmation message is displayed.

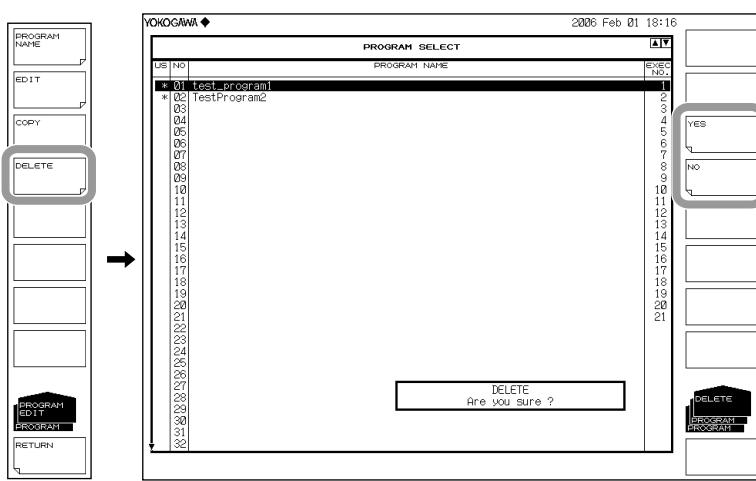

17. Press the **YES** or **NO** soft key to delete the program or cancel.

## Program Editing Operations

The following describes the operation of the various soft keys when editing programs. Each description assumes that the program editing screen is open (by pressing **PROGRAM**, followed by the **PROGRAM EDIT > EDIT** soft keys).

### Selecting Commands

The following two types of commands are available.

#### Function Commands

These commands execute the same function as a function switch (including the contents of a soft key).


(Commands corresponding to the soft keys such as SINGLE and SPAN)

#### Special Commands


These commands include jump commands, program control commands for conditional decision, etc., control commands to an external device, and data output commands.

- To select function commands or special commands, press the **COMMAND SELECT** or **SPECIAL COMMAND** soft keys, respectively. The function command or special command selection screen is displayed.

#### Function commands

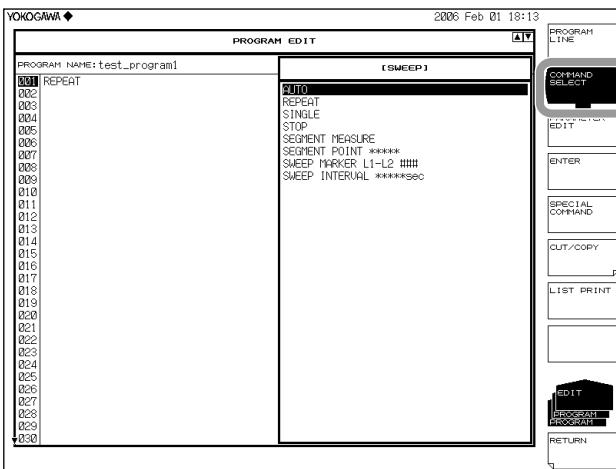

#### Special commands

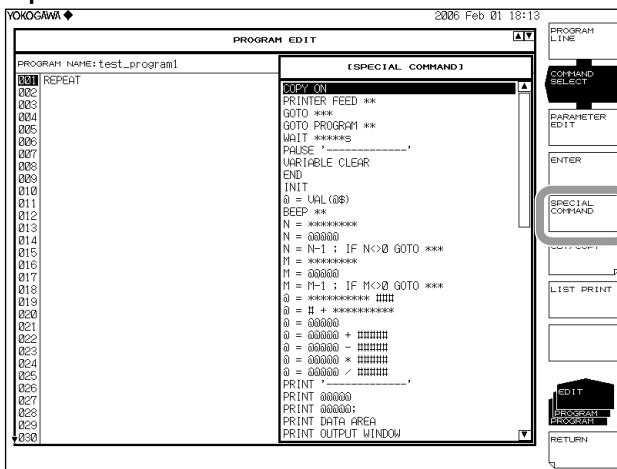

- Select a command using the **rotary knob** or the **arrow keys**, and press the **ENTER** soft key. The selected command is entered. When entering commands that require parameter settings, the parameter setting screen is displayed.
- Enter the parameter and press the **ENTER** soft key. The parameter is set.

#### Note


- The \*\*\*\* portion of commands are numbers, the ### portion is the selected parameter, and ----- is text input.
- Function commands can also be set using the mouse. Right-click the mouse to display a shortcut list of panel keys. Left-clicking enters the function command corresponding to the selected panel key.

## 8.1 Editing a Program

### Editing Parameters

Modifying Parameters of an Entered Command

1. Select the line of the command whose parameter you wish to modify using the **rotary knob** or the **arrow keys**. The **PARAMETER EDIT** soft key becomes enabled.
2. Press the **PARAMETER EDIT** soft key. The parameter setting screen is displayed.

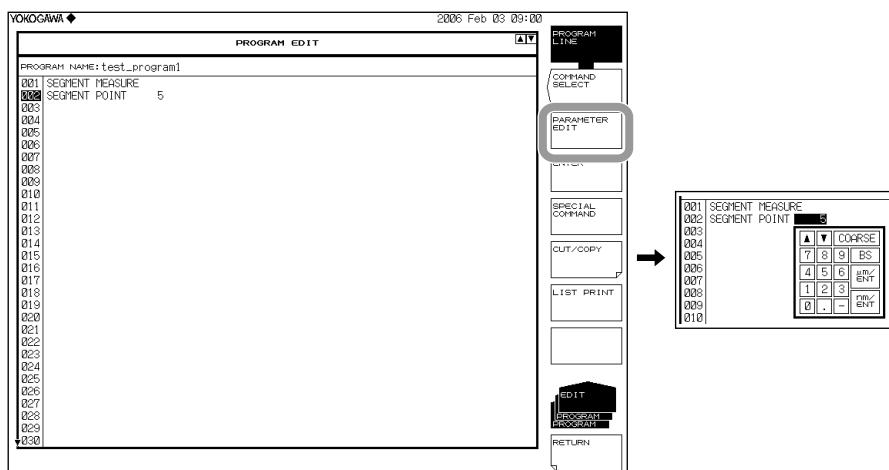

3. Enter the parameter and press the **ENTER** soft key. The parameter is set.


### Note

The parameter setting screen displayed differs depending on the type of parameter.

### Inserting, Copying, or Deleting a Line

You can copy or delete the contents of a line.

1. Press the **CUT/COPY** soft key. The CUT/COPY screen is displayed.

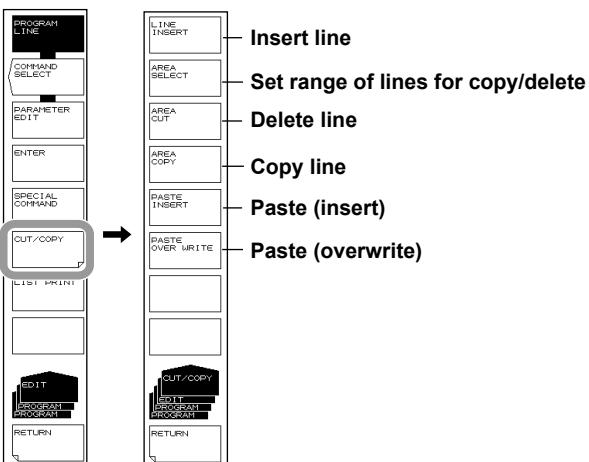

### Inserting a Line

2. Select a line number on which to insert a line using the **rotary knob** or the **arrow keys**.
3. Press the **LINE INSERT** soft key. One line is inserted above the selected line number.

### Note

If commands have been entered in all 200 lines, a new line cannot be inserted.

**Deleting a Line**


- 2.** To delete one line, select the line to delete using the **rotary knob**.  
To delete multiple lines, select the first or last line to delete and press the **AREA SELECT** soft key.  
Select the range of lines to delete using the **rotary knob** or the **arrow keys**.
- 3.** Press the **AREA CUT** soft key. The specified range of lines is deleted.  
To restore the deleted line, press **UNDO/LOCAL**.

**Copying a Line**

- 2.** To copy one line, select the line to copy using the **rotary knob** or the **arrow keys**.  
To copy multiple lines, select the first or last line to copy and press the **AREA SELECT** soft key.  
Select the range of lines to copy using the **rotary knob** or the **arrow keys**.
- 3.** Press the **AREA COPY** soft key. The specified range of lines is copied.
- 4.** Select a copy destination line using the **rotary knob** or the **arrow keys**.
- 5.** To insert the copied lines, press the **PASTE INSERT** soft key.  
To overwrite with the copied lines, press the **PASTE OVER WRITE** soft key.  
The copied lines are pasted, starting from the line selected as the copy destination. To restore the pasted contents, press **UNDO/LOCAL**.

**Printing Out a Program List (On the AQ6370C, AQ6373 or AQ6375)**

- 1.** Press the **LIST PRINT** soft key. The program list is printed by the built-in printer.

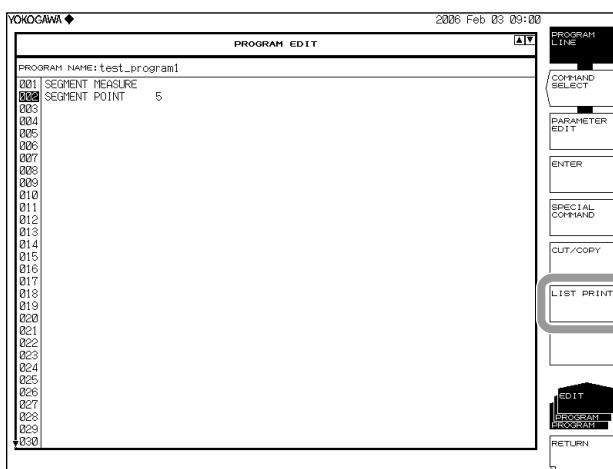**Note**

The LIST PRINT soft key is disabled if the built-in printer is not installed.

### Explanation

#### Programs

Up to 64 programs can be registered.

A program key can be assigned to each program allowing you to execute the program simply by pressing its soft key.

#### Commands

There are two types of executable commands.

##### Function Commands

(Commands corresponding to the soft keys such as SINGLE and SPAN)

##### Special Commands

These commands include jump commands, program control commands for conditional decision, etc., control commands to an external device, and data output commands.

For detailed information on commands, see section 8.3, "Program Function Commands."

#### Merging a Program

You can combine two different programs into one program.

The copied program is pasted onto the end of another specified program.

## 8.2 Executing a Program

There are two methods for executing a program: specifying then executing the program, and assigning the program to a soft key and executing it directly with that key.


### Procedure

#### Specifying and Executing a Program

1. Press **PROGRAM**.

The program menu is displayed.

2. Press the **PROGRAM EXECUTE** soft key. The program selection screen appears.

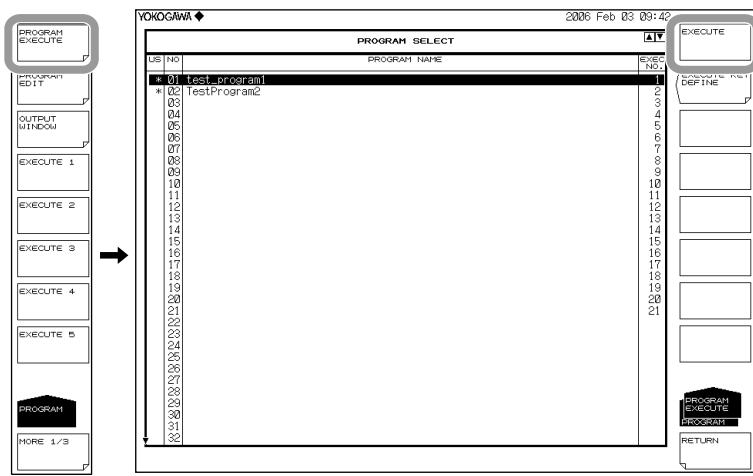

3. Select a program to execute using the **rotary knob** or the **arrow keys**.
4. Press the **EXECUTE** soft key. The program executes.

#### Note

To stop the program during execution, press the **PROGRAM EXIT** soft key.


## 8.2 Executing a Program

### Assigning a Program to a Soft Key and Executing Assigning to a Soft Key

**1. Press PROGRAM.**

The program menu is displayed.

**2. Press the PROGRAM EXECUTE soft key. The program selection screen appears.**

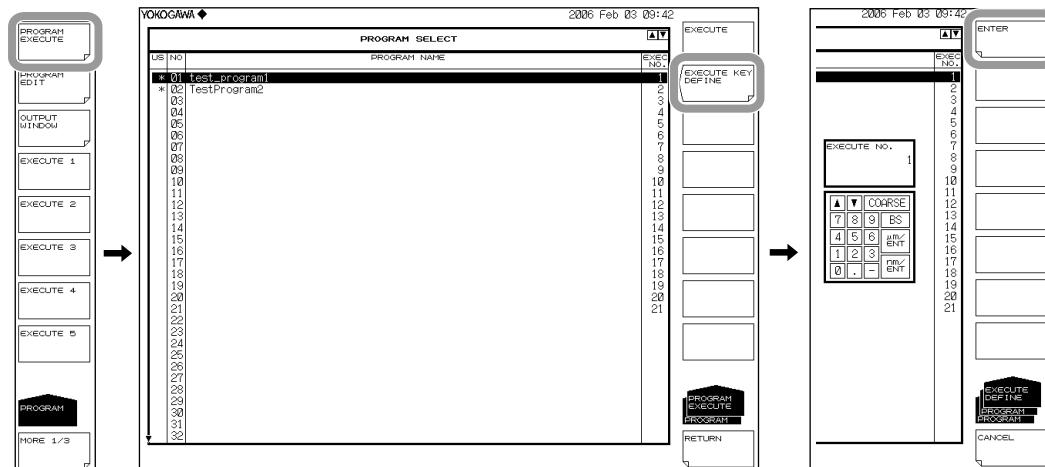

- 3. Select a program to assign using the rotary knob or the arrow keys.**
- 4. Press the EXECUTE KEY DEFINE soft key. A screen for assigning soft keys is displayed.**
- 5. Enter a soft key number between 1 and 21 and press the ENTER soft key. If a program is already assigned to that number, the existing program is overwritten.**


**Note**

A single program cannot be assigned to multiple soft keys.

### Executing the Program

**1. Press PROGRAM.**

The program menu is displayed.

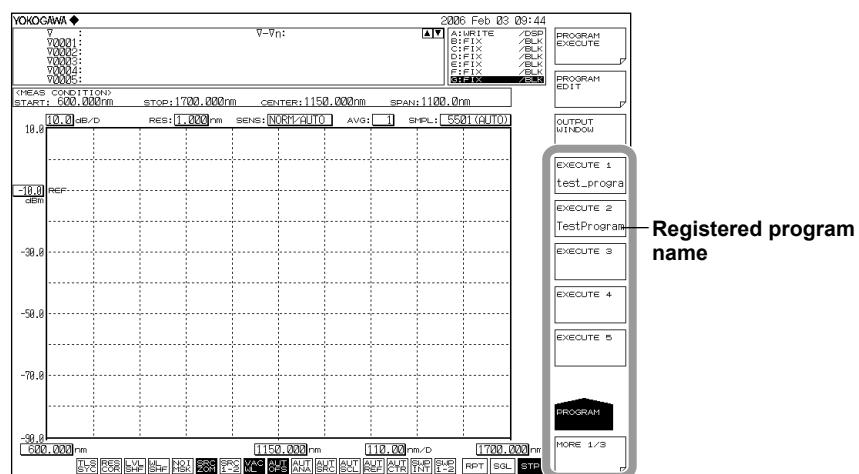


- 2. Press a soft key from EXECUTE 1 to EXECUTE 21. The program assigned to the soft key executes.**

## Displaying the OUTPUT WINDOW

### 1. Press PROGRAM.

The program menu is displayed.

### 2. Press the OUTPUT WINDOW soft key. The OUTPUT WINDOW is displayed.

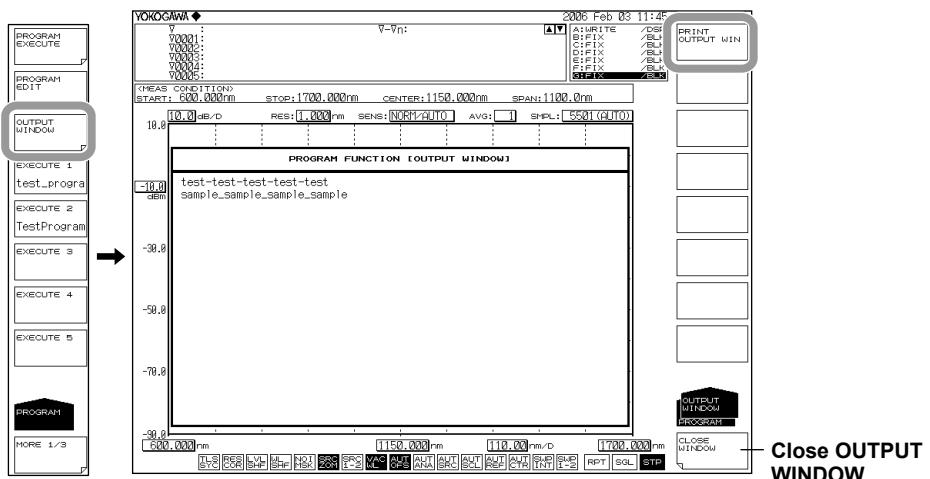

### Note

If there is no data to display in the OUTPUT WINDOW, the OUTPUT WINDOW soft key is disabled. Data and characters output by the DATA OUTPUT command are displayed.

3. To output the contents of the OUTPUT WINDOW to the built-in printer, press the **PRINT OUTPUT WIN** soft key (On the AQ6370C, AQ6373 or AQ6375).
4. To close the OUTPUT WINDOW, press the **CLOSE WINDOW** soft key.

### Note

- The contents of the OUTPUT WINDOW are held until execution of the OUTPUT WINDOW CLEAR special command.
- The contents of the OUTPUT WINDOW can be stored in a file. See the main unit user's manual (IM AQ6370C-01EN(AQ6370C), IM AQ6373-01EN(AQ6373), IM AQ6373B-01EN(AQ6373B) or IM AQ6375-01EN(AQ6375)) for details.
- If the contents of the OUTPUT WINDOW exceeds 200 lines, data will be erased beginning from the first line, in turn.
- Turning off the power switch on the instrument erases data in the OUTPUT WINDOW.

### Explanation

#### Using Special Commands

During program execution, you can perform unique operations with commands.

##### When Executing a Program Including “PAUSE ‘-----’”

The program pauses.

The message included in the “PAU2SE ‘-----’” line is displayed, and the program pauses. To resume execution of the program, press the CONTINUE soft key.

If a program is executed via remote control, the “PAUSE ‘-----’” command is ignored.

##### When Executing a Program Including the “DATA INPUT -----’;@’ Command

After the program executes, a data entry window is displayed.

In this case, one of two types of windows will appear depending on the @ variable.

String variables: Enter a file name using the same procedure as that of label input and press the DONE soft key.

Numerical variables: A data entry window is displayed. Enter an arbitrary number using the rotary knob, arrow keys, or ten key. If a program is executed via remote control, the “DATA INPUT -----’;@’ command is ignored.

##### Outputting Data Using “DATA OUTPUT @@@@”

When executing a program, the OUTPUT WINDOW for displaying output data is displayed.

The contents of the variables specified by “@@@@” appear in the OUTPUT WINDOW. Up to 200 lines can be displayed in the OUTPUT WINDOW. Only 20 lines can be displayed at once. To display lines other than the first 20, use the rotary knob or arrow keys to scroll.

The OUTPUT WINDOW can be displayed during execution of a program. To do so, use the “OUTPUT WINDOW ###” special command. Note that the OUTPUT WINDOW disappears if the program ends.

## Error Encountered upon Execution of a Program

If an error occurs during the running of a program, an error number indicating the details of the error is displayed in a window, and execution of the program is stopped.

### Classification of Error Numbers

- 300–307 Errors caused by attempting a setting in manual operation which is disabled
- 320–326 Special command-related errors
- 340–347 Input/output-related errors
- 360–369 External memory-related errors
- 380, 381 Other errors

The above numbers can be read out using the SYSTem:ERRor[:NEXT]? command (see section 7.6, “Instrument-Specific Commands”).

No.	Message	Cause	Instrument models on which the command is valid
300	Parameter out of range	A variable value is out of range or is not defined for a command that sets a parameter using variables.	
302	Scale unit mismatch	There is a difference between the Y-axis scale of the active trace and the unit of a parameter in the “LINE MKR 3 or 4” command.	
303	No data in active trace	Setting of the moving marker, a peak (or bottom) search, or activation of the analysis function was made with no data in the active trace.	
304	Marker value out of range	Specified wavelength was out of the sweep range in the moving marker or line wavelength marker setting command.	
305	No data in traces A or B	No waveform data in traces A or B when executing the “EDFA NF” command	
306	Invalid data	Trace had no data when attempting to save it to memory or to write it to FD/INT.	
307	Unsuitable Write item	All data items were OFF at execution of “WRITE DATA”.	
320	Undefined variable	A command containing an undefined variable was executed.	
321	Variable unit mismatch	The unit of each variable does not agree within a command containing two or more variables.	
322	Overflow	An overflow occurred in an arithmetic operation.	
323	Undefined marker variable	A command containing a marker-value variable was executed when no marker had been displayed.	
324	Invalid marker variable	A command containing the corresponding variable was executed at a time other than immediately after execution of a spectrum width search, peak search, etc.	
325	Undefined line number	GOTO command's jumping destination is a number other than 1 to 200.	
326	F1 greater than F2	F1>F2 when the “IF F1 @@@@ F2” command was executed.	
340	Printer paper empty	No printer paper.	AQ6370C/ AQ6373/AQ6375
341	Printer head up	No print is made because the printer's head-up lever is raised.	AQ6370C/ AQ6373/AQ6375
345	Option does not respond	No response from an external device.	
346	Option is not connected	No external device is connected.	
347	GP-IB2 not system controller	System controller connected to the GP-IB2 port has been set to an external computer.	AQ6370C/ AQ6373/AQ6375
360	Disk full	No file can be created due to insufficient free space in the external memory.	

## 8.2 Executing a Program

No.	Message	Cause	Instrument models on which the command is valid
361	Disk not inserted	No external memory is connected.	
362	Disk is write protected	The external memory is write protected.	
363	Disk not initialized	External memory is not initialized. Or, it has been formatted in a format not supported by this instrument.	
364	Directory full	Directory is full, therefore no file can be created.	
365	File not found	The specified file cannot be read because it has not been found. Or, the file does not exist on the disk.	
366	File is write protected	The file is specified to be read only, so that it cannot be rewritten or deleted.	
367	No data	No data to store.	
368	File is not a trace file	A file cannot be read because it is not a trace file.	
369	Illegal file name	A file cannot be saved due to an incorrect file name.	
371	Directory already exist	Unable to make the directory because a directory with the same name already exists.	
380	Undefined program	An attempt was made to run a program that is not defined.	
381	Syntax error	Command incorrect. (a program has been rewritten for some reason)	
382	Program nesting over	Nesting is not possible because the program nesting is already too deep.	
383	Program reentrant error	The destination of the GOTO command is set to its own program number. This will create an infinite loop.	

## 8.3 Program Function Commands

There are two types of commands used in a program: function commands which are input using a panel switch, and other special commands.

### Variables

Variables that can be used in a program are shown in the table below.

Type	Variable Name	Description
Generalized variables	E, G-K, O-R, T, U, V, X, Y, Z <sup>1</sup> A\$, B\$, C\$, D\$	Contains a generalized numeric variable.
GP-IB variables	S A\$, B\$, C\$, D\$	Contains a generalized string variable. Performs serial polling and stores received status bytes. This variable is also used as a generalized numeric variable.
	FILE\$ TIME\$	Contains data received via the GP-IB2 port. This variable is also used as a generalized string variable (on the AQ6370C, AQ6373 or AQ6375). Date & time/file name variables Contains the name of the last file accessed. Contains the date and time. (Ex. 2005 Sep 08 20:45:37)
Marker variables	WM W1 W2 W2-W1 W(CH) LM L1 L2 L2-L1 L(CH)	Contains the wavelength value of the moving marker. Contains the wavelength value of fixed marker 1. Contains the wavelength value of fixed marker 2. Contains the wavelength difference between fixed markers 1 and 2. Contains the level values of fixed markers (CH: 1 to 1024). Contains the level value of the moving marker. Contains the level value of fixed marker 1. Contains the level value of fixed marker 2. Contains the level difference between fixed markers 1 and 2. Contains the level values of fixed markers (CH: 1 to 1024).
Analysis variables On the AQ6370C / AQ6370D or AQ6373B valid variables	SPWD PKWL MEANWL PKLVL MODN SMSR SMSR2 WDMCHN WDMWL(CH) WDMlvl(CH) WDMsnr(CH) MKPWR PMD	Contains spectrum width applied in making a spectrum width search. Contains a peak (or bottom) wavelength value applied in making a peak (or bottom) search or spectrum width search. Contains center wavelength applied in making spectrum width search. Contains a peak (or bottom) level value applied in making a peak (or bottom) search or spectrum width search. Contains the number of modes applied in making a spectrum width search. Contains the side mode suppression ratio (level difference) applied in making SMSR measurements. Contains the longer wavelength side's value of the side mode suppression ratio (level difference) when an SMSR3 or SMSR4 measurement is executed (on the AQ6370C or AQ6370D). Contains the number of channels detected in performing WDM analysis. Contains the center wavelength of channel CH used in performing WDM analysis. Contains the level of channel CH used in performing WDM analysis. Contains SNR of channel CH used in performing WDM analysis. Contains power obtained in making between line-markers power measurements. Contains the PMD value obtained in PMD analysis.

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### 8.3 Program Function Commands

---

Type	Variable Name	Description
Analysis variables		
On the AQ6373/AQ6373B, invalid variables		
	NFCHN	Contains the number of channels detected in performing EDFA-NF analysis.
	NFWL(CH)	Contains the center wavelength of channel CH used in performing EDFA-NF analysis.
	NFLVLI(CH)	Contains the input signal level of channel CH used in performing EDFA-NF analysis.
	NFLVLO(CH)	Contains the output signal level of channel CH used in performing EDFA-NF analysis.
	NFASELV(CH)	Contains the ASE level of channel CH used in performing EDFA-NF analysis.
	NFGAIN(CH)	Contains the gain of channel CH used in performing EDFA-NF analysis.
	NFNF(CH)	Contains NF of channel CH used in performing EDFA-NF analysis.
Only the AQ6373/AQ6373B, valid variables		
	DOMWL	Dominant wavelength value is entered when measuring the dominant wavelength.
	XCOL	The chromaticity coordinate value X is entered when performing COLOR analysis.
	YCOL	The chromaticity coordinate value Y is entered when performing COLOR analysis.
	ZCOL	The chromaticity coordinate value Z is entered when performing COLOR analysis.
Program control variables	M	Contains loop counter data.
	N	Contains loop counter data.
	F1	Contains a conditional judgment variable.
	F2	Contains a conditional judgment variable.
	CH	Contains an element number variable used in accessing an array variable (1–1024).
Temprate variables	GONO	Contains GONO judgment results

### Principles of Variable-based Arithmetic Operations

For assignment of units after arithmetic operations when a variable with a unit is used in the operation, see below.

Expression	Results
(With a unit) × (Without unit)	With a unit
(With a unit)/(Without unit)	With a unit
(Without unit) + (Without unit)	Without unit
(Without unit) – (Without unit)	Without unit
(Without unit) × (Without unit)	Without unit
(Without unit) / (Without unit)	Without unit
(nm) + (nm)	(nm)
(nm) – (nm)	(nm)
(nm) / (nm)	Without unit
(dB) + (dB)	(dB)
(dB) – (dB)	(dB)
(dB) + (dB)	(dBm)
(dBm) – (dB)	(dBm)
(dBm) – (dBm)	(dB)
(#W) + (#W)	(#W)
(#W) – (#W)	(#W)
(#W) / (#W)	Without unit

#### Note

- For the units of dBm/nm, W/nm, dB/km, and %, dBm, W, dB, and without unit apply respectively in terms of variables.
- Arithmetic operations are made as noted above according to the unit of a variable, and the unit is appended to the result obtained after operation.
- If an arithmetic operation is made in any combination other than the above (addition, subtraction, multiplication, or division of variables with different units), the result of the operation has no units.
- The units of #W are treated as follows:

1 mW=1  
1 mW=0.001  
1 nW=0.000001  
1 pW=0.00000001

### Specifications of “@=VAL(@\$)” Command

A character string other than the numerics located before a value (starting with a sign or number) in @\$ character string will be ignored, and are converted as follows.

- “ , ”
- Numbers up to the next string or delimiter

If no numeric exists in @\$ character string, “0” is substituted for variable @.

## 8.3 Program Function Commands

---

### List of Function Commands

A description is given of the program commands of each function command. The optical spectrum analyzers on which the program command is valid is indicated along with the parameter range and variables supported. For the AQ6370C, AQ6373, AQ6373B, and AQ6375, if commands are valid for only some of the instruments, the models are so indicated. Models are not noted for commands that are valid for all instruments.

#### **SWEEP**

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
AUTO	Auto sweep	
REPEAT	Repeat sweep	
SINGLE	Single sweep	
STOP	Sweep stop	
SEGMENT MEASURE	Makes measurements only by a specified number of points starting at the position of the wavelength being stopped.	
SEGMENT POINT *****	Specifies the number of points to be measured with the SEGMENT MEASURE key	1-50001 (1 step)
SWEEP MKR L1-L2 ###	Selects ON/OFF of sweep function between markers	###: ON or OFF
SWEEP INTVL *****sec	Sets the interval time for repeat sweep	MINIMUM, 1 to 99999sec (1 step) (MINIMUM when set to 0.)

#### **Note**

---

Program commands not having a model listed in the chart are valid on all models (AQ6370C, AQ6373, AQ6373B, and AQ6375).

---

**CENTER**

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
CENTER WL ****.***nm	Sets measurement center wavelength.	AQ6370C/AQ6370D 600.000 to 1700.000nm (0.001 step) AQ6373/AQ6373B 350.000 to 1200.000nm (0.001 step) AQ6375 1200.000 to 2400.000nm (0.001 step)
CENTER WL @@@@	Sets the value of variable @@@@ to measurement center wavelength	@@@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), PKWL, MEANWL, WDMWL(CH), NFWL(CH)
		On the AQ6370C or AQ6370D WAM1, WAM2, WAM3, WAM4 valid variables
CENTER FREQ ***.*** THz	Sets measurement center frequency.	AQ6370C/AQ6370D 176.5000 to 500.0000THz (0.0001 step) AQ6373/AQ6373B 250.0000 to 856.5000THz (0.0001 step) AQ6375 125.0000 to 250.0000THz (0.0001 step)
CENTER FREQ @@@@	Sets the value of variable @@@@ to measurement center frequency	@@@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2,WAM1, WAM2, WAM3, WAM4, W(CH), PKWL, MEANWL, WDMWL(CH), NFWL(CH)
CENTER WNUM ****.***cm <sup>-1</sup>	Sets measurement center wavenumber.	AQ6375 4167.000 to 8333.000cm <sup>-1</sup> (0.001 step)
CENTER WNUM @@@@	Sets the value of variable @@@@ to measurement center wavenumber	@@@@@: G, H, I, J, K, P, Q, R, S, X, Y, Z, WM, W1, W2,W(CH), PKWL, MEANWL
START WL ***.*** nm	Sets measurement-starting wavelength.	AQ6370C/AQ6370D 50.000 to 1700.000 nm (0.001 step) AQ6373/AQ6373B 1.000 to 1200.000 nm (0.001 step) AQ6375 600.000 to 2400.000 nm (0.001 step)
START FREQ ***.*** THz	Sets measurement-starting frequency.	AQ6370C/AQ6370D 11.5000 to 500.0000 THz (0.0001 step) AQ6373/AQ6373B 10.0000 to 856.5000 THz (0.0001 step) AQ6375 60.0000 to 250.0000 THz (0.0001 step)
START WNUM ****.***cm <sup>-1</sup>	Sets measurement-starting wavenumber.	AQ6375 2067.000 to 8333.000cm <sup>-1</sup> (0.001 step)

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
STOP WL ****.*nm	Sets measurement-ending wavelength.	AQ6370C/AQ6370D 600.000 to 2250.000 nm (0.001 step) AQ6373/AQ6373B 350.000 to 1625.000 nm (0.001 step) AQ6375 1200.000 to 3000.000 nm (0.001 step)
STOP FREQ ***.*THz	Sets measurement-ending frequency.	AQ6370C/AQ6370D 176.5000 to 6650.0000 THz (0.0001 step) AQ6373/AQ6373B 250.0000 to 999.9000 THz (0.0001 step) AQ6375 125.0000 to 315.0000 THz (0.0001 step)
STOP WNUM ****.*cm <sup>-1</sup>	Sets measurement-ending wavenumber.	AQ6375 4167.000 to 10433.000cm <sup>-1</sup> (0.001 step)
PEAK->CENTER	Sets the center frequency of the waveform on the active trace	
MEAN WL->CENTER	Performs a spectrum width search on the active trace, and sets the results of center wavelength to the measurement center wavelength.	
AUTO CENTER ###	Executes every time a sweep finishes. <PEAK →CENTER> Function ON>Selects OFF	###: ON or OFF
VIEW SCALE->MEAS SCALE	Sets the current display conditions to measuring conditions.	

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### SPAN

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
SPAN WL ****.*nm	Sets the measuring span.	AQ6370C/AQ6370D 0.0 to 1100.0 nm (0.1 step) AQ6373/AQ6373B 0, 0.5 to 850.0 nm (0.1 step) AQ6375 0, 0.5 to 1200.0 nm (0.1 step)
SPAN WL @@@@ @@@@ Sets the value of variable @@@@ to the measuring spa		@@@@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, W2-W1, SPWD, WAM2-WAM1, WAM4-WAM3
SPAN FREQ ***.*THz	Sets the measuring span.	AQ6370C/AQ6370D 0, 0.01 to 330.00 THz (0.01 step) AQ6373/AQ6373B 0, 0.05 to 610.00 THz (0.01 step) AQ6375 0.01 to 130.00 THz (0.01 step)
SPAN FREQ @@@@ @@@@ Sets the value of variable @@@@ to the measuring span		@@@@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, W2-W1, SPWD, WAM2-WAM1, WAM4-WAM3

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
SPAN WNUM ****.***cm <sup>-1</sup>	Sets the measuring span.	AQ6375 0.5 to 4200.0 cm <sup>-1</sup> (0.1 step)
SPAN WNUM @@@@ @@@@ to the measuring span	Sets the value of variable @@@@ to the measuring span	@@@@@: G, H, I, J, K, P, Q, R, S, X, Y, Z, W2-W1, SPWD
START WL ****.***nm	Sets measurement-starting wavelength.	AQ6370C/AQ6370D 50.000 to 1700.000 nm (0.001 step)
START FREQ ***.**** THz	Sets measurement-starting frequency.	AQ6373/AQ6373B 1.000 to 1200.000 nm (0.001 step)
START WNUM ****.***cm <sup>-1</sup>	Sets measurement-starting wavenumber.	AQ6375 600.000 to 2400.000 nm (0.001 step)
STOP WL ****.***nm	Sets measurement-ending wavelength.	AQ6370C/AQ6370D 600.000 to 2250.000 nm (0.001 step)
STOP FREQ ***.**** THz	Sets measurement-ending frequency.	AQ6373/AQ6373B 350.000 to 1625.000 nm (0.001 step)
STOP WNUM ****.***cm <sup>-1</sup>	Sets measurement-ending wavenumber.	AQ6375 1200.000 to 3000.000 nm (0.001 step)
Δλ->SPAN	Performs a spectrum width search on the active trace, and sets the results to the measuring span.	AQ6375
0nm SWEEP TIME ** sec	Sets sweep time used when a sweep is made in a 0 nm measuring span.	0(MINIMUM), 1 to 50 (1step)
VIEW SCALE->	Sets the current display conditions	
MEAS SCALE	to measuring conditions.	

## 8.3 Program Function Commands

---

### LEVEL

The following command is not available on the AQ6375 if the horizontal axis is set to Wavenumber mode.

LEVEL UNIT #####      #####: dBm, dBm/nm

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
REFERENCE LEVEL ***.*dBm	Sets the reference level value used for LOG scaling.	-90.0 to 30.0dBm (0.1 step)
REFERENCE LEVEL ***.*##	Sets the reference level value used for LIN scaling	1.00pW to 1000mW (1.00 to 9.99 [pW, nW, μW, mW] :0.01 step 10.0 to 99.9(100)[pW, nW, μW, (mW)] :0.1 step 100 to 999 [pW, nW, μW, mW] : 1 step ## is , pW, nW, μW, mW (select one of the above)
REFERENCE LEVEL @@@@ @@@@ @@@@ @@@@ @@@@	Sets the value of variable @@@@ @@@@ @@@@ @@@@ @@@@ to the reference level value	AQ6370C/AQ6370D @@@@ @@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, LM, L1, L2, L(CH), PKLVL, WDMLVL(CH), FLVI(CH), NFLVO(CH), NFASELV(CH), MKPWR, LAM1, LAM2, LAM3, LAM4
LEVEL SCALE **.*dB/D	Sets a level scale value.	0 (LINEAR), 0.1 to 10.0dB/DIV (0.1 step)
LEVEL SCALE @@@@ @@@@ @@@@ @@@@ @@@@	Sets the value of variable @@@@ @@@@ @@@@ @@@@ @@@@ to the level scale	@@@@ @@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, L2-L1, SMSR, SMSR2, WDMSNR(CH), NFN(F(CH), LAM2-LAM1, LAM4-LAM3
BASE LEVEL ****	Lower value for linear scale setting. Use units set under REF LEVEL. If exceeds 90% of upper units of scale, execution error results	0 to 900 (0.1 step)
PEAK->REF LEVEL	Sets peak level of the waveform on the active trace to the reference level value	
AUTO REF LEVEL ####	Executes after each sweep finishes. Selects ON/OFF for the <PEAK → REF LEVEL> function.	####: ON/OFF
LEVEL UNIT #####	Sets the unit of a level scale.	####: dBm, dBm/nm

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### Note

For the AQ6375, dBm/nm and W/nm cannot be selected for LEVEL UNIT when the horizontal axis is wavenumber. (DBM/NM parameters cannot be set.)

---

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
Y SCALE DIVISION ##DIV	Sets the level scale division.	##: 8, 10, 12
REF LEVEL POSITION **DIV	Sets the position of the reference level on the level scale	0 to 12 (1 step)
SUB SCALE LOG **.*dB/D	Sets the sub scale value used for LOG scaling.	0.1 to 10.0dB/DIV (0.1 step)
SUB SCALELIN *.**/D	Sets the sub scale value used for LIN scaling.	0.005 to 1.250 (0.005 step)
SUB SCALE **.*dB/km	Sets the sub scale value used for dB/km scaling.	0.1 to 10.0 (0.1 step)
SUB SCALE **.*%/D	Sets the sub scale value used for %D scaling.	0.5 to 125.0 (0.1 step)
OFFSET LEVEL **.*dB	Sets the sub scale offset value used for LOG scaling	-99.9 to 99.9 (0.1 step)
OFFSET LEVEL ***.*dB/km	Sets the sub scale offset value used for dB/km scaling	-99.9 to 99.9 (0.1 step)
SCALE MINIMUM **.*	Sets the lower sub scale value used for linear scaling.	000 to 12.50 (0.01 step)
SCALE MINIMUM ***.*%	Sets the lower sub scale value used for &D scaling.	0.0 to 1250.0 (0.1 step)
LENGTH **.*km	Sets fiber length.	0.001 to 99.999 (0.001 step)
AUTO SUB SCALE ###	Automatically sets the sub scale from the calculated trace waveform	###: ON/OFF
SUB REF LEVEL POSITION **DIV	Sets the position of the reference level on the sub level scale	0 to 12 (1 step)

### 8.3 Program Function Commands

---

#### SETUP

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
RESOLUTION WL *.*.*nm	Sets the wavelength resolution.	AQ6370C/AQ6370D 0.020 to 2.000 (1-2-5 step) AQ6373/AQ6373B 0.010 to 10.000 (1-2-5 step) AQ6375 0.050 to 2.000 (1-2-5 step)
RESOLUTION WL @****@	Sets the value of variable @****@ to the wavelength resolution	@****@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, W2-W1, SPWD
RESOLUTION FREQ ***GHz	Sets the frequency resolution.	AQ6370C/AQ6370D 4 to 400 (1-2-4 step) AQ6373/AQ6373B 2 to 2000 (1-2-4 step) AQ6375 10 to 400 (1-2-4 step)
RESOLUTION FREQ@****@	Sets the value of variable @****@ to the frequency resolution	@****@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, W2-W1, SPWD, WAM2-WAM1, WAM4-WAM2
RESOLUTION WNUM *.*.*cm <sup>-1</sup>	Sets the wavenumber resolution.(only for AQ6375)	AQ6375 0.10 to 5.00 (1-2-5 step)
RESOLUTION WNUM @****@	Sets the value of variable @****@ to the wavenumber resolution(only for AQ6375)	@****@: G, H, I, J, K, P, Q, R, S, X, Y, Z, W2-W1, SPWD
SENS NORMAL/HOLD	Sets the measuring sensitivity to NORMAL/HOLD	
SENS NORMAL/AUTO	Sets the measuring sensitivity to NORMAL/AUTO	
SENS NORMAL	Sets measuring sensitivity to NORMAL	
SENS MID	Sets measuring sensitivity to MID.	
SENS HIGH1	Sets measuring sensitivity to HIGH1.	AQ6370C/AQ6370D
SENS HIGH1/CHOP	Sets measuring sensitivity to HIGH1/ CHOP	AQ6375
SENS HIGH2	Sets measuring sensitivity to HIGH2.	AQ6370C/AQ6370D
SENS HIGH2/CHOP	Sets measuring sensitivity to HIGH2/ CHOP	AQ6375
SENS HIGH3	Sets measuring sensitivity to HIGH3	AQ6370C/AQ6370D
SENS HIGH3/CHOP	Sets measuring sensitivity to HIGH3/ CHOP	AQ6375
CHOPPER #####	Switches chopper mode.	AQ6370C /AQ6370D/AQ6373/ AQ6373B

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
AVERAGE TIMES ***	Sets the number of averaging times.	1 to 999 (1 step)
AVERAGE TIMES @	Sets the number of averaging times to the value of variable @	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, M, N
SAMPLING POINT AUTO ###	Sets sampling points per sweep automatically.	###: ON/OFF
SAMPLING POINT ****	Sets sampling points per sweep.	101 to 50001 (1 step)
SAMPLING POINT @	Sets the sampling points to the variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, M, N
SAMPLING INTERVAL ****nm	Sets the measurement sampling interval per sweep	AQ6370C/AQ6370D/AQ6373/AQ6373B 0.001 to SPAN/101 (0.001 step) AQ6375 0.002 to SPAN/101 (0.001 step)
SAMPLING INTERVAL @	Sets the sampline interval per sweep to the value of variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, W2-W1, SPWD, WAM2-WAM1, WAM4-WAM3
MEASURE WAVELENGTH AIR	Sets the measurement wavelength to an air wavelength	
MEASURE WAVELENGTH VACUUM	Sets measurement wavelength to a vacuum wavelength.	
X SCALE UNIT WAVELENGTH	Sets axis X to wavelength display mode.	
X SCALE UNIT FREQUENCY	Sets axis X to frequency display mode.	
X SCALE UNIT WAVENUMBER	Sets axis X to wavenumber display mode.	AQ6375
SWEEP SPEED ##	Sets the sweep speed	AQ6370C /AQ6370D/AQ6373B ##: 1x/2x
PLS LIGHT MEASURE OFF	Turns OFF pulse light measurement mode	
PEAK HOLD****msec	Sets the HOLD time for PEAK HOLD ****: 1 to 9999 pulse light measurement	
EXTERNAL TRIGGER MODE	Sets external trigger mode	
EXTERNAL TRIGGER EDGE RISE	Detects the falling edge of an external trigger signal	
EXTERNAL TRIGGER EDGE FALL	Detects the rising edge of an external trigger signal	
EXTERNAL TRIGGER DELAY ****.*μs	After detection of an external trigger signal, and sets the delay time until data acquisition	0.0 to 1000.0 (0.1 step)
GATE MODE ****.*msec	Sets the sampling interval on the gate sampling mode	AQ6370C /AQ6370D/AQ6373B ****.* : 0.1 to 1000.0 (0.1 step)
GATE LOGIC POSI	Sets the gate signal logic of gate sampling to the positive logic	AQ6370C /AQ6370D/AQ6373B
GATE LOGIC NEGA	Sets the gate signal logic of gate sampling to the negative logic	AQ6370C /AQ6370D/AQ6373B
TLS SYNC SWEEP ###	Select the synchronous sweep function ON/OFF	AQ6370C/AQ6375 ###: ON/OFF
RESOLUTION CORRECTION ###	Turns the wavelength resolution correction function ON/OFF	AQ6370C /AQ6370D/AQ6373/AQ6373B ###: ON/OFF
SMOOTHING ###	Turns the smoothing function ON/OFF	AQ6370C/AQ6370D/AQ6373/AQ6373B ###: ON/OFF
FIBER CORE SIZE #####	Switches the fiber core size mode.	AQAQ6373/AQ6373B #####: SMALL/LARGE
FIBER CONNECTOR #####	Sets the optical fiber connector type.	AQ6370C/AQ6370D #####: NORMAL / ANGLED

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### 8.3 Program Function Commands

---

#### TRACE

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
ACTIVE TRACE #	Sets trace # to active trace.	#: A to G
DISPLAY #	Sets trace # to display mode.	#: A to G
BLANK #	Sets trace # to invisible mode.	#: A to G
WRITE #	Sets trace # to write mode.	#: A to G
FIX #	Sets trace # to data-fixing mode.	#: A to G
MAX HOLD #	Sets trace # to max. value detection mode.	#: A to G
MIN HOLD #	Sets trace # to min. value detection mode.	#: A to G
ROLL AVG # ***	Sets trace # to sequential addition averaging mode.	#: A to G, 2 to 100 (1 step)
C=A-B(LOG)	Sets trace C to TRACE A-B computation mode (LOG)	
C=B-A(LOG)	Sets trace C to TRACE B-A computation mode (LOG)	
C=A+B(LOG)	Sets trace C to TRACE A+B computation mode (LOG)	
C=A+B(LIN)	Sets trace C to TRACE A+B computation mode (LIN)	
C=A-B (LIN)	Sets trace C to TRACE A-B computation mode (LIN)	
C=B-A(LIN)	Sets trace C to TRACE B-A computation mode (LIN)	
C=1-k(A/B) k=*.****	Sets trace C to 1-k (TRACE A/B) 1.0000 to 20000.0000 computation mode (0.0001 step)	
C=1-k(B/A) k=*.****	Sets trace C to 1-k (TRACE B/A) 1.0000 to 20000.0000 computation mode (0.0001 step))	
F=C-D(LOG)	Sets trace F to TRACE C-D computation mode (LOG)	
F=D-C(LOG)	Sets trace F to TRACE D-C computation mode (LOG)	
F=C+D(LOG)	Sets trace F to TRACE C+D computation mode (LOG)	
F=D-E(LOG)	Sets trace F to TRACE D-E computation mode (LOG)	
F=D+E(LOG)	Sets trace F to TRACE D+E computation mode (LOG)	
F=C+D(LIN)	Sets trace F to TRACE C+D computation mode (LIN)	
F=C-D(LIN)	Sets trace F to TRACE C-D computation mode (LIN)	
F=D-C(LIN)	Sets trace F to TRACE D-C computation mode (LIN)	
F=D+E(LIN)	Sets trace F to TRACE D+E computation mode (LIN)	
F=D-E(LIN)	Sets trace F to TRACE D-E computation mode (LIN)	
F=E-D(LIN)	Sets trace F to TRACE E-D computation mode (LIN)	
G=C-F(LOG)	Sets trace G to TRACE C-F computation mode (LOG)	

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
G=F-C(LOG)	Sets trace G to TRACE F-C computation mode (LOG)	
G=C+F(LOG)	Sets trace G to TRACE C+F computation mode (LOG)	
G=E-F(LOG)	Sets trace G to TRACE E-F computation mode (LOG)	
G=F-E(LOG)	Sets trace G to TRACE F-E computation mode (LOG)	
G=E+F(LOG)	Sets trace G to TRACE E+F computation mode (LOG)	
G=C+F(LIN)	Sets trace G to TRACE C+F computation mode (LIN)	
G=C-F(LIN)	Sets trace G to TRACE C-F computation mode (LIN)	
G=F-C(LIN)	Sets trace G to TRACE F-C computation mode (LIN)	
G=E+F(LIN)	Sets trace G to TRACE E+F computation mode (LIN)	
G=E-F(LIN)	Sets trace G to TRACE E-F computation mode (LIN)	
G=F-E(LIN)	Sets trace G to TRACE F-E computation mode (LIN)	
G=NORM A	Sets the normalized data of trace A to be displayed on trace G.	
G=NORM B	Sets the normalized data of trace B to be displayed on trace G.	
G=NORM C	Sets the normalized data of trace C to be displayed on trace G.	
G=CURVE FIT A **dB	Sets curve fit processed data from TRACE A to be displayed on trace G.	0 to 99 (1 step)
G=CURVE FIT B **dB	Sets curve fit processed data from TRACE B to be displayed on trace G.	0 to 99 (1 step)
G=CURVE FIT C **dB	Sets curve fit processed data from TRACE C to be displayed on trace G.	0 to 99 (1 step)
G=CURVE FIT PEAK A **dB	Sets peak fit processed data from TRACE A to be displayed on trace G.	0 to 99 (1 step)
G=CURVE FIT PEAK B **dB	Sets peak curve fit processed data from trace B to be displayed on trace G.	0 to 99 (1 step)
G=CURVE FIT PEAK C **dB	Sets peak curve fit processed data from trace C to be displayed on trace G.	0 to 99 (1 step)
G=MARKER FIT **dB	Sets curve fit processed data from the placed delta marker to be displayed on trace G.	0 to 99 (1 step)
CVFIT OPERATION AREA####	Sets the target range for calculation when creating curve fit processed data.	#####: ALL/IN L1-L2/OUT L1-L2
CURVE FIT/CURVE FIT PEAK ALGO ####	Sets the fitting function when creating a fitting function.	#####: GAUSS/LORENZ/3RD POLY/4TH POLY/5TH POLY
TRACE #->#	Copies data from TRACE of the variable @ to TRACE of the variable @	#: A to G
TRACE # CLEAR	Clears trace # data.	#: A to G
ALL TRACE CLEAR	Clears all trace data.	

### 8.3 Program Function Commands

---

#### ZOOM

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
ZOOM CENTER WL ****.*nm	Sets the display scale's center wavelength.	AQ6370C/AQ6370D 600.000 to 1700.000 (0.001 step) AQ6373/AQ6373B 350.000 to 1200.000 (0.001 step) AQ6375 1200.000 to 2400.000 (0.001 step)
ZOOM CENTER @#####	Sets the value of variable @##### to the display scale center wavelength	AQ6370C/AQ6370D @#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), PKWL, MEANWL, WDMWL(CH), NFWL(CH), WAM1, WAM2, WAM3, WAM4
ZOOM CENTER FREQ ***.*THz	Sets the display scale's center frequency.	AQ6370C/AQ6370D 176.5000 to 500.0000 THz (0.0001 step) AQ6373/AQ6373B 250.0000 to 856.5000 THz (0.0001 step) AQ6375 125.5000 to 2500.0000 THz (0.0001 step)
ZOOM CENTER FREQ @#####	Sets the value of variable @##### to the display scale center frequency	AQ6370C/AQ6370D @#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, PKWL, MEANWL, WDMWL(CH), NFWL(CH) , WAM1, WAM2, WAM3, WAM4
ZOOM CENTER WNUM****.*cm <sup>-1</sup>	Sets the display scale's center wavenumber.(only for AQ6375)	4167.000 to 8333.000 cm <sup>-1</sup> (0.001 step)
ZOOM CENTER WNUM@#####	Sets the value of variable @##### to the display scale center wavenumber	@#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), S, X, Y, Z, WM, W1, W2, W(CH), PKWL, MEANWL, WDMWL(CH), NFWL(CH)
ZOOM SPAN WL ****.*nm	Sets the display scale's span.	AQ6370C/AQ6370D 0.1 to 1100.0 nm (0.1 step) AQ6373/AQ6373B 0.1 to 850.0 nm (0.1 step) AQ6375 0.1 to 1200.0 nm (0.1 step)
ZOOM SPAN WL @#####	Sets the value of variable @##### to the display scale span	AQ6370C/AQ6370D @#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, S, X, Y, Z, W2-W1, SPWD, WAM2-WAM1, WAM4-WAM3
ZOOM SPAN FREQ ***.*THz	Sets the display scale's span.	AQ6370C/AQ6370D 0.01 to 330.00 THz (0.01 step) AQ6373/AQ6373B 0.01 to 610.00 THz (0.01 step) AQ6375 0.01 to 130.00 THz (0.01 step)
ZOOM SPAN FREQ @#####	Sets the value of variable @##### to the display scale span	AQ6370C/AQ6370D @#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, W2-W1, SPWD, WAM2-WAM1, WAM4-WAM3
ZOOM SPAN WNUM ***.*cm <sup>-1</sup>	Sets the display scale's span.	AQ6375 0.5 to 4200.0 cm <sup>-1</sup> (0.1 step)
ZOOM SPAN WNUM @#####	Sets the value of variable @##### to the display scale span. (only for AQ6375)	@#####: G, H, I, J, K, P, Q, R, S, X, Y, Z, W2-W1, SPWD

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
ZOOM START WL ****.***nm	Sets the starting wavelength of the display scale.	AQ6370C 50.000 to 1699.950 nm (0.001 step) AQ6373/AQ6373B 1.000 to 1199.950 nm (0.001 step) AQ6375 600.000 to 2400.000 nm (0.001 step)
ZOOM START FREQ ***.***THz	Sets the starting frequency of the display scale.	AQ6370C 11.5000 to 499.9950 THz (0.0001 step) AQ6373/AQ6373B 10.0000 to 856.4950 THz (0.0001 step) AQ6375 60.0000 to 250.0000 THz (0.0001 step)
ZOOM START WNUM ***.***cm <sup>-1</sup>	Sets the starting wavenumber of the display scale.	AQ6375 2067.000 to 8333.000 cm <sup>-1</sup> (0.001 step)
ZOOM STOP WL ****.***nm	Sets the ending wavelength of the display scale.	AQ6370C 600.050 to 2250.000 nm (0.001 step) AQ6373/AQ6373B 350.050 to 1625.000 nm (0.001 step) AQ6375 1200.000 to 3000.000 nm (0.001 step)
ZOOM STOP FREQ ***.***THz	Sets the ending frequency of the display scale.	AQ6370C 176.5050 to 665.0000 (0.0001 step) AQ6373/AQ6373B 250.0050 to 999.9000 (0.0001 step) AQ6375 125.0000 to 315.0000 (0.0001 step)
ZOOM STOP WNUM ***.***cm <sup>-1</sup>	Sets the ending wavenumber of the display scale.	AQ6375 4167.000 to 10433.000 cm <sup>-1</sup> (0.001 step)
PEAK->ZOOM CENTER	Sets the peak wavelength of the waveform on the active trace. Sets the wavelength to the display scale's center wavelength.	
OVERVIEW DISPLAY OFF	Sets OVERVIEW display during ZOOM to OFF	
OVERVIEW DISPLAY LEFT	Sets OVERVIEW display during ZOOM to the left side of the waveform screen	
OVERVIEW DISPLAY RIGHT	Sets OVERVIEW display during ZOOM to the right side of the waveform screen	
OVERVIEW SIZE LARGE	Sets OVERVIEW display during ZOOM to a large display	
OVERVIEW SIZE SMALL	Sets OVERVIEW display during ZOOM to a small display	
ZOOM INITIALIZE	Resets the display scale to the initial state.	

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

## 8.3 Program Function Commands

---

### DISPLAY

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
NORMAL DISPLAY	Sets the screen into normal display mode.	
SPLIT DISPLAY	Sets the screen into split display mode.	
TRACE # UPPER	Sets trace # to the top screen of the #: A to G split display.	
TRACE # LOWER	Sets trace # to the bottom screen of #: A to G the split display.	
UPPER HOLD ###	Holds the top screen of the split display. ####: ON/OFF	
LOWER HOLD ###	Holds the bottom screen of the split display. ####: ON/OFF	
LABEL '---56 chars---'	Displays a label comment in the label area. If a semicolon ( ; ) is added to the end, the comment (variable value) specified by the next LABEL command is displayed.	
LABEL @@@@@	Sets the contents of variable @@@@@ to the label area	AQ6370C/AQ6370D @:@:@:@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), W2-W1, LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), NFCHN, NFWL(CH), NFLVLI(CH), NFLVLO(CH), NFASELV(CH), NFGAIN(CH), NFNF(CH), MKPWR, PMD, M, N, CH, A\$, B\$, C\$, D\$, FILE\$, TIME\$, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3
LABEL @@@@@;	Sets the contents of variable @@@@@ to the label display. The comment (variable value) specified by the next LABEL command is displayed.	AQ6370C/AQ6370D @:@:@:@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), W2-W1, LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), NFCHN, NFWL(CH), NFLVLI(CH), NFLVLO(CH), NFASELV(CH), NFGAIN(CH), NFNF(CH), MKPWR, PMD, M, N, CH, A\$, B\$, C\$, D\$, FILE\$, TIME\$, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
LABEL CLEAR	Clears the LABEL command in the label area.	
NOISE MASK ***dB	Displays waveform data with the data at or below the set level masked	OFF (-999), -100 to 0 (1 step)
MASK LINE VERTICAL	Sets the mask value in the noise mask function or lower to zero.	
MASK LINE HORIZONTAL	Sets the mask value in the noise mask function or lower to the mask value.	
TRACE # CLEAR	Clears trace # data. #: A to G	
ALL TRACE CLEAR	Clears all trace data.	
DISPLAY OFF	Turns the display OFF	AQ6370C/AQ6370D/AQ6373B
DISPLAY ON	Turns the display ON	AQ6370C/AQ6370D/AQ6373B

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### MARKER

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
MARKER ****.***nm	Sets the marker to the specified wavelength position on the active trace (according to the wavelength value)	AQ6370C 600.000 to 1700.000 (0.001 step) AQ6373/AQ6373B 350.000 to 1200.000 (0.001 step) AQ6375 600.000 to 2400.000 (0.001 step)
MARKER ***.****THz	Sets the marker to the specified wavelength position on the active trace (according to the frequency value)	AQ6370C 176.5000 to 500.0000 (0.0001 step) AQ6373/AQ6373B 250.0000 to 856.5000 (0.0001 step) AQ6375 60.0000 to 250.0000 (0.0001 step)
MARKER ***.****cm <sup>-1</sup>	Sets the marker to the specified wavenumber position on the active trace (according to the wavenumber value)	AQ6375 2067.000 to 8333.000 (0.0001 step)
MARKER @@@@#@	Sets a marker to the wavelength position of variable @@@@#@	AQ6370C/AQ6370D @@@@#@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), MEANWL, PKWL, WDMWL(CH), NFWL(CH), WAM1, WAM2, WAM3, WAM4
SET MARKER ****	Sets fixed marker **** to the moving marker position	1 to 1024 (1 step)
SET MARKER @	Sets the fixed marker of variable @ to the moving marker position	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
CLEAR MARKER ****	Clears fixed marker ****.	1 to 1024 (1 step)
CLEAR MERKER @	Clears the fixed marker of variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, N, M
MARKER->CENTER	Sets the wavelength value of a marker to the measurement center wavelength.	
MARKER->ZOOMCENTER	Sets the wavelength value of a marker to the display scale's center wavelength	
MARKER->REF LEVEL	Sets the marker level value to thereference level.	

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
ADV MARKER ##,***.*nm	Sets the advanced marker to the specified wavelength position (according to the wavelength value)	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4 ***.*: 600.000 to 1700.000 (0.001 step)
ADV MARKER ##,***.*THz	Sets the advanced marker to the specified frequency position (according to the frequency value)	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4 ***.*: 176.5000 to 500.0000 (0.001 step)
ADV MARKER ##,@@@@@	Sets an advanced marker to the wavelength position of variable @@@@@	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4, @@@@@: G,H,I,J,K,P,Q,R,S,X,Y,Z,WM,W1,W2,W(CH),WAM1,WAM2,WAM3,WA M4,MEANWL,PKWL,WDMWL(CH),NFWL(CH)
ADV MARKER TRACE ##,###	Sets the trace of advanced marker to ####	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4 ###: TRA/TRB/TRC/TRD/TRE/TRF/TRG)
ADV MARKER SELECT ##,#####	Sets the type of advanced marker to ####	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4 #####: OFF/NORMAL/DENSITY/INTEGRAL
ADV MARKER INTEGRAL RANGE ##,***.*GHz	Sets the integration range of the advanced marker	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4 ***.* : 1.0 to 999.9 (0.1 step)
ADV MARKER PEAK SEARCH ##	Detects the peak and sets the advanced marker	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4
ADV MARKER BOTTOM SEARCH ##	Detects the bottom and sets the advanced marker	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4
ADV MARKER NEXT SEARCH ##	Detects the next peak whose level is the current advanced marker position and sets the advanced marker	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4
ADV MARKER SEARCH RIGHT ##	Detects the closest peak to the right of the current advanced marker position and sets the advanced marker	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4
ADV MARKER SEARCH LEFT ##	Detects the closest peak to the left of the current advanced marker position and sets the advanced marker	AQ6370C/AQ6370D/AQ6373B ##:M1,M2,M3,M4
ADV MARKER BANDWIDTH **.*nm	Sets the normalization bandwidth of the power density marker	AQ6370C/AQ6370D/AQ6373B **.* : 0.1 to 10.0 (0.1 step)
ADV MARKER ALL CLEAR	Clears all advanced markers on the screen	AQ6370C/AQ6370D/AQ6373B
ALL MARKER CLEAR	Clears all markers from the screen.	
LINE MARKER1****.*nm	Sets line marker 1 to a specified wavelength position (according to a wavelength value).	AQ6370C 600.000 to 1700.000 (0.001 step) AQ6373/AQ6373B 350.000 to 1200.000 (0.001 step) AQ6375 600.000 to 2400.000 (0.001 step)
LINE MARKER1 ***.*THz	Sets line marker 1 to a specified frequency position (according to a frequency value).	AQ6370C 176.5000 to 500.0000 (0.0001 step) AQ6373/AQ6373B 250.0000 to 856.5000 (0.0001 step) AQ6375 60.5000 to 250.0000 (0.0001 step)

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
LINE MARKER1 ***.****cm <sup>-1</sup>	Sets line marker 1 to a specified wavenumber position (according to a wavenumber value).	AQ6375 2067.000 to 8333.000 (0.001 step)
LINE MARKER1@{@@:@@	Sets line marker 1 to the wavelength position of variable @@@@	AQ6370C/AQ6370D @{@@:@@:E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), MEANWL, PKWL, WDMWL(CH), NFLWL(CH), WAM1, WAM2, WAM3, WAM4
LINE MARKER2****.***nm	Sets line marker 2 to a specified wavelength position (according to a wavelength value).	AQ6370C/AQ6370D 600.000 to 1700.000 (0.001 step) AQ6373/AQ6373B 350.000 to 1200.000 (0.001 step) AQ6375 600.000 to 2400.000 (0.001 step)
LINE MARKER2 ***.****THz	Sets line marker 2 to a specified frequency position (according to a frequency value).	AQ6370C/AQ6370D 176.5000 to 500.0000 (0.0001 step) AQ6373/AQ6373B 250.0000 to 856.5000 (0.0001 step) AQ6375 60.0000 to 250.0000 (0.0001 step)
LINE MARKER2 ***.****cm <sup>-1</sup>	Sets line marker 2 to a specified wavenumber position (according to a wavenumber value).	AQ6375 2067.000 to 8333.000 (0.001 step)
LINE MARKER2@{@@:@@	Sets line marker 2 to the wavelength position of variable @@@@	AQ6370C/AQ6370D @{@@:@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W(CH), MEANWL, PKWL, WDMWL(CH), NFLWL(CH), WAM1, WAM2, WAM3, WAM4
LINE MARKER3****.***dB	Sets line marker 3 to a specified level.	-139.90 to 159.90 (0.01 step)
LINE MARKER3 ****.***dBm	Sets line marker 3 to a specified level.	-210.00 to 50.00 (0.01 step)
LINE MARKER3 *.***##	Sets line marker 3 to a specified level.	1.00pW to 1000mW (1.00 to 9.99[pW, nW, mW, mW]: 0.01 step 10.0 to 99.9(100) [pW, nW, mW, (mW): 0.1 step 100 to 999 [pW, nW, mW, mW]: 1 step ## is , pW, nW, mW, mW (Select one of the above)
LINE MARKER3 **.***	Sets line marker 3 to a specified level.	0.00 to 2500.00 (0.01 step)
LINE MARKER3@{@@:@@	Sets line marker 3 to the level position of variable @@@@	AQ6370C/AQ6370D @{@@:@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, LM, L1, L2, L(CH), PKLVL, WDMLVL(CH), NFLVI(CH), NFLVO(CH), NFASELV(CH), MKPWR, LAM1, LAM2, LAM3, LAM4

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
LINE MARKER4****.***dB	Sets line marker 4 to a specified level.	-139.90 to 159.90 (0.01 step)
LINE MARKER4 ****.***dBm	Sets line marker 4 to a specified level.	-210.00 to 50.00 (0.01 step)
LINE MARKER4 *.*##	Sets line marker 4 to a specified level.	1.00pW to 1000mW (1.00 to 9.99[pW, nW, μW, mW]: 0.01 step 10.0 to 99.9(100) [pW, nW, μW, (mW): 0.1 step 100 to 999 [pW, nW, μW, mW]: 1 step) ## is , pW, nW, μW, mW(Select one of the above)
LINE MARKER4 **.***	Sets line marker 4 to a specified level.	0.00 to 2500.00 (0.01 step)
LINE MARKER4@*****	Sets line marker 4 to the level position of variable @*****	@@@@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, LM, L1, L2, L(CH), PKLVL, WDMLVL(CH), NFLVLI(CH), NFLVLO(CH), NFASELV(CH), MKPWR
MARKER L1-L2->SPAN	Sets the range surrounded by line markers 1 and 2 to the measuring span.	
MARKER L1-L2->ZOOM SPAN	Sets the range surrounded by line markers 1 and 2 to the display scale span.	
LINE MARKER CLEAR	Clears line markers on the screen.	
MARKER OFFSET LIST	Displays the difference from the moving marker.	
MARKER SPACING LIST	Displays a difference to a neighboring marker.	
MARKER AUTO UPDATE ###	Makes the level position of a fixed marker follow the active trace waveform.	###: ON/OFF
MARKER UNIT nm	Sets a wavelength marker value to the wavelength display.	
MARKER UNIT THz	Sets a wavelength marker value to the frequency display.	
MARKER UNIT cm <sup>-1</sup>	Sets a wavelength marker value to the wavenumber display.	AQ6375
SEARCH/ANA L1-L2 ###	Selects ON/OFF for the analysis function in the range surrounded by line markers 1 and 2	###: ON/OFF
SEARCH/ANAZOOM AREA ###	Selects ON/OFF for the analysis function of the display scale range	###: ON/OFF
MARKER LIST PRINT	Prints out multiple marker values.	AQ6370C/AQ6373/AQ6375

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

**PEAK SEARCH**

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
PEAK SEARCH	Performs a peak search on the active trace waveform	
BOTTOM SEARCH	Performs a bottom search on the active trace waveform	
NEXT SRCH	Searches for the next peak/bottom after the peak/bottom level of the active trace waveform	
NEXT SRCH RIGHT	Searches for the peak/bottom to the right of the peak/bottom marker of the active trace waveform	
NEXT SRCH LEFT	Searches for the peak/bottom to the left of the peak/bottom marker of the active trace waveform	
SET MARKER ****	Sets fixed marker to the moving marker **** position	1–1024 (1 step)
SET MARKER @	Sets the fixed marker of variable @ to the moving marker position	@: G, H, I, J, K, P, Q, R, S, X, Y, Z, S, N, M
CLEAR MARKER ****	Clears fixed marker ****.	1–1024 (1 step)
CLEAR MERKER @	Clears the fixed marker of variable @.	@: G, H, I, J, K, P, Q, R, S, X, Y, Z, S, N, M
ALL MARKER CLEAR	Clears all markers from the screen.	
AUTO SEARCH ###	Selects ON/OFF of the peak/bottom search function conducted each sweep	###: ON/OFF
MODE DIFF **.**dB	Sets the level difference of the mode judgment criteria used for peak search or waveform analysis.	0.01–50.00 (0.01 step)
SEARCH/ANA L1-L2 ###	Selects ON/OFF for the analysis function in the range surrounded by line markers 1 and 2	###: ON/OFF
SEARCH/ANAZOOM AREA ###	Selects ON/OFF for the analysisFunction of the display scale range	###: ON/OFF
SEARCH MODE #####	Sets the search mode	AQ6370C/AQ6370D/AQ6373B #####: SINGLE/MULTI
MULTI SEARCH THRESH **.**dB	Sets the multi search threshold	AQ6370C/AQ6370D/AQ6373B 0.01: 99.99 (0.01 step)
MULTI SEARCH SORT BY #####	Sets the multi search detection list sort order	AQ6370C/AQ6370D/AQ6373B #####: WL/LEVEL

## 8.3 Program Function Commands

---

### ANALYSIS

For the AQ6373/AQ6373B, replace “WDM” with “OSNR(WDM)” for all commands that start with “WDM.”

Example) WDM ANALYSIS→OSNR(WDM) ANALYSIS

The following commands are not available.

All commands that start with “EDFA-NF”

The following commands are not available on the AQ6375 if the wavenumber markers are set.

- All commands that start with “WDM”
- All commands that start with “EDFA-NF”
- All commands that start with “FILTER”

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
SPEC WD THRESH **.**dB	Performs a THRESH-based spectrum width search according to the specified threshold value	0.01 to 50.00 (0.01 step)
PARAM THRESHK **.**	Sets the magnification for the THRESH based spectrum width search	1.00 to 10.00 (0.01 step)
PARAM THRESH MODE FIT ###	Turns ON/OFF the function that sets the marker to the peak of the mode when performing a THRESH-based spectrum width search.	###: ON/OFF
SPEC WD ENV **.**dB	Performs an envelope-based spectrum width search using the specified threshold value	0.01 to 50.00 (0.01 step)
PARAM ENV TH2 **.**dB	Sets the cutoff value for the envelope-based spectrum width search.	0.01 to 50.00 (0.01 step)
PARAM ENV K **.**dB	Sets the cutoff value for the envelope-based using the THRESH method.	1.00 to 10.00 (0.01 step)
SPEC WD RMS **.**dB	Performs an RMS-based spectrum width search according to a specified threshold.	0.01 to 50.00 (0.01 step)
PARAM RMS K **.**	Sets the magnification for an RMS-based spectrum width search	1.00 to 10.00 (0.01 step)
SPEC WD PEAK RMS **.**dB	Performs an RMS-based spectrum width search according to a specified threshold value	0.01 to 50.00 (0.01 step)
PARAM PEAK RMS K**.**	Sets the magnification for a PEAK-RMS-based spectrum width search	1.00 to 10.00 (0.01 step)
SPEC WD NOTCH **.**dB	Measures the NOTCH width using a specified threshold value	0.01 to 50.00 (0.01 step)
PARAM NOTCH K **.**	Sets a magnification based on notch width measurement	1.00 to 10.00 (0.01 step)
NOTCH FROM #####	Sets the reference for making notch width measurements.	#####: PEAK/BOTTOM
SMSR *	Sets the execution mode applied in SMR measurement	1, 2, 3, 4
SMSR MASK ±**.**nm	Sets a mask range close to the peak during SMSR1 measurements	0.00 to 99.99 (0.01 step)

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
POWER	Performs power analysis	
POWER OFFSET ***.**dB	Sets a correction value in power measurements	-10.00 to 10.00 (0.01 step)
DFB-LD ANALYSIS	Performs analysis necessary for DFB-LD.	
FP-LD ANALYSIS	Performs analysis necessary for FP-LD.	
LED ANALYSIS	Performs analysis necessary for LED.	
PMD ANALYSIS	Performs analysis necessary for PMD.	
PMD THRESH **.**dB	Sets a threshold value for PMD analysis	0.01 to 50.00 (0.01 step)
WDM ANALYSIS	Performs analysis necessary for WMD.	
WMD THRESH **.**dB	Sets a threshold value for WDM analysis	0.1 to 99.9 (0.1 step)
WDM MODE DIFF ***.**dB	Sets the minimum peak/bottom difference for channel detection during WDM analysis.	0.01 to 50.00 (0.01 step)
WDM DISPLAY MASK OFF	Cancels level threshold value settingwhen masking display channels	
WDM DISPLAY MASK ****.**dB	Sets the level threshold value when masking display channels	-100.00 to 0.00 (0.01 step)
WDM NOISE ALGO AUTO-FIXFIX	Sets noise level measuring algorithm to AUTO	
WDM NOISE ALGO MANUAL FIX	Sets noise level measuring algorithmto MANUAL FIX	
WDM NOISE ALGO AUTO CTR	Sets noise level measuring algorithmto AUTO CTR	
WDM NOISE ALGO MANUAL CTR	Sets noise level measuring algorithmto MANUAL CTR	
WDM NOISE ALGO PIT	Sets noise level measuring algorithmto PIT	
WDM NOISE AREA **.**nm	Sets an area used for noise level analysis in a range centered on channel wavelength.	0.01 to 10.00 (0.01 step)
WDM NOISE AREA @	Sets an area used for noise level analysis in a range of variable @ centered on channel wavelength.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
WDM MASK AREA **.**nm	Sets the signal light spectrum range to mask as centered on channel wavelength	0.01 to 10.00 (0.01 step)
WDM MASK AREA @	Sets the signal light spectrum range to mask as centered on channel wavelength, to the range of variable @	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
WDM FITTING ALGO LINEAR	Sets the fitting algorithm for finding noise level to linear interpolation mode	
WDM FITTING ALGO GAUSS	Sets the fitting algorithm for finding noise level to normal distribution curve mode	
WDM FITTING ALGO LORENZ	Sets the fitting algorithm for finding noise level to Lorenz curve mode	
WDM FITTING ALGO3RD POLY	Sets the fitting algorithm for finding noise level in 3rd polynomial mode.	

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
WDM FITTING ALGO4TH POLY	Sets the fitting algorithm for finding noise level in 4th polynomial mode	
WDM FITTING ALGO5TH POLY	Sets the fitting algorithm for finding noise level in 5th polynomial mode	
WDM NOISE BANDWIDTH *.*nm	Sets bandwidth applied in measuring noise	0.01 to 1.00 (0.01 step)
WDM DUAL TRACE ####	Makes setting so that both TRACES A ####: ON/OFF and B are used in analyzing WDM.	
WDM DISPLAY ABSOLUTE	Sets the display of WDM analysis results to absolute value display.	
WDM DISPLAY RELATIVE	Sets the display of WDM analysis results to relative value display.	AQ6370C/AQ6370D/AQ6375
WDM DISPLAY DRIFT MEAS	Sets the display of WDM analysis results to drift value display (drift display using past measurement wavelength as a reference)	
WDM DISPLAY DRIFT GRID	Sets the display of WDM analysis results to drift value display (using grid wavelength as a reference)	AQ6370C/AQ6370D/AQ6375
WDM CH RELATION #####:	Sets the display format of an inter-channel level absolute value when WDM analysis display is in absolute value display	#####: OFFSET/SPACING
WDM REF CHANNELHIGHEST	Sets the reference channel when the CH RELATION is OFFSET to the channel with the highest level	
WDM CHANNEL NO.****	Sets the reference channel when the CH RELATION is OFFSET	1 to 1024 (1 step)
WDM MAX/MIN RESET	Resets MAX/MIN data during DRIFT (MEAS, GRID) measurement	
WDM OUTPUT SLOPE ####	Displays the least square approximation line of a channel peak.	####: ON/OFF
WDM POINT DISPLAY ####	Displays the range of data used in fitting on the waveform screen.	####: ON/OFF
WDM SIGNAL POWER#####	Sets the signal power calculation method.	AQ6370C/AQ6373/AQ6373B #####: PEAK / INTEGRAL
WDM INTEGRAL RANGE ***GHz	Sets the signal power integral range.	AQ6370C/AQ6373/AQ6373B 10 to 999 (1step)
COLOR ANALYSIS	Performs a color analysis	AQ6373/AQ6373B
EDFA NF ANALYSIS	Performs analysis necessary for EDFA-NF measurements.	AQ6370C/AQ6370D/AQ6375
EDFA NF THRESH **.*dB	Sets an EDFA-NF analysis threshold.	AQ6370C/AQ6370D/AQ6375 0.1 to 99.9 (0.1 step)
EDFA NF MODE DIFF **.*dB	Sets the minimum peak/bottom difference for channel detection during EDFA-NF analysis.	AQ6370C/AQ6370D/AQ6375 0.01 to 50.00 (0.01 step)
EDFA NF OFFSET(IN) ***.*dB	Sets a signal light offset value used for NF and Gain calculation	AQ6370C/AQ6370D/AQ6375 -99.99 to 99.99 (0.01 step)
EDFANF OFFSET(IN)@@@@@	Sets the offset value of the signal used for NF and Gain calculation to the variable @@@@@	AQ6370C/AQ6370D/AQ6375 @@@@@:E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
EDFA NF OFFSET(OUT) ***.**dB	Sets an output light offset value used for NF and Gain calculation	AQ6370C/AQ6370D/AQ6375 -99.99 to 99.99 (0.01 step)
EDFA NF OFFSET(OUT) @#####	Sets an output light offset value used for NF and Gain calculation to the variable @#####	AQ6370C/AQ6370D/AQ6375 @#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
EDFA NF ASE ALGOAUTO FIX	Sets the ASE level measuring algorithm to ATUO FIX	AQ6370C/AQ6370D/AQ6375
EDFA NF ASE ALGO MANUAL FIX	Sets the ASE level measuring algorithm to MANUAL FIX	AQ6370C/AQ6370D/AQ6375
EDFA NF ASE ALGOAUTO CTR	Sets the ASE level measuring algorithm to AUTO CTR	AQ6370C/AQ6370D/AQ6375
EDFA NF ASE ALGOMANUAL CTR	Sets the ASE level measuring algorithm to MANUAL CTR	AQ6370C/AQ6370D/AQ6375
EDFA NF ASE AREA **.**nm	Sets an area used for ASE level analysis in a range centered on channel wavelength	AQ6370C/AQ6370D/AQ6375 0.01 to 10.00 (0.01 step)
EDFA NF ASE AREA @	Sets an area used for ASE level analysis in a range centered on variable @	AQ6370C/AQ6370D/AQ6375 @#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
EDFA NF MASK AREA **.**nm	Sets the signal light spectrum range to mask as centered on channel wavelength	AQ6370C/AQ6370D/AQ6375 0.01 to 10.00 (0.01 step)
EDFA NF MASK AREA @	Sets the signal light spectrum range to mask as centered on variable @	AQ6370C/AQ6370D/AQ6375 @#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
EDFA NF FITTING ALGO LINEAR	Sets the fitting algorithm for finding ASE level to linear interpolation mode	AQ6370C/AQ6370D/AQ6375
EDFA NF FITTING ALGO GAUSS	Sets the fitting algorithm for finding ASE level to normal distribution curve mode	AQ6370C/AQ6370D/AQ6375
EDFA NF FITTING ALGO LORENZ	Sets the fitting algorithm for finding ASE level to Lorenz curve mode	AQ6370C/AQ6370D/AQ6375
EDFA NF FITTING ALGO 3RD POLY	Sets the fitting algorithm for finding ASE level in 3rd polynomial mode	AQ6370C/AQ6370D/AQ6375
EDFA NF FITTING ALGO 4TH POLY	Sets the fitting algorithm for finding ASE level in 4th polynomial mode	AQ6370C/AQ6370D/AQ6375
EDFA NF FITTING ALGO 5TH POLY	Sets the fitting algorithm for finding ASE level in 5th polynomial mode	AQ6370C/AQ6370D/AQ6375
EDFA NF POINTDISPLAY ###	Displays the range of data used in fitting on the waveform screen.	AQ6370C/AQ6370D/AQ6375 ###: ON/OFF
EDFA NF RES BWMEASURED	For the resolution, use the value determined from the waveform using THRESH 3dB analysis.	AQ6370C/AQ6370D/AQ6375
EDFA NF RES BWCAL DATA	For the resolution, use the actual resolution value stored in the instrument.	AQ6370C/AQ6370D/AQ6375
EDFA NF SHOTNOISE ###	Set whether to include/not include Shot Noise in the NF computation	AQ6370C/AQ6370D/AQ6375 ###: ON/OFF
FILTER(PEAK) ANALYSIS	Performs optical filter (PEAK) analysis.	
FILTER(BOTTOM) ANALYSIS	Performs optical filter (BOTTOM) analysis.	
WDMFILTER(PEAK) ANALYSIS	Performs multi-channel type optical filter (PEAK) analysis	AQ6370C/AQ6375
WDM FILTER(BOTTOM) ANALYSIS	Performs multi-channel type optical filter (BOTTOM) analysis.	AQ6370C/AQ6375

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
SWITCH DISPLAY TO TRACE&TABLE	Displays both waveforms and tables in the display of analysis results.	
SWITCH DISPLAY TO TABLE	Displays only tables in the display of analysis results.	
SWITCH DISPLAY TO TRACE	Displays only traces in the display of analysis results.	
SWITCH DISPLAY TO GRAPH&TABLE	Displays both graphs and tables in the display of analysis results	AQ6370C
SWITCH DISPLAY TO GRAPH	Displays only graphs in the display of analysis results	AQ6370C
AUTO ANALYSIS ###	Selects ON/OFF of the waveform analysis function activated each time a sweep is made	###: ON/OFF
ANALYSIS RESULT PRINT	Prints out analysis results.	AQ6370C/AQ6373/AQ6375
RESULT WRITE INT: #####.***'	Specifies a filter name and saves analysis results to internal memory.	'#####.***': File name
RESULT WRITE EXT: #####.***'	Specifies a file name and saves analysis results to internal memory.	'#####.***': File name
RESULT WRITE INT	Saves analysis results in internal memory. File names are assigned automatically.	
RESULT WRITE EXT	Saves analysis results in external memory. File names are assigned automatically.	
RESULT WRITE INT @@	Specifies a file name and saves analysis results to internal memory under the file name specified in the variable @@.	@@: A\$, B\$, C\$, D\$
RESULT WRITE EXT @@	Specifies a file name and saves analysis results to floppy disk under the file name specified in the variable @@.	@@: A\$, B\$, C\$, D\$
SEARCH/ANA L1-L2 ###	Sets ON/OFF for the analysis function in the range surrounded by line markers 1 and 2.	###: ON/OFF
SEARCH/ANAZOOM AREA ###	Selects ON/OFF for the analysis function of the display scale range	###: ON/OFF

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### MEMORY

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
SAVE #>MEMORY **	Writes the contents of the selected TRACE from the specified memory number.	0 to 63 (1 step) #: A, B, C, D, E, F, G
SAVE #>MEMORY @	Writes the contents of the selected TRACE from the memory number in variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z #: A, B, C, D, E, F, G
RECALL MEMORY **->#	Reads the contents of the selected TRACE from the specified memory number.	0 to 63 (1 step) #: A, B, C, D, E, F, G
RECALL MEMORY @->#	Reads the contents of the selected TRACE from the memory number in variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z #: A, B, C, D, E, F, G
CLEAR MEMORY **	Clears trace data in the memory	0 to 63 (1 step)
CLEAR MEMORY @	Clears the trace data in the memory specified by the variable @/	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

**FILE**

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
WRITE TRACE # INT: #####.***'	Assign a file name to specified TRACE data and save it to internal memory	#: A, B, C, D, E, F, G '#####.***': file name
WRITE TRACE # EXT: ' #####.***'	Assign a file name to specified TRACE data and save it in external memory	#: A, B, C, D, E, F, G '#####.***': file name
WRITE TRACE # INT	Saves specified TRACE data in internal memory. File names are assigned automatically	#: A, B, C, D, E, F, G
WRITE TRACE # EXT	Saves specified TRACE data in external memory. File names are assigned automatically	#: A, B, C, D, E, F, G
WRITE TRACE # INT@@	Saves specified TRACE data in internal memory under the file name specified in the variable @@.	#: A, B, C, D, E, F, G @@: A\$, B\$, C\$, D\$
WRITE TRACE # EXT @@	Saves specified TRACE data in external memory under the file name specified in the variable @@.	#: A, B, C, D, E, F, G @@: A\$, B\$, C\$, D\$
TRACE WRITE:BINARY	Sets the data storage format to BINARY	
TRACE WRITE:CSV	Sets the data storage format to CSV	
WRITE ALL TRACE INT: #####.CSV'	Specify a file name for all TRACE data and save to internal memory.	'#####.CSV': File name
WRITE ALL TRACE EXT: #####.CSV'	Specify a file name for all TRACE data and save to external memory.	'#####.CSV': File name
WRITE ALL TRACE INT:	Save all TRACE data to internal memory. A file name is automatically assigned	
WRITE ALL TRACE EXT:	Save all TRACE data to external memory. A file name is automatically assigned	
WRITE ALL TRACE INT @@	Save all TRACE data under file names specified by the @@ variable to internal memory	@@: A\$, B\$, C\$, D\$
WRITE ALL TRACE EXT @@	Save all TRACE data under file names specified by the @@ variable to external memory	@@: A\$, B\$, C\$, D\$
WRITE MEMORY ** INT: #####.***'	Specifies a file name and save the memory data in internal memory	**: 0 to 63 (1 step) '#####.***': file name
WRITE MEMORY ** EXT: #####.***'	Specifies a file name and save the memory data in external memory	**: 0 to 63 (1 step) '#####.***': file name
WRITE MEMORY**INT	Saves memory data in internal memory. File names are assigned automatically	**: 0 to 63 (1 step)
WRITE MEMORY ** EXT	Saves memory data in external memory. File names are assigned automatically	**: 0 to 63 (1 step)
WRITE MEMORY ** INT @@	Saves memory data under the file name specified in the variable @@ in internal memory	**: 0 to 63 (1 step) @@: A\$, B\$, C\$, D\$
WRITE MEMORY ** EXT @@	Saves memory data under the file name specified in the variable @@ in external memory	**: 0 to 63 (1 step) @@: A\$, B\$, C\$, D\$
WRITE GRAPH INT: #####.***'	Specifies a file name and saves graphic data in internal memory.	'#####.***': File name

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
WRITE GRAPH EXT: #####.***'	Specifies a file name and saves graphic data in external memory.	'#####.***': file name
WRITE GRAPH INT	Saves graphic data in internal memoryFile names are assigned automatically	
WRITE GRAPH EXT	Saves graphic data in external memoryFile names are assigned automatically	
WRITE GRAPH INT @@	Saves graphic data under the file name specified by the variable @@ in internal memory.	@@: A\$, B\$, C\$, D\$
WRITE GRAPH EXT @@	Saves graphic data under the file name specified by the variable @@ in external memory.	@@: A\$, B\$, C\$, D\$
GRAPH COLOR MODE:	Sets the graphic color mode to black & white.	
GRAPH COLOR MODE:COLOR	Sets the graphic color mode to screencolor mode	
GRAPH COLOR MODE: PRESET COLOR	Sets the graphic color mode to PRESET COLOR (waveform in color, background in black & white)	
GRAPH TYPE:BMP	Sets the graphic file type to BMP	
GRAPH TYPE:TIFF	Sets the graphic file type to TIFF	
WRITE SETTING INT: #####.ST7'	Specifies a file name and savessetting data to internal memory.	AQ6375 '#####.ST7': file name
WRITE SETTING INT: #####.ST8'	Specifies a file name and savessetting data to internal memory.	AQ6370C '#####.ST8': file name
WRITE SETTING INT: #####.ST9'	Specifies a file name and savessetting data to internal memory.	AQ6373/AQ6373B '#####.ST9': file name
WRITE SETTING EXT: #####.ST7'	Specifies a file name and savessetting data to external memory.	AQ6375 '#####.ST7': file name
WRITE SETTING EXT: #####.ST8'	Specifies a file name and savessetting data to external memory.	AQ6370C '#####.ST8': file name
WRITE SETTING EXT: #####.ST9'	Specifies a file name and savessetting data to external memory.	AQ6373/AQ6373B '#####.ST9': file name
WRITE SETTING INT	Saves setting data to internal memoryFile names are assigned automatically	
WRITE SETTING EXT	Saves setting data to external memoryFile names are assigned automatically	
WRITE SETTING INT @@	Saves setting data under the file name specified in the variable @@ to internal memory.	@@: A\$, B\$, C\$, D\$
WRITE SETTINGEXT @@	Saves setting data under the file name specified in the variable @@ to external memory	@@: A\$, B\$, C\$, D\$
DATA:ADD WRITE	Writes an added data file	
DATA:OVER WRITE	Overwrites a data file	
DATA WRITE:CSV	Sets the data storage format to CSV	
DATA WRITE:DT7	Sets the data storage format to DT7	AQ6375
DATA WRITE:DT8	Sets the data storage format to DT8	AQ6370C
DATA WRITE:DT9	Sets the data storage format to DT9	AQ6373
WRITE DATA INT: #####.***'	Specifies a file name and saves data to internal memory	'#####.***': file name
WRITE DATA EXT: #####.***'	Specifies a file name and saves data to external memory	'#####.***': file name
WRITE DATA INT	Specifies a file name and saves data to internal memory. File names are assigned automatically.	

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
WRITE DATA EXT	Specifies a file name and saves data to external memory. File names are assigned automatically.	
WRITE DATA INT @@	Specifies a file name and saves data under the file name specified by the variable @@ in internal memory.	@@: A\$, B\$, C\$, D\$
WRITE DATA EXT @@	Specifies a file name and saves data under the file name specified by the variable @@ in external memory.	@@: A\$, B\$, C\$, D\$
DATA DATE&TIME ###	Selects ON/OFF of date and time output.	###: ON/OFF
DATA LABEL ###	Selects ON/OFF of label output.	###: ON/OFF
DATA DATA AREA ###	Selects ON/OFF of data area output.	###: ON/OFF
DATA CONDITION ###	Selects ON/OFF of measuring conditions output.	###: ON/OFF
DATA TRACE DATA ###	Selects ON/OFF of waveform data output.	###: ON/OFF
DATA OUTPUT WINDOW ###	Selects ON/OFF of contents output of the OUTPUT WINDOW PROGRAM function .	###: ON/OFF
READ TRACE # INT:'#####.\$\$\$'	Assigns a file name to specified TRACE data and reads it from internal memory	'#####.\$\$\$': file name #: A, B, C, D, E, F, G
READ TRACE # EXT:'#####.\$\$\$'	Assigns a file name to specified TRACE data and reads it from external memory	'#####.\$\$\$': file name #: A, B, C, D, E, F, G
READ TRACE # INT @@	Reads TRACE data in the file name specified by the variable @@ from internal memory	#: A, B, C, D, E, F, G @@: A\$, B\$, C\$, D\$
READ TRACE # EXT @@	Reads TRACE data in the file name specified by the variable @@ from external memory	#: A, B, C, D, E, F, G @@: A\$, B\$, C\$, D\$
READ MEMORY **INT:'#####.\$\$\$'	Specifies a file name and reads memory data from internal memory	'#####.\$\$\$': file name 0 to 63 (1 step)
READ MEMORY **EXT:'#####.\$\$\$'	Specifies a file name and reads memory data from external memory	'#####.\$\$\$': file name 0 to 63 (1 step)
READ MEMORY **INT @@	Reads memory data in the file name specified by the variable @@ from internal memory	**: 0 to 63 (1 step) @@: A\$, B\$, C\$, D\$
READ MEMORY **	Reads memory data in the file name specified by the variable @@ from external memory	**: 0 to 63 (1 step) @@: A\$, B\$, C\$, D\$
READ SETTING INT:'#####.\$\$\$'	Specifies a file name and reads setting data from internal memory	'#####.\$\$\$': file name
READ SETTING EXT:'#####.\$\$\$'	Specifies a file name and saves setting data from external memory	'#####.\$\$\$': file name
READ SETTING INT @@	Reads setting data of the file name specified by the variable @@ from internal memory	@@: A\$, B\$, C\$, D\$
READ SETTING EXT @@	Reads setting data of the file name specified by the variable @@ from external memory	@@: A\$, B\$, C\$, D\$

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
READ DATA INT: #####.\$\$\$'	Specifies a file name and reads datafrom internal memory	'#####.\$\$\$': file name
READ DATA EXT: #####.\$\$\$'	Specifies a file name and reads datafrom external memory	'#####.\$\$\$': file name
READ DATA INT @@	Reads data in the file namespecified @@: A\$, B\$, C\$, D\$ by thevariable @@ frominternal memory	
READ DATA EXT @@	Reads data in the file name specifiedby the variable @@ from externalmemory	@@: A\$, B\$, C\$, D\$
READ ALL TRACE INT: #####.CSV'	Specify a file name for all TRACE data and reads from internal memory.	'#####.CSV': File name
READ ALL TRACE EXT: #####.CSV'	Specify a file name for all TRACE data and reads from external memory.	'#####.CSV': File name
READ ALL TRACE INT @@	Reads all TRACE data under file names specified by the @@ variable from internal memory	@@: A\$, B\$, C\$, D\$
READ ALL TRACE EXT @@	Save all TRACE data under file names specified by the @@ variable from external memory	@@: A\$, B\$, C\$, D\$
READ TEMPLATE EXT: #####.\$\$\$'	Specifies a file name and reads a templatefrom external memory	'#####.\$\$\$': file name
READ TARGET LINE EXT:#####.\$\$\$'	Specifies a file name and reads target line data from external memory	'#####.\$\$\$': file name
DELETE INT: #####.\$\$\$'	Deletes files in internal memory	'#####.\$\$\$': file name
DELETE EXT: #####.\$\$\$'	Deletes files in external memory	'#####.\$\$\$': file name
DELETE INT @@	Deletes files specified by the variable @@: A\$, B\$, C\$, D\$ from internal memory	
DELETE EXT @@	Deletes files specified by the variable @@: A\$, B\$, C\$, D\$ from external memory	
RENAME INT:## @@	Changes the names of files in internal memory specified by the variable ## to the file name specified by the variable @@	##, @@: A\$, B\$, C\$, D\$
RENAME EXT:## @@	Changes the names of files in external memory specified by the variable ## to the file names specified by the variable @@	##, @@: A\$, B\$, C\$, D\$
REMOVE USB STORAGE	Brings USB storage media online	
WRITE LOGGING INT:#####.LG8	Specifies a file name and saves the logging data in internal memory	AQ6370C/AQ6370D #####.LG8: file name
WRITE LOGGING EXT:#####.LG8	Specifies a file name and saves the logging data in external memory	AQ6370C/AQ6370D #####.LG8: file name
WRITE LOGGING INT:#####.LG9	Specifies a file name and saves the logging data in internal memory	AQ6370B #####.LG9: file name
WRITE LOGGING EXT:#####.LG9	Specifies a file name and saves the logging data in external memory	AQ6370B #####.LG9: file name
WRITE LOGGING INT	Automatically assigns a file name and saves the logging data in internal memory	AQ6370C/AQ6370D/AQ6373B
WRITE LOGGING EXT	Automatically assigns a file name and saves the logging data in external memory	AQ6370C/AQ6370D/AQ6373B
WRITE LOGGING INT@@	Save logging data under file names specified by the @@ variable to internal memory	AQ6370C/AQ6370D/AQ6373B @@: A\$: B\$: C\$: D\$

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
WRITE LOGGING EXT@@@	Save logging data under file names specified by the @@ variable to external memor	AQ6370C/AQ6370D/AQ6373B @@@: A\$: B\$: C\$: D\$
LOGGING SAVE CSV###	Sets whether data logging results will be saved to a file in CSV format.	AQ6370C/AQ6370D/AQ6373B ###: ON/OFF
LOGGING SAVE TRACE###	Sets whether temporary saved waveform files will be saved when data logging results is saved.	AQ6370C/AQ6370D/AQ6373B ###: ON/OFF
READ LOGGING INT:#####.\$\$\$	Specifies a file name and reads data from internal memory	AQ6370C/AQ6370D/AQ6373B #####.\$\$\$: file name
READ LOGGING EXT:#####.\$\$\$	Specifies a file name and reads data from external memory	AQ6370C/AQ6370D/AQ6373B #####.\$\$\$: file name
READ LOGGING INT@@@	Reads data in the file name specified by the variable @@ from internal memory	AQ6370C/AQ6370D/AQ6373B @@@: A\$: B\$: C\$: D\$
READ LOGGING EXT@@@	Reads data in the file name specified by the variable @@ from external memory	AQ6370C/AQ6370D/AQ6373B @@@: A\$: B\$: C\$: D\$

### 8.3 Program Function Commands

#### ADVANCE

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
TEMPLATE GO/NO GO ##	Sets whether GO/NO-GO judgment is made	###: ON/OFF
TEMPLATE DISPLAY ###	Turns the template data display ON/OFF. ON: UPPER LINE=ON LOWER LINE=ON TARGET LINE=ON	###: ON/OFF
TEMPLATE DISPLAY UPPER ###	Sets ON/OFF of upper line display.	###: ON/OFF
TEMPLATE DISPLAY LOWER ###	Sets ON/OFF of lower line display.	###: ON/OFF
TEMPLATE DISPLAY TARGET ###	Sets ON/OFF of target line display.	###: ON/OFF
TMPLATE TEST TYPE UPPER	Sets if GO/NO-GO judgment at the upper line is made.	
TMPLATE TEST TYPE LOWER	Sets if GO/NO-GO judgment at the lower line is made.	
TMPLATE TEST TYPE UP & LOW	Sets if GO/NO-GO judgment at the upper and lower lines is made.	
TMPLATE WL SHIFT****.***nm	Sets the amount of wavelength shift of the template.	-999.999 to 999.999 (0.001 step)
TEMPLATE LEVEL SHIFT ***.**dB	Sets the amount of level shift of the template.	-99.99 to 99.99 (0.01 step)
DATA LOGGING START	Starts data logging	AQ6370C/AQ6370D/AQ6373B
DATA LOGGING ITEM#####	Sets the data logging source	AQ6370C/AQ6370D/AQ6373B #####: WDM, PEAK, MULTI-PEAK, DFBLD
DATA LOGGING MODE####	Sets the data logging mode (maximum channel mode or maximum logging mode)	AQ6370C/AQ6370D/AQ6373B # # #: MODE1(MAX 1024 ch, 2001 times), MODE2(MAX 256 ch, 10001 times)
DATA LOGGING INTERVAL #####	Sets the measurement interval of data logging	AQ6370C/AQ6370D/AQ6373B #####: SWEEP TIME, 1sec, 2sec, 5sec, 10sec, 30 sec, 1 min, 2 min, 5 min , 10min
DATA LOGGING TEST DURATION *****s	Sets the measurement duration of data logging (in seconds)	AQ6370C/AQ6370D/AQ6373B *****: 1 to 8639999(1 step)
DATA LOGGING PEAK TH TYPE###	Sets how the threshold for detecting the data logging mode (peak or bottom) is specified	AQ6370C/AQ6370D/AQ6373B ###: ABS, REL
DATA LOGGING PEAK TH (ABS)****.**dBm	Sets the threshold (absolute value) for detecting the data logging mode	AQ6370C/AQ6370D/AQ6373B ****: 20.00 to -100.00
DATA LOGGING PEAK TH (REL)**.**dB	Sets the threshold (relative value) for detecting the data logging mode	AQ6370C/AQ6370D/AQ6373B **.**: 0.01 to 99.99
DATA LOGGING CH MATCHING TH ± *.**nm	Sets the threshold of the channel-matching wavelength $\lambda$ for data logging	AQ6370C/AQ6370D/AQ6373B *.**: 0.01 to 1.00
DATA LOGGING MEMORY #####	Sets the temporary area for saving waveform files of data logging	AQ6370C/AQ6370D/AQ6373B ###: INTERNAL, EXTERNAL
DATA LOGGING TRACE LOGGING ###	Sets whether waveforms will be logged during data logging	AQ6370C/AQ6370D/AQ6373B ###: ON/OFF

**SYSTEM**

The following commands are not available on the AQ6373/AQ6373B

All commands that start with “SYSTEM GRID”

The following commands are not available on the AQ6375 if the wavenumber markers are set.

- All commands that start with “SYSTEM GRID”
- All commands that start with “CUSTOM GRID”
- All commands that start with “GRID REFERENCE”

<b>Program Command</b>	<b>Description</b>	<b>Instrument models on which the command is valid, parameter ranges, and supported variables.</b>
OPTICAL ALIGNMENT	Aligns the optical axis of a monochromator optical system.	
EXT OPTICAL ALIGNMENT	Aligns the optical axis of a monochromator optical system using the external light source.	
SELF WL CALIBRATION	Sets the light source to be wavelength calibrated for the internal light source.	AQ6370C/AQ6370D/AQ6375
EXT WL CALIBRATION *****.***nm	Sets the light source to be wavelength calibrated for the external light source (laser type)	AQ6370C/AQ6370D 600.000 to 1700.000 (0.001 step) AQ6373/AQ6373B 350.000 to 1200.000 (0.001 step) AQ6375 1200.000 to 2400.000 (0.001 step)
EXT-GAS WL CALIBRATION *****.***nm	Sets the light source to be wavelength calibrated for the external light source (gas cell type)	AQ6370C/AQ6370D 600.000 to 1700.000 (0.001 step) AQ6375 1200.000 to 2400.000 (0.001 step)
EMIS LINE WL CALIBRATION ****. *** nm	Sets the light source to be wavelength calibrated for the external light source (emission line light source type)	AQ6373B 350.000 to 1200.000 (0.001 step)
WL SHIFT **.***nm	Sets the amount of wavelength shift.	-5.000 to 5,000 (0.001 step)
LEVEL SHIFT ***.***dB SYSTEM GRID 200GHz	Sets the amount of level shift. Sets system grid to a 200 GHz spacing grid table.	-60.000 to 60,000 (0.001 step)
SYSTEM GRID 100GHz	Sets system grid to a 100 GHz spacing grid table.	
SYSTEM GRID 50GHz	Sets system grid to a 50 GHz spacing grid table.	
SYSTEM GRID 25GHz	Sets system grid to a 25 GHz spacing grid table.	
SYSTEM GRID 12.5GHz	Sets system grid to a 12.5 GHz spacing grid table.	
CUSTOM GRID STARTWL *****nm	Inputs the user grid table startwavelength.	1000.0000 to 1700.0000 (0.0001 step)
CUSTOM GRID STARTFREQ ***.***THz	Inputs the user grid table startfrequency.	176.3486 to 299.7924 (0.0001 step)
CUSTOM GRID STOP WL *****nm	Inputs the user grid table stopwavelength.	1000.0000 to 1700.0000 (0.0001 step)
CUSTOM GRID STOPFREQ ***.***THz	Inputs the user grid table stopfrequency.	176.3486 to 299.7924 (0.0001 step)
CUSTOM GRID SPACING ***.*GHz	Inputs the user grid table gridspacing.	0.1 to 999.9 (0.1 step)

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter ranges, and supported variables.
GRID REFERENCE WL ****.****nm	Inputs the reference wavelength of the grid table.	AQ6370C/AQ6370D 1000.0000 to 1700.0000 (0.0001 step) AQ6375 1200.0000 to 2400.0000 (0.0001 step)
GRID REFERENCE FREQ ***.*****THz	Inputs the reference frequency of the grid table.	AQ6370C/AQ6370D 176.3486 to 299.7924 (0.0001 step) AQ6375 125.0000 to 250.0000 (0.0001 step)
REMOTE INTERFACE: GP-IB	Sets the remote interface to GP-IB	
REMOTE INTERFACE: RS-232	Sets the remote interface to RS-232	
REMOTE INTERFACE: ETHERNET	Sets the remote interface to Ethernet	
TLS ADDRESS **	Sets the GP-IB address of the turnable laser source used by the synchronous sweep function	AQ6370C/AQ6375 0 to 30 (1 step)
SELECT COLOR *	Selects the display color of the screen.	1 to 5 (1 step)
UNCAL WARNING DISPLAY ###	Displays UNCAL and warning.	###: ON/OFF
BUZZER CLICK ###	Turns the key press click soundON/ OFF	###: ON/OFF
BUZZER WARNING ###	Turns the warning/error buzzerON/ OFF	###: ON/OFF
LEVEL DISPLAY DIGIT *	Sets the number of displayed digits (decimal place) of the level data displayed under the marker area and ANALYSIS results.	1 to 3 (1 step)
WINDOW TRANSPARENT ###	Selects ON/OFF of the transparent display function for the split display and OVERVIEW window	###: ON/OFF
AUTO OFFSET ###	Turns auto offset ON/OFF.	###: ON/OFF
AUTO OFFSET INTERVAL *** min	Sets the time interval for executing the auto offset function	AQ6370C/AQ6370D/AQ6373/ AQ6373B ***: integer
TRIGGER INPUT SAMPLING TRIGGER	Sets the trigger input mode to sampling trigger	
TRIGGER INPUT SWEEP TRIGGER	Sets the trigger input mode to sweeptrigger	
TRIGGER INPUT SAMPLING ENABLE	Sets the trigger input mode to sampling enable	AQ6370C/AQ6370D/AQ6373B
TRIGGER OUTPUT SWEEP STATUS	Sets the trigger output mode to sweep status	
TRIGGER OUTPUT OFF	Turns OFF the trigger output mode	
REMOVE USB STORAGE	Brings USB storage media online	

## Lists of Special Commands

### General Commands

Program Command	Description	Parameter Rng, Avail Variables
COPY ON	Produces a hard copy of the screen on a printer.	AQ6370C/AQ6373/AQ6375
	Produces a hard copy of the screen to file.	AQ6370D/AQ6373B
PRINTER FEED **	Feeds printer paper.	AQ6370C/AQ6373/AQ6375 1 to 10 (1 step)
GOTO ***	Makes a jump to line ***.	1 to 200 (1 step)
GOTO PROGRAM **	Makes a jump to program ** to run it from the first line. After completing running of program **, control returns to the original program. However, if there is an END command in program **, return to the jump source is not performed and the program ends. When a program is executed using this command, variables are not initialized.	
WAIT *****S	Makes a wait of **** seconds.	1 to 99999 (1 step)
PAUSE '---56 chars--'	Pauses execution of a program and causes a message window to appear. This window displays a message and an explanation of the CONTINUE key. Pressing the CONTINUE soft key closes the window and executes the program. If a program is started via GP-IB, no pause is made.	
VARIABLE CLEAR	Initializes all variables used in a program.	
END	Ends a program.	
INIT	Initializes all parameters, but does not clear variables.	
@=VAL(@\$)	Converts the string in variable @ to a numerical value and substitutes the value into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z @\$: A\$, B\$, C\$, D\$
BEEP **	Buzzer sounds for ** x 100 msec.	1 to 10 (1 step)

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

### Loop Control

Program Command	Description	Parameter Rng, Avail Variables
N=*****	Substitutes a value into variable N.	1 to 99999999 (1 step)
N=@@@@#@	Copies the contents of variable @@@@# to variable N.	@@@#@: MODN, WDMCHN, NFCHN, GONO, M
N-N-1;IF N<>0GOTO ***	Subtracts "1" from variable N and, if the result is not "0," makes a jump to line ***.	1 to 200 (1 step)
M=*****	Substitutes a value into variable M.	1 to 99999999 (1 step)
M=@@@@#@	Copies the contents of variable @@@@# to variable M.	@@@#@: MODN, WDMCHN, NFCHN, GONO, N
M-M-1;IF M<>0 GOTO ***	Subtracts "1" from variable N and, if the result is not "0," makes a jump to line ***.	1 to 200 (1 step)

## 8.3 Program Function Commands

---

### Variable Calculations

Program Command	Description	Parameter Rng, Avail Variables
<code>@ = ***** ###</code>	Substitutes a value into variable @. For @: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, ******, a real number of 10 or fewer T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, CH digits can be specified, including a sign and the decimal point.	*****: -999999999 to 999999999 (1 step) ###: nm, dB, dBm, pW, nW, mW, mW, W, THz, cm <sup>-1</sup> (AQ6375), '(without units)
<code>@ = # + *****</code>	Adds value ***** to variable # and substitutes the value into variable @. ***** can be specified with a real number of 10 or fewer digits, including a sign and the decimal point. By specifying a negative value, you can cause subtraction to be made from variable #.	@, #: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, CH *****: -999999999 to 999999999 (1 step)
<code>@ = @@@@ @</code>	Copies the contents of variable @@@@ @ to variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, CH @@@ @: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), NFCHN, NFNL(CH), NFLVLI(CH), NFLVLO(CH), NFASELV(CH), NFGAIN(CH), NFNF(CH), MKPWR, PMD, M, N, CH, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3
<code>@ = @@@@ @ + #####</code>	Performs addition, subtraction, multiplication, and/or division between variables.	#####: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, CH @@@ @: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), NFCHN, NFNL(CH), NFLVLI(CH), NFLVLO(CH), NFASELV(CH), NFGAIN(CH), NFNF(CH), MKPWR, PMD, M, N, CH, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3
<code>@ = @@@@ @ - #####</code>		
<code>@ = @@@@ @ * #####</code>		
<code>@ = @@@@ @ / #####</code>		
<code>@\$ = @\$</code>	Copies string variable @\$ to stringvariable @.	@\$: A\$, B\$, C\$, D\$
<code>@\$ = MID(@\$, @, @)</code>	Substitutes @'s worth of characters in the string that is distant from the start of character variable @\$ by the number of characters in the numerical variable @ into character variable @\$.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z @\$: A\$, B\$, C\$, D\$
<code>@\$ = '--56 chars--'</code>	Substitutes string to character variable @\$: A\$, B\$, C\$, D\$ @\$.. (56 chars max)	

### 8.3 Program Function Commands

Program Command	Description	Parameter Rng, Avail Variables
<code>@\$ =@\$+@\$</code>	Substitutes the character string obtained by concatenating character variable @\$ and character variable @\$ into character variable @\$.	AQ6370D @\$: A\$: B\$: C\$: D\$
<code>@\$ =STR(@)</code>	Converts variable @ into a character string and substitutes it into character variable @\$	AQ6370D @: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z @\$: A\$: B\$: C\$: D\$
<code>@\$ =DATEINFO(###)</code>	Substitutes the date and time into character variable @\$.	AQ6370D @\$: A\$: B\$: C\$: D\$ ####: DATE&TIME, DATE, TIME

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D.

#### Print Output (on the AQ6370C, AQ6373 or AQ6375

Program Command	Description	Parameter Rng, Avail Variables
<code>PRINT ---56 chars ---'</code>	Prints out a character string in '''. If a semicolon ( ; ) is added to the end of the string, after printing, no line feed is made, but a character string or the variable values specified by the next PRINT command are printed out successively.	
<code>PRINT @@@@@</code>	Adds units to the value of variable @@@@@ and prints the result.	@@@@@: G, H, I, J, K, P, Q, R, S, X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), NFCHN, NFWL(CH), NFLVLI(CH), NFLVLO(CH), NFASELV(CH), NFGAIN(CH), NFNF(CH), MKPWR, PMD, M, N, CH, A\$, B\$, C\$, D\$, FILE\$, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3
<code>PRINT @@@@@:;</code>	Adds units to the value of variable @@@@@ and prints the result. After printing, no line feed is made but a character string or the variable values specified by the command are continuously printed	@@@@@: G, H, I, J, K, P, Q, R, S, X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), NFCHN, NFWL(CH), NFLVLI(CH), NFLVLO(CH), NFASELV(CH), NFGAIN(CH), NFNF(CH), MKPWR, PMD, M, N, CH, A\$, B\$, C\$, D\$, FILE\$, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3
<code>PRINT DATA AREA</code>	Prints out the contents of the data area.	
<code>PRINT OUTPUT WINDOW</code>	Prints out the contents of OUTPUT WINDOW	

## 8.3 Program Function Commands

---

### Condition Judgement

Program Command	Description	Parameter Rng, Avail Variables
IF F1 <= @@@@ @@@@ <= F2 GOTO ***	Value of variable @@@@ @@@@ is F1 or greaterIf less than F2, jumps to line ***	@@@@ @@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), FNCHN, NFWL(CH), NFLVL(CH), NFLVI(CH), NFLVO(CH), NFSELV(CH), NFGAIN(CH), NFNFC(H), MKPWR, PMD, M, N, CH, A\$, B\$, C\$, D\$, FILE\$, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3 ***: 1 to 200 (1 step)
F1 = ***** ####	Substitutes a value into variable F1. For ***** , a real number of 10 or fewer digits can be specified including a sign and the decimal point.	####: nm, dB, dBm, pW, nW, mW, mW, W, THz, cm <sup>-1</sup> (AQ6375), '(without units) *****: -999999999 to 999999999 (1 step)
F2 = *****	Substitutes a value into #### variable F2. For ***** , a real number of 10 or fewer digits can be specified, including a sign and the decimal point.	####: nm, dB, dBm, pW, nW, mW, mW, W, THz, cm <sup>-1</sup> (AQ6375), '(without units) *****: -999999999 to 999999999 (1 step)
F1 = @@@@ @@@@	Copies the contents of variable @@@@ @@@@ to the variable F1.	@@@@ @@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), FNCHN, NFWL(CH), NFLVL(CH), NFLVLO(CH), NFSELV(CH), NFGAIN(CH), NFNFC(H), MKPWR, PMD, M, N, CH, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3
F2 = @@@@ @@@@	Copies the contents of variable @@@@ @@@@ to the variable F2.	@@@@ @@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), WDMSNR(CH), FNCHN, NFWL(CH), NFLVL(CH), NFLVLO(CH), NFSELV(CH), NFGAIN(CH), NFNFC(H), MKPWR, PMD, M, N, CH, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3
@ = LEVEL (****.***nm)	Substitutes the level of the point of wavelength ****.*** nm on an active trace into variable @.	@: G, H, I, J, K, P, Q, R, S, X, Y, Z ****.***: 600.000 to 1700.000 (0.001 step)

### 8.3 Program Function Commands

Program Command	Description	Parameter Rng, Avail Variables
@ = LEVEL (@@@@@)	Substitutes the level of the point of the wavelength @@@@@ (variable) on the active trace into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z @@@@@: G, H, I, J, K, P, Q, R, S, X, Y, Z, WM, W1, W2, W(CH), MEANWL, PKWL, WDMLVL(CH), WDMWL(CH), NFWL(CH)
IF @@@@@ < @@@@@ GOTO ***	Compares the large and small relationship of two variables and if the conditions are met, makes a jump to line ***.	@@@@@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z, WM, W1, W2, W2-W1, W(CH), LM, L1, L2, L2-L1, L(CH), SPWD, MEANWL, PKWL, PKLVL, MODN, GONO, SMSR, SMSR2, WDMCHN, WDMWL(CH), WDMLVL(CH), \
IF @@@@@ =< @@@@@ GOTO ***		WDMSNR(CH), FNCHN, NFWL(CH), -NFLVLI(CH), NFLVLO(CH), NFASELV(CH), NFGAIN(CH), NFNF(CH),
IF @@@@@ = @@@@@ GOTO ***		MKPWR, PMD, M, N, CH, WAM1, WAM2, WAM3, WAM4, WAM2-WAM1, WAM4-WAM3, LAM1, LAM2, LAM3, LAM4, LAM2-LAM1, LAM4-LAM3 ***: 1 to 200 (1 step),

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D

### External Control

Program Command	Description	Instrument models on which the command is valid, parameter Rng, Avail Variables
SEND **' ---56 chars---	Sets the external instrument at address ** that is connected to the GP-IB2 connector as the listener, and sends the command in the single quotes (''). The delimiter is CR/LF.	AQ6370C/AQ6373/AQ6375 0 to 30 (1 step)
SEND **' ---56 chars---';@	Sets the external instrument at address ** that is connected to the GP-IB2 connector as the listener, and following the command in the single quotes (''), sends the value of variable @. The delimiter is CR/LF.	AQ6370C/AQ6373/AQ6375 0 to 30 (1 step) @: G, H, I, J, K, P, Q, R, S, X, Y, Z
SEND **' ---20 chars---'; @;---20 chars ---'	Sets the external instrument at address ** that is connected to the GP-IB2 connector as the listener, and following the command in the single quotes (''), sends the value of variable @, and the command in the single quotes (''). The delimiter is CR/LF.	AQ6370C/AQ6373/AQ6375 0 to 30 (1 step) @: G, H, I, J, K, P, Q, R, S, X, Y, Z
SEND RS232 '---56 chars---	Sets the external instrument that is connected to the RS-232 connector as the listener, and sends the command in single quotes (''). The delimiter is the set value of SET DELIMITER.	
SEND RS232 '---56 chars---';@	Sets the external instrument that is disconnected to the RS-232 connector as the listener, and following the command in single quotes (''), sends the value of variable @. The delimiter is the setting value of SET DELIMITER.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter Rng, Avail Variables
SEND RS232 '---20 chars---'; @:'---20 chars ---'	Sets the external instrument that is disconnected to the RS-232 connector as the listener, and following the cmd. in single quotes (' '), sends the value of variable @, and also sends the cmd in single quotes. The delimiter is the setting value of SET DELIMITER.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
SEND LAN @\$, ***** ; ---56 chars--- *@\$: computer name or IP address ****: Port number	Specifies the external instrument that is connected to the LAN connector and that is specified by the computer name, IP address, and port number as the listener, and sends the command and sends the command in single quotes (' '). Delimiter is value of SET DELIMITER	Port Numeber: 1024 to 65535 @ \$: A\$, B\$, C\$, D\$
SEND LAN @\$, ***** ; '---56 chars---' ;@ *@\$: computer name or IP address ****: Port number	Specifies the external instrument that is connected to the LAN connector and that is specified by the computer name, IP address, and port number as the listener, and sends the command and following the commnd in single quotes (' '), sends the value of the variable @. Delimiter is value of SET DELIMITER.	Port Number: 1024 to 65535 @: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z @ \$: A\$, B\$, C\$, D\$
SEND LAN @\$ , ***** , '--20 chars?';@ "?20 chars?*@\$: computer name or IP address ****: Port Number	Specifies the external instrument that is disconnected to the LAN connector and that is specified by the computer name, IP address, and port number as the listener, and following the commnd in single quotes (' '), sends the value of variable @, as well as the command in single quotes. The delimiter is the setting value of SET DELIMITER.	Port Number: 1024 to 65535 @: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R,S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z @ \$: A\$, B\$, C\$, D\$
RECEIVE **;@\$	Sets the external instrument at address ** that is connected to the GP-IB2 connector as the talker, receives the specified message, and substitutes it into the character variable @\$. Up to 512 characters can be received. The delimiter is CR/LF.	AQ6370C/AQ6373/AQ6375 0 to 30 (1 step) @\$: A\$, B\$, C\$, D\$
SENDR RS-232 '---56 chars---' ; @\$	Sends a query command to the external instrument connected to the RS-232 connector, and substitutes the message received from the external instrument into character variable @\$. Up to 512 characters can be received. Delimiter is value of SET DELIMITER	@ \$: A\$, B\$, C\$, D\$
SENDR LAN @\$ , ***** , '---56 chars---' ; @\$ *@\$: computer name or IP address ****: Port number	Sends a query command to the external instrument that is connected to the LAN connector and which is specified by the computer name, IP address, and port number stored in variable @\$. Substitutes the message received from the external instrument into character variable @\$. Up to 512 characters can be received. The delimiter is the setting value of SET DELIMITER.	Port Number: 1024 to 65535 @ \$: A\$, B\$, C\$, D\$
RESET OPTION	On the external instrument connectedto the GP-IB2 connector performs a remote clear, device clear, andinterface clear.	AQ6370C/AQ6373/AQ6375

### 8.3 Program Function Commands

Program Command	Description	Instrument models on which the command is valid, parameter Rng, Avail Variables
SPOLL **;S	Sets the external instrument at address **. Performs a serial poll on the external instrument at address **, and substitutes standby into variable S.	AQ6370C/AQ6373/AQ6375 0 to 30 (1 step)
SET DELIMITER ###	On the external instrument being remotely controlled with the RS-232 or LAN port, sets the delimiter that is sent/received by the instrument.	###:CR, LF, CR+LF

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D

### Substitution of Measuring Conditions

Program Command	Description	Parameter Rng, Avail Variables
@ = CENTER	Substitutes the current measurement center wavelength into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
@ = SPAN	Substitutes the current sweep width into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
@ = REF LEVEL	Substitutes the current reference level into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
@ = RESOLUTION	Substitutes the current measurement resolution into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
@ = SAMPLING POINT	Substitutes the current number of samples into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
@ = ZOOM CENTER	Substitutes the current display center wavelength into variable @.	@: E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z
@ = ZOOM SPAN	Substitutes the current display width into variable @.	E <sup>1</sup> , G, H, I, J, K, O <sup>1</sup> , P, Q, R, S, T <sup>1</sup> , U <sup>1</sup> , V <sup>1</sup> , X, Y, Z

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D

## 8.3 Program Function Commands

---

### User I/O

Program Command Description	Parameter Rng, Avail Variables
DATA INPUT '---56 chars---';@	Pauses program execution, and gets the value/string input into variable @by the user. The Input Window appears on screen displaying a character string in ''. When variable @ is numerical it accepts numerical input and when it is a string variable it accepts string input.
DATA OUTPUT	The string in single quotes (') is output to the OUTPUT WINDOW. If a semicolon is added to the end of the string, no line feed is made after output of the string, but a character string or the variable values specified by the next DATA OUTPUT command are output successively.
DATA OUTPUT @##@	The value of variable @##@ is output to the OUTPUT WINDOW with units added.
DATA OUTPUT @##@@:	Outputs the value of variable @##@ to the OUTPUT WINDOW with units added. After a string is output, no line feed is sent, but the value of the string or variable of the next DATA OUTPUT command is output.
DATA OUTPUT DATA AREA	Outputs the contents of the data area to the OUTPUT WINDOW.
OUTPUT WINDOWCLEAR	Clears the contents of the OUTPUTWINDOW.
OUTPUT WINDOW ###	Sets whether to display or hide the OUTPUT WINDOW on the screen. ####: ON or OFF

1: Generalized variables E, O, T, U, and V are valid only for the AQ6370D

## 8.4 Controlling an External Instrument with the Program Function

Using the program function, the instrument can remote control the external devices which are connected by various interfaces. In addition, it is possible to remote control the multiple external devices by one program source.

### Remote Control of External Instruments Using the GP-IB2 Port

You can perform sending of remote commands, receiving of talker data, and serial polling on the instrument connected to the GP-IB2 port. The GP-IB address of the connected instrument is specified with program commands, and communication is carried out.

Do not set the same GP-IB address as that of the setting value of the **GP-IB2 PORT ADDRESS** key. If the same address is used, the instrument cannot communicate normally with the external device.

#### Send Commands

```
SEND ** 'control command/query command (56 chars)'
SEND ** 'control command/query command (56 chars)' ;@
SEND ** 'control command/query command (20 chars)' :@:' control command/query
command (20 chars)
**: GP-IB command
```


#### Receive Commands

```
RECEIVE **;@$
```

\*\*: GP-IB command

#### Note

- A controller such as a PC that is connected to the GP-IB2 port cannot remotely control the AQ6370C.
- Even if an external device to be controlled by the AQ6370C using program functions or a wavelength turnable laser source is connected to the GP-IB1 port, it cannot remote control the AQ6370C.
- The GP-IB1 and GP-IB2 ports are independent of each other. Thus, a controller connected to the GP-IB1 port cannot directly send a message to an external device connected to the GP-IB2 port.
- With a controller connected to the GP-IB1 port, connecting the GP-IB1 port and the GP-IB2 port results in improper operations. Do not connect a cable between these ports, or turn the SYSTEM CONTROLLER OFF. The default is ON.
- Using a command such as SEND\*\*'control command/query command (56 chars)';@, if you insert <wsp> between the command string and the variable @, add "—" to the end of the command.



- The GP-IB2 port is not available on the AQ6370D / AQ6373B.

### Remote Control Using the RS-232 Port

Using the program function, the unit can send remote commands, receive talker data, and perform serial polling on the external device which is connected to the RS-232 port. Connect a cross cable to the RS-232 interface at the back side of the instrument. See chapter 4 for the various serial communication settings. If you want to receive query data from the external device, use the send/receive command. Query data is stored in the specified string variable @\$.

#### Send Commands

```
SEND RS-232 'control command (56 chars)'  
SEND RS-232 'control command (56 chars)' ;@  
SEND RS-232 'control command (20 chars)' :@:' control command (20 chars)'
```

#### Send/Receive Command

```
SENDRCV RS-232 'query command (56 chars)';@$
```

#### Note

---

- Depending on the external device connected, there are times when it is necessary to change the delimiter setting of the send command. If the setting for the delimiter must be changed, use the SET SEND DELIMITER special command and make the setting match that of the instrument on the receiving end. (Default: CR+LF)
  - Using a command such as SEND RS232 'control command (56 characters)';@, if you insert <wsp> between the command string and the variable @, add "—" to the end of the command.
- 

### Remote Control of an External Instrument Using the LAN Port

Using the program function, specify the “Computer Name” or “IP address” and “Port Number” of the external device connected to the LAN connector to perform remote control. “Computer Name” or “IP address” must be entered it in the character variable @\$ of the program command. If you want to receive query data from the external device, use the send/receive command. Query data is stored in the specified string variable @\$.

#### Send Commands

```
SEND LAN @$ **** 'control command (56 chars)'  
SEND LAN @$ **** 'control command (56 chars)' ;@  
SEND LAN @$ **** 'control command (20 chars)' :@:' control command (20 chars)  
@$: Computer name or IP address  
****: Port Number'
```

#### Send/Receive Command

```
SENDRCV LAN @$ **** 'query command (56 characters)'  
@$: computer name or IP address  
****: Port number
```

#### Note

---

- Be sure to set the instrument's IP address correctly.
  - When using DHCP, the instrument's IP address is automatically set. Set ADDRESS SETTING under TCP/IP SETTING to AUTO (DHCP).
  - Please ask your network administrator for details about network connections.
  - Using a command such as SEND LAN 'control command (56 characters)';@, if you insert <wsp> between the command string and the variable @, add "—" to the end of the command.
-

## 8.5 Sample Program

Here, an example is given of performing the operation below.

### Conditions

After the measuring conditions have been set, the program performs a single sweep.

Then it searches for a spectrum width and peak wavelength, and outputs the results to the label area and OUTPUT WINDOW. It repeats these operations ten times with a wait of three seconds between repetitions.

```

001 CENTER WL 1555.00nm           :Set measurement conditions
002 SPAN 10.0nm
003 REFERENCE LEVEL -10.0dBm
004 RESOLUTION 0.1nm
005 AVERAGE TIMES 1
006 SENS NORMAL/HOLD
007 OUTPUT WINDOW CLEAR

008 OUTPUT WINDOW ON             :Clear the OUTPUT WINDOW
                                 data.

009 N=10 :Set loop counter N to 10
010 SINGLE                         :Display the OUTPUT
                                 WINDOW.

011 SPEC WD THRESH 20.0dB         :Set loop, counter N to 10
                                 Perform a single sweep.

012 DATA OUTPUT 'Wd = ;          :Perform a spectrum width
                                 search
                                 :Output spectrum width
                                 to OUTPUT WINDOW and the
                                 label area.

013 LABEL 'Wd = ;                :Perform a peak search
014 DATA OUTPUT SPWD;
015 LABEL SPWD ;
016 PEAK SEARCH
017 DATA OUTPUT 'Pk = ;          :Output the peak wavelength
                                 value to OUTPUT WINDOW and
                                 the label area.

018 LABEL 'Pk = ;                :Wait three second.
019 DATA OUTPUT PKWL
020 LABEL PKWL
021 WAIT 3S                      :Subtract 1 from loop
                                 counter N and if the
                                 result is not 0, make a
                                 jump to line 010.

022 N=N-1 ; IF N <> 0 GOTO 10   :Exit the Program.

023 END

```

## 8.5 Sample Program

---

The following program specifies an external device connected to the [GP-IB2] connector as a listener to send a device message and then specifies the device as a talker to receive data from it.

Received data is displayed on the OUTPUT WINDOW. The program repeats these operations 10 times.


```
001  OUTPUT WINDOW CLEAR          :Clear the OUTPUT WINDOW  
                               data.  
002  OUTPUT WINDOW ON           :Display the OUTPUT  
                               WINDOW.  
003  N=10 :Set loop counter N to 10    :Set "10" to loop counter  
                                         "N."  
004  SEND 1'B,C1,E1,H1,S      :Specify the external  
                               device of address 1 as  
                               a listener to send the  
                               contents of ' ' to it.  
005  WAIT 1S:1                 :Cause a wait of 1 sec.  
006  RECEIVE 1;A$              :Specify the device of  
                               address 1 as a talker to  
                               receive data from it and  
                               substitute received data  
                               into character variable  
                               A$.  
007  DATA OUTPUT @0000@        :Output the contents of A$  
                               to OUTPUT WINDOW.  
008  N=N-1;IF N<>0 GOTO 4     :Substart 1 from loop  
                               counter N and if the  
                               result is not 0, make a  
                               jump to line 004.  
009  END                      :End the program.
```

# Switching Command Modes

To use AQ6317-compatible commands, you must place the instrument in AQ6317 command mode.

## Procedure

1. Press **SYSTEM**. The system setting menu is displayed.
2. Press the **MORE1/4** soft key. The communication interface setting menu is displayed.
3. Press the **REMOTE INTERFACE** soft key. The setting menu for the interface to be used is displayed.
4. Press the **GP-IB** soft key to specify GP-IB as the communication interface.
5. Press the **COMMAND FORMAT** soft key. The command format setting menu is displayed.
6. Press the **AQ6317** soft key.

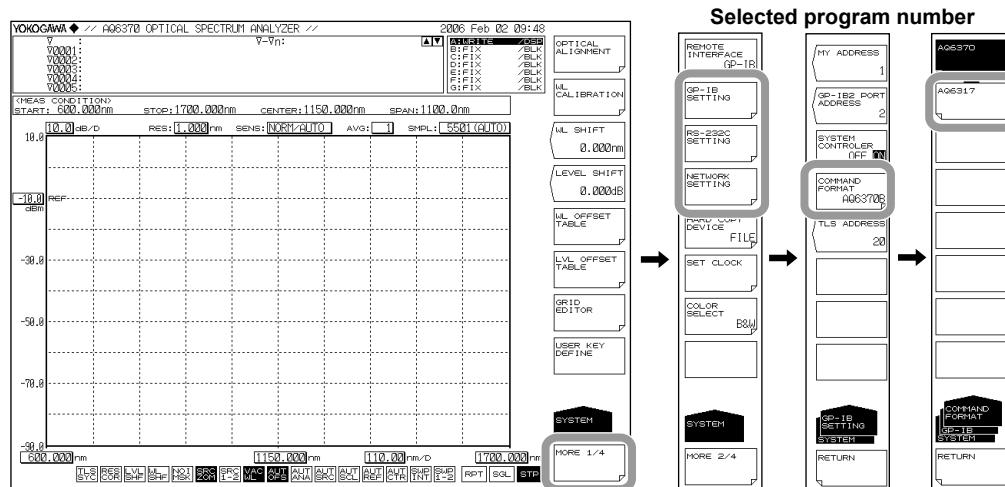

App

**Explanation**

Because remote control via the GP-IB interface of the /AQ6375 complies with the IEEE 488.2 standard, it is not compatible with the conventional model AQ6317 (complying with the IEEE 488.1 standard) as to the remote commands and internal actions.

However, by placing the instrument in AQ6317-compatible command mode, you can use some of the AQ6317 commands. Status register operation also has compatibility with the AQ6317. When you switch the command mode, it causes all the contents of the status registers and queues and receive buffer and talker output buffer to be initialized.

**Operation in AQ6317-Compatible Mode**

The instrument operates as follows when it is remote controlled in the AQ6317-compatible mode.

- The majority of AQ6317 control commands and talker commands are available.
- Talker data is output in the AQ6317-compatible format.
- To send multiple commands at one time, use a comma “,” as a separator.
- If receiving multiple query commands in a single line, the instrument outputs only data relative to the last query command.

**Switching Command Modes with Commands**

The command mode can also be switched using the following GP-IB commands.

Commands to use when in AQ6370C, AQ6373, AQ6373B or AQ6375 mode (invalid in the AQ6317-compatible mode)

```
:SYSTem:COMMunicate:CFORmat<wsp><mode>
<mode> = AQ6317|AQ6370|AQ6370C|AQ6375|AQ6373|AQ6373B|0|1
    AQ6317 = Switch to AQ6317-compatible mode
    AQ6370 = Switch to AQ6370C/AQ6375/AQ6373/AQ6373B mode
    AQ6370C = Switch to AQ6370C mode (for AQ6370C)
    AQ6375 = Switch to AQ6375 mode (for AQ6375)
    AQ6373 = Switch to AQ6373 mode (for AQ6373)
    AQ6373B = Switch to AQ6373B mode (for AQ6373B)
```

```
:SYSTem:COMMunicate:CFORmat?
```

```
0 = AQ6317
1 = AQ6370C, AQ6373, AQ6373B or AQ6375
```

Commands to use when in AQ6317-compatible mode (result in errors when in AQ6370C/AQ6370D/AQ6373/AQ6373B/AQ6375 mode)

    Control commands

```
CFORM*
```

```
*: 0 = AQ6317-compatible mode, 1 = AQ6370C, AQ6373, AQ6373B or AQ6375 mode
CFORM?
```

```
0 = AQ6317-compatible mode, 1 = AQ6370C, AQ6373, AQ6373B or AQ6375 mode
```

## AQ6317 Status Byte

The status byte of AQ6317-compatible mode operates like the status byte in the AQ6317. Refer to the manuals for the AQ6317 series for the details of GP-IB.

Bit	Function and Setting Condition	Clear Timing
Bit 7	0	
Bit 6	Send an SRQ signal.	<ul style="list-style-type: none"><li>Upon execution of serial polling</li><li>Upon receipt of DCL or SDC</li></ul>
Bit 5	When receiving data exceeding the receive buffer capacity of 512 byte “1” is set.	<ul style="list-style-type: none"><li>Upon execution of serial polling</li><li>Upon receipt of DCL or SDC</li><li>At a start of measurement</li></ul>
Bit 4	0	
Bit 3	When a command data error occurs, set “1”.	<ul style="list-style-type: none"><li>Upon receipt of DCL or SDC</li><li>Upon execution of serial polling</li><li>At a start of measurement</li></ul>
Bit 2	Warning error (including errors upon execution of a Program) occurs, set “1”. For the contents of the warning its number can be output	<ul style="list-style-type: none"><li>When the warning error display disappears</li><li>Upon execution of serial polling</li><li>Upon receipt of DCL or SDC</li><li>At a start of measurement</li></ul>
Bit 1	When the execution of a copy or program terminates, set “1”.	<ul style="list-style-type: none"><li>Upon execution of serial polling</li><li>Upon receipt of DCL or SDC</li><li>At a start of measurement</li></ul>
Bit 0	After sweep finishes, “1” is set.	<ul style="list-style-type: none"><li>Upon execution of serial polling</li><li>Upon receipt of DCL or SDC</li><li>At a start of measurement</li></ul>

# List of the AQ6317-Compatible Commands

For compatibility with the AQ6370C/AQ6373/AQ6373B/AQ6375, see the following table, AQ6317-Compatible Commands.

AQ6317 Series Control Command	Operates in AQ6317- Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
3D	x	-	
3DRCL	x	-	
A+BCL	o	:CALCulate:MATH:TRC<wsp>A+B (LIN)	
A=B	o	:TRACe:COPY<wsp>TRB, TRA	
A=C	o	:TRACe:COPY<wsp>TRC, TRA	
A-BC	o	:CALCulate:MATH:TRC<wsp>A-B (LOG)	
A-BCL	o	:CALCulate:MATH:TRC<wsp>A-B (LIN)	
ACTV*	o	:TRACe:ACTive<wsp><trace name> <trace name>=TRA TRB TRC	
ANA?	o	:CALCulate:DATA?	Diff. talker format
ANGL***	x	-	
AREA*	x	-	
ARES?	x	-	
ARESDSP*	x	-	
ATANA*	o	:CALCulate[:IMMEDIATE]:AUTO<wsp> OFF ON 0 1	
ATCTR*	o	:CALCulate:MARKer:MAXimum: SCENter:AUTO<wsp> OFF ON 0 1	
ATOFS*	o	:CALibration:ZERO[:AUTO]<wsp> OFF ON 0 1	
ATREF*	o	:CALCulate:MARKer:MAXimum: SRLevel:AUTO	
ATSCL*	o	:DISPlay[:WINDOW]:TRACE: Y2[:SCALE]:AUTO<wsp>OFF ON 0 1	
ATSR*	o	:CALCulate:MARKer:AUTO<wsp> OFF ON 0 1	
AUTO	o	:INITiate:SMODe<wsp>AUTO 3; INITiate	
AVG****	▲	:SENSe:AVERage:COUNT<wsp> <integer>	Diff. parameter range
B=A	o	:TRACe:COPY<wsp>TRA, TRB	
B=C	o	:TRACe:COPY<wsp>TRC, TRB	
B-AC	o	:CALCulate:MATH:TRC<wsp> B-A(LOG)	
B-ACL	o	:CALCulate:MATH:TRC<wsp>B-A (LIN)	
BASL***.*	o	:DISPlay[:WINDOW]:TRACE:Y1[:SCALE]: SPACING<wsp>LINEar 1; :DISPlay[:WINDOW]:TRACE:Y1[:SCALE]: BLEVel<wsp><NRf>[MW]	
BD*	o	-	
BLKA	o	:TRACe:STATE:TRA<wsp>OFF 0	
BLKB	o	:TRACe:STATE:TRB<wsp>OFF 0	
BLKC	o	:TRACe:STATE:TRC<wsp>OFF 0	
BTSR	o	:CALCulate:MARKer:MINimum	

List of the AQ6317-Compatible Commands

AQ6317 Series Control Command	Operates in AQ6317-Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
BZCLK*	○	:SYSTem:BUZZer:CLICK<wsp>OFF  ON 0 1	
BZWRN*	○	:SYSTem:BUZZer:WARNing<wsp> OFF ON 0 1	
C=A	○	:TRACe:COPY<wsp>TRA, TRC	
C=B	○	:TRACe:COPY<wsp>TRC, TRB	
CLMES	○	-	
CLR	○	:TRACe:DELetE<wsp>TRA; :TRACe:DELetE<wsp>TRB; :TRACe:DELetE<wsp>TRC	
CNDDT*	○	:MMEMory:STORe:DATA:ITEM<wsp> CONDITION, OFF ON 0 1	
COPY*	○	:HCOPY[:IMMediate]	
CRS*	○	-	
CTR=M	○	:CALCulate:MARKer:SCENter	
CTR=P	○	:CALCulate:MARKer:MAXimum:SCENter	
CTR***.***	▲	:SENSe:WAVelength:CENTER<wsp> <NRf>[HZ]	Diff. parameter range
CTRWL****.*.*	▲	:SENSe:WAVelength:CENTER<wsp> <NRf>[M]	Diff. parameter range
CVFTC**	×	-	Same cmd for TRACE G
CVPKC**	×	-	Same cmd for TRACE G
CWPLS?	▲	-	Diff. query data 0: Except CW 1: CW
D&TDT*	○	:MMEMory:STORe:DATA:ITEM<wsp> DATE, OFF ON 0 1	
DATE?	○	:SYSTem:DATE?	Diff. talker format
DATE YR.MO.DY	○	:SYSTem:DATE<wsp><year>,<month>,<day>	
TIME HH:MM	○	:SYSTem:TIME<wsp><hour>,<minute>, <second>	
DEFCL*	▲	:DISPlay:COLor<wsp><mode> <mode>=0: B&W, 1-5: mode 1 - mode 5	Diff. display color
DEL'@@@@.***'	○	:MMEMory:DELetE<wsp><"file name">, EXTernal	
DFBAN	○	:CALCulate:CATegory<wsp>DFBLd 4	
DFBLDo;□;▲;****	▲	-	
DIR?	×	-	
DISP?	○	-	
DSPA	○	:TRACe:STATE:TRA<wsp>ON 1	
DSPB	○	:TRACe:STATE:TRB<wsp>ON 1	
DSPA?	○	:TRACe:STATE:TRA?	
DSPB?	○	:TRACe:STATE:TRB?	
DSPC	○	:TRACe:STATE:TRC<wsp>ON 1	
DSPC?	○	:TRACe:STATE:TRC?	
DTAD*	○	:MMEMory:STORe:DATA:MODE<wsp> ADD OVER 0 1	
DTARA*	○	:MMEMory:STORe:DATA:ITEM<wsp> DATA, OFF ON 0 1	
DUTCH***; #####.##	×	-	

App

## List of the AQ6317-Compatible Commands

AQ6317 Series Control Command	Operates in AQ6317- Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
DUTCHF***;	x	-	
###.###			
DUTLEV**.*	x	-	
DUTSNR**.*	x	-	
EDFCVF*	x	-	
EDFTH**.*	x	-	
EDNF	x	-	
ENVK**.*	o	:CALCulate:PARameter[:CATegory]: SWENvelope:K<wsp><NRf>	
ENVT1**.*	o	:CALCulate:PARameter[:CATegory]: SWENvelope:TH1<wsp><NRf>[DB]	
ENVT2**.*	o	:CALCulate:PARameter[:CATegory]: SWENvelope:TH2<wsp><NRf>[DB]	
EXEC**	o	:PROGram:EXECute<wsp><integer>	
EXTRG	o	:TRIGger[:SEQUence]:STATE<wsp> OFF ON 0 1	
FIG*	o	:UNIT:POWer:DIGit<wsp>1 2 3	
FILBTM○;△;***	▲	:CALCulate:PARameter[:CATegory]: FILBtm<wsp><item>,<paramater>,<data>	
FILBTMAN	o	:CALCulate:CATegory<wsp>FILBtm 14	
FILPKO○;△;***	▲	:CALCulate:PARameter[:CATegory]: FILPk<wsp><item>,<paramater>,<data>	
FILPKAN	o	:CALCulate:CATegory<wsp>FILPk 13	
FIXA	o	:TRACe:ATTRibute:TRA<wsp>FIX 1	
FIXB	o	:TRACe:ATTRibute:TRB<wsp>FIX 1	
FIXC	o	:TRACe:ATTRibute:TRC<wsp>FIX 1	
FMKR****.****	▲	:CALCulate:MARKer:X<wsp>0,<NRf>[HZ]	Diff. parameter range
FPAN	o	:CALCulate:CATegory<wsp>FPLD 5	
FPLD○;△;****	▲	:CALCulate:PARameter[:CATegory]: FPLD<wsp><item>,<paramemter>,<data>	
GP2ADR**	o	:SYSTem:COMMunication:GP-IB2: ADDReSS<wsp><integer>	
GRCOL*	▲	-	Valid only when the parameter is 0 or 1
GRFMT*	o	-	
HD*	o	-	
HELP*	x	-	
*IDN?	o	*IDN?	
INIT	o	:SYSTem:PRESet	
KABC	o	:CALCulate:MATH:TRC<wsp>1-K(A/B)	
KABCK****.****	o	:CALCulate:MATH:TRC:K<wsp><NRf>	
KBAC	o	:CALCulate:MATH:TRC<wsp>1-K(B/A)	
KYDNE	x	-	
L1FMK****.****	▲	:CALCulate:LMARKer:X<wsp>1,<NRf>[HZ]	Diff. parameter range
L1MK****.*	▲	:CALCulate:LMARKer:X<wsp>1,<NRf>[M]	Diff. parameter range

## List of the AQ6317-Compatible Commands

<b>AQ6317 Series Control Command</b>	<b>Operates in AQ6317-Comp Mode</b>	<b>AQ6370C/AQ6375/AQ6370D/AQ6373/AQ6373B Control Command Corresponding to AQ6317 Command</b>	<b>Remarks</b>
L1MK?	▲	:CALCulate:LMARker:X?<wsp>1	Diff. parameter range
L2FMK****.***	▲	:CALCulate:LMARker:X<wsp>2,<NRf>[HZ]	Diff. parameter range
L2MK****.***	▲	:CALCulate:LMARker:X<wsp>2,<NRf>[M]	Diff. parameter range
L2MK?	▲	:CALCulate:LMARker:X?<wsp>2	Diff. parameter range
L3DB****.**	▲	:CALCulate:LMARker:Y<wsp>3,<NRf>[DB]	Diff. parameter range
L3DBM****.**	▲	:CALCulate:LMARker:Y<wsp>3,<NRf>[DBM]	Diff. parameter range
L3LN*.***E±**	▲	:CALCulate:LMARker:Y<wsp>3,<NRf>	Diff. parameter range
L3MK?	▲	:CALCulate:LMARker:Y?<wsp>3	Diff. parameter range
L4DB****.**	▲	:CALCulate:LMARker:Y<wsp>4,<NRf>[DB]	Diff. parameter range
L4DBM****.**	▲	:CALCulate:LMARker:Y<wsp>4,<NRf>[DBM]	Diff. parameter range
L4LN*.***E±**	▲	:CALCulate:LMARker:Y<wsp>4,<NRf>	Diff. parameter range
L4MK?	▲	:CALCulate:LMARker:Y?<wsp>4	Diff. parameter range
LBL '*****'	▲	:DISPlay[:WINDOW]:TEXT:DATA<wsp><string>	Diff. no. of chars
LBLCL	○	:DISPlay[:WINDOW]:TEXT:CLEAR	
LBLDT*	○	:MMEMory:STORe:DATA:ITEM<wsp>LABel,OFF ON 0 1	
LCALT****;#.###	▲	:CALibration:POWeR:OFFSet:TABLE<wsp><integer>,<NRf> [DB]	Diff. parameter range
LDATAR****-R****	○	:TRACe[:DATA]:X?<wsp><trace name>[,<start point>,<stop point>]	
LDATBR****-R****		:TRACe[:DATA]:Y?<wsp><trace name>[,<start point>,<stop point>]	
LDATCR****-R****		:TRACe[:DATA]:SNUmber?<wsp><trace name>	
WDATAR****-R****			
WDATBR****-R****			
WDATCR****-R****			
DTNUM A			
DTNUM B			
DTNUM C			
LMEM\$\$R****-R****	○		
WMEM\$\$R****-R****			
DTNUM **			

App

## List of the AQ6317-Compatible Commands

AQ6317 Series Control Command	Operates in AQ6317- Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
LDTDIG*	○	-	
LED $\circ$ ; ▲; ****	▲	:CALCulate:PARameter[:CATegory]: LED<wsp><item>,<paramater>,<data>	
LEDAN	○	:CALCulate:CATegory<wsp>LED 6	
LHLD*	○	:DISPlay[:WINDow]:SPLit<wsp>ON 1; :DISPlay[:WINDow]:SPLit:HOLD: LOWer<wsp>OFF ON 0 1	
LMKCL	○	:CALCulate:LMARker:AOFF	
LN $\circ$ G $\circ$ T***.*	○	:DISPlay[:WINDow]:TRACe:Y2[:SCALe]: LENGth<wsp><NRf>[KM]	
LOFSKM***.*	○	:DISPlay[:WINDow]:TRACe:Y2[:SCALe]: OLEvel<wsp><NRf>[DB/KM]	
LOFST***.*	○	:DISPlay[:WINDow]:TRACe:Y2[:SCALe]: OLEvel<wsp><NRf>[DB]	
LOGLMT***	×	-	
LPF	×	-	
LSCL**.*	○	:DISPlay[:WINDow]:TRACe:Y1[:SCALe]: SPACing<wsp>LOGarighmic 0; :DISPlay[:WINDow]:TRACe:Y1[:SCALe]: PDIVision<wsp><integer>[DIV]	
LSUNT*	○	:DISPlay[:WINDow]:TRACe:Y1[:SCALe]: UNIT<wsp>DBM DBM/NM	
LTABS	×	-	
LTALM?	×	-	
LTALMDT?	×	-	
LTATSL*	×	-	
LTATSET	×	-	
LTCH***	×	-	
LTCHCUR***	×	-	
LTINTVL****.*	×	-	
LTL	×	-	
LTLHI***.*	×	-	
LTLLOW***.*	×	-	
LTLVLCTR***.*	×	-	
LTLVLSCL**.*	×	-	
LTREFINI	×	-	
LTREFSET	×	-	
LTREL	×	-	
LTSNR	×	-	
LTSNRCTR***.*	×	-	
LTSNRLIM**.*	×	-	
LTSNRSCL**.*	×	-	
LTSWP	×	-	
LTTIME****	×	-	
LTTCMCUR****	×	-	
LTWL	×	-	
LTWLCTR****.*	×	-	
LTWLLOW**.*	×	-	
LTWLSPN****.*	×	-	
LVSFT***.*	○	:SENSe:CORRection:LEVel:SHIFT<wsp> <NRf>[DB]	

## List of the AQ6317-Compatible Commands

<b>AQ6317 Series Control Command</b>	<b>Operates in AQ6317-Comp Mode</b>	<b>AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command</b>	<b>Remarks</b>
MAXA	○	:TRACe:ATTRibute:TRA<wsp>MAX 2	
MCLR***	▲	:CALCulate:MARKer[:STATe]<wsp><marker>,OFF 0	Diff. parameter range
MEM*	×	-	
MESWL*	○	:SENSe:CORRection:RVELocity: MEDium<wsp>AIR VACuum 0 1	
MIMSK**.*	×	-	
MINB	○	:TRACe:ATTRibute:TRB<wsp>MIN 3	
MKCL	○	:CALCulate:MARKer:AOFF	
MKR***	▲	:CALCulate:MARKer[:STATe]<wsp><marker>, ON 1	Diff. parameter range
MKR?	○	:CALCulate:MARKer:X?<wsp>0	
MKR?****	○	:CALCulate:MARKer:X?<wsp><marker>	Diff. parameter range
MKR1	○	:CALCulate:MARKer[:STATe]<wsp>1, ON 1	
MKR1?	○	:CALCulate:MARKer:X?<wsp>1	
MKR2	○	:CALCulate:MARKer[:STATe]<wsp>2, ON 1	
MKR2?	○	:CALCulate:MARKer:X?<wsp>2	
MKROS*	○	:CALCulate:MARKer:FUNCTION: FORMAT<wsp>OFFSet SPACing 0 1	
MKRPRT	○	:HCOPY[:IMMediate]:FUNCTION:MARKer: LIST	
MKRUP*	○	:CALCulate:MARKer:FUNCTION: UPDate<wsp>OFF ON 0 1	
MKUNT*	○	:CALCulate:MARKer:UNIT<wsp> WAVelength FREQuency 0 1	
MLTMKR*	×	-	
MODFT*	○	:CALCulate:PARAmeter[:CATegory]: SWTHresh:MFIT<wsp>OFF ON 0 1	
MODIF**.*	○	:CALCulate:PARAmeter:COMMON: MDIFF<wsp><NRf>[DB]	
MSKL*	○	:DISPlay[:WINDOW]:TRACe:Y:NMASK: TYPE<wsp>VERTical HORIzontal 0 1	
NCHMOD*	○	:CALCulate:PARAmeter[:CATegory]: NOTCh:TYPE<wsp>PEAK BOTTom 0 1	
NCHTH**.*	○	:CALCulate:PARAmeter[:CATegory]: NOTCh:TH<wsp><NRf>[DB]	
NMSK****	▲	:DISPlay[:WINDOW]:TRACe:Y:NMASK <wsp><NRf>[DB]	Diff. parameter range
NORMC	×	-	Same cmd for TRACE G
GNORMD	○	:DISPlay[:WINDOW]:SPLit<wsp>OFF 0	
NSR	○	:CALCulate:MARKer:MAXimum:NEXT or :CALCulate:MARKer:MINimum:	
NEXTNSRL	○	:CALCulate:MARKer:MAXimum:LEFT or :CALCulate:MARKer:MINimum:LEFT	
NSRR	○	:CALCulate:MARKer:MAXimum:RIGHT or :CALCulate:MARKer:MINimum:RIGHT	

App

## List of the AQ6317-Compatible Commands

AQ6317 Series Control Command	Operates in AQ6317- Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
OFIN***.**	x	-	
OFOUT***.**	x	-	
OPALIGN	o	:CALibration:ALIGN[:IMMEDIATE]	
PKHLD****	o	-	
PKSR	o	:CALCulate:MARKer:MAXimum	
PKSR?	o	-	
PLMES	x	-	• PKHLD**** when PEAK HOLD MODE • EXTRG when EXT TRIGGER MODE
PLMOD?	o	-	
PLMSK**.**	x	-	
PMD	o	:CALCulate:CATegory<wsp>PMD 9	
PMDTH**.**	o	:CALCulate:PARameter[:CATegory]: PMD:TH<wsp><NRf>[DB]	
PMRPT	x	-	
PMRST	x	-	
PMSGL	x	-	
PMSTP	x	-	
PMST?	x	-	
PMUNT*	x	-	
POFS**.**	o	:CALCulate:PARameter[:CATegory]: POWER:OFFSet<wsp><NRf>[DB]	
PRDEL**	o	-	
PREXT	o	-	
PRFED**	▲	:HCOPY[:IMMEDIATE]:FEED	Amount of feed
PRMK**.**	o	:CALCulate:PARameter[:CATegory]: SWPKrms:K<wsp><NRf>	
PRMTH**.*	o	:CALCulate:PARameter[:CATegory]: SWPKrms:TH<wsp><NRf>[DB]	
PWR	o	:CALCulate:CATegory<wsp>POWER 8	
RAVA***	o	:TRACe:ATTRibute:RAVG[:TRA]<wsp> <integer>	
RAVB***	o	:TRACe:ATTRibute:RAVG:TRB<wsp><integer>	
RCLA**	▲	:MEMORY:LOAD<wsp><integer>,TRA	Diff. parameter range
RCLB**	▲	:MEMORY:LOAD<wsp><integer>,TRB	Diff. parameter range
RCLC**	▲	:MEMORY:LOAD<wsp><integer>,TRC	Diff. parameter range
RD*'@@@@'	o	:MMEMory:LOAD:TRACe<wsp> <trace name>,<"file name">,EXTernal <trace name>=TRA TRB TRC	Loads external memory
RD3D*'@@@@'	x	-	
RDDT'@@@@'	o	:MMEMory:LOAD:DATA<wsp> <"file name">,EXTernal	Loads external memory
RDLT'@@@@'	x	-	
RDMEM** '@@@@'	o	:MMEMory:LOAD:MEMory<wsp> <integer>,<"file name">,EXTernal	Loads external memory
RDPRG** '@@@@'	o	:MMEMory:LOAD:PROGram<wsp> <program number>,<"file name">, EXTernal	Loads external memory
RDSET'@@@@'	o	:MMEMory:LOAD:SETting<wsp> <"file ame">,EXTernal	Loads external memory

## List of the AQ6317-Compatible Commands

<b>AQ6317 Series Control Command</b>	<b>Operates in AQ6317-Comp Mode</b>	<b>AQ6370C/AQ6375/AQ6370D/AQ6373/AQ6373B Control Command Corresponding to AQ6317 Command</b>	<b>Remarks</b>
RDTMP'@@@@'	▲	:MMEMory:LOAD:TEMPlate<wsp><template>,<"file name">,EXTerinal<template> = UPPer LOWer TARGet	Loads external memory
REF = M	○	:CALCulate:MARKer:SRLevel	
REF = P	○	:CALCulate:MARKer:MAXimum:SRLevel	
REFL***.*	▲	:DISPlay[:WINDOW]:TRACe:Y1[:SCALe] :SPACing<wsp>LOGarithmic 0; :DISPlay[:WINDOW]:TRACeY1[:SCALe] :RLEVel<wsp><NRf>[DBM]	Diff. parameter range
REFL*.*.*	○	:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: SPACing<wsp>LINEar 1; :DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: RLEVel<wsp><NRf>[MW]	
REFLN*.*.*	○	:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: SPACing<wsp>LINEar 1; :DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: RLEVel<wsp><NRf>[NW]	
REFLP*.*.*	×	-	
REFLU*.*.*	○	:DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: SPACing<wsp>LINEar 1; :DISPlay[:WINDOW]:TRACe:Y1[:SCALe]: RLEVel<wsp><NRf>[UW]	
REFL?	▲	:DISPlay[:WINDOW]:Y1[:SCALe]: RLEVel?	Diff. parameter range
REL*	×	-	
RESCOR*	○	-	
RESLN*.*.*	▲	:SENSe:BANDwidth :BWIDth [:RESolution]<wsp><NRf>[M]	Diff. parameter range
RESLNF***	×	-	
RMSK**.*.*	○	:CALCulate:PARAmeter[:CATegory]: RMS:K<wsp><NRf>	
RMSTH**.*.*	○	:CALCulate:PARAmeter[:CATegory]: RMS:TH<wsp><NRf>[DB]	
RPT	○	:INITIate:SMODe<wsp>REPeat 2; INITiate	
*RST	▲	*RST	Diff. operation
SAVEA**	▲	:MEMory:STORe<wsp><integer>,TRA	Diff. parameter range
SAVEB**	▲	:MEMory:STORe<wsp><integer>,TRB	Diff. parameter range
SAVEC**	▲	:MEMory:STORe<wsp><integer>,TRC	Diff. parameter range
SENS?	○	:SENSe:SENSe?	0 if SENS is set to NORMAL
SD*	○	-	
SEGP****	▲	:SENSe:SWEep:SEGMeNT:POINTs<wsp><integer>	Diff. parameter range
SGL	○	:INITIate:SMODe<wsp>SINGle 1	

App

## List of the AQ6317-Compatible Commands

AQ6317 Series Control Command	Operates in AQ6317- Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
SHI1	▲	:SENSe:SENSe<wp>HIGH1 3; :SENSe:CHOPer<wp>OFF 0	Chopper Unused
SHI2	▲	:SENSe:SENSe<wp>HIGH2 4; :SENSe:CHOPer<wp>OFF 0	Chopper Unused
SHI3	▲	:SENSe:SENSe<wp>HIGH3 5; :SENSe:CHOPer<wp>OFF 0	Chopper Unused
SKM**.*	○	DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:UNIT<wp>DB/KM 2 DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:PDIVisioN<wp><NRf> [DB/KM]	
SLIN*.*	○	DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:UNIT<wp>LINEar 1 DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:PDIVisioN<wp><NRf>	
SLOG**.*	○	DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:UNIT<wp>DB 0 DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:PDIVisioN<wp><NRf> [DB]	
SMEAS	○	:INITiate:SMODe<wp>SEGment 4	
SMID	○	:SENSe:SENSe<wp>MID 2	
SMIN**.*	○	DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:SMINimum<wp><NRf>	
SMINP**.*	○	DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:SMINimum<wp><NRf>[%]	
SMPL***	▲	:SENSe:SWEep:POINTs<wp><integer>	Diff. parameter range
SMSR*	○	:CALCulate:PARameter[:CATegory] :SMSR:MODE<wp>SMSR1 SMSR2	
SNAT	○	:SENSe:SENSe<wp>NAUT 1	
SNHD	○	:SENSe:SENSe<wp>NHLD 0	
SP = LM	○	:CALCulate:LMARker:SSPan	
SPAN***.*	▲	:SENSe:WAvelength:SPAN<wp><NRf>[M]	Diff. parameter range
SPANF***.*	▲	-	Diff. parameter range
SPLIT	○	DISPlay[:WINDoW]:SPLit<wp>ON 1	
SPN = W	○	-	
SPS**.*	○	DISPlay[:WINDoW]:TRACe:Y2[:SCALE]: UNIT<wp>% 3 DISPlay[:WINDoW]:TRACe:Y2[:SCALE]: PDIVisioN<wp><NRf>[%]	
SRLMK*	○	:CALCulate:LMARker:SRAnge<wp> OFF/ON 0 1	
SRMSK***	○	-	
SRQ*	○	*SRE<wp><integer>	
SSE*	×	-	
SSMSK***.*	○	:CALCulate:PARameter[:CATegory]: SMSR:MASK<wp><NRf>[M]	
SSUNT?	○	DISPlay[:WINDoW]:TRACe:Y2 [:SCALE]:UNIT?	

## List of the AQ6317-Compatible Commands

<b>AQ6317 Series Control Command</b>	<b>Operates in AQ6317-Comp Mode</b>	<b>AQ6370C/AQ6375/AQ6370D/AQ6373/AQ6373B Control Command Corresponding to AQ6317 Command</b>	<b>Remarks</b>
STAF***.***	▲	:SENSe:WAVelength:STARt<wsp><NRf>[HZ]	Diff. parameter range
STAWL****.**	▲	:SENSe:WAVelength:STARt<wsp><NRf>[M]	Diff. parameter range
STP	○	:ABORT	
STPF***.***	▲	:SENSe:WAVelength:STOP<wsp><NRf>[HZ]	Diff. parameter range
STPWL****.**	▲	:SENSe:WAVelength:STOP<wsp><NRf>[M]	Diff. parameter range
SW*	○	:CALCulate:CATegory<wsp>SWTHresh 0	
SWDSP*	×	-	
SWENV**.**	○	:CALCulate:PARameter[:CATegory]: SWEnvlope:TH1<wsp><NRf>[DB]	
SWEET?	○	-	
SWPI*****	○	:SENSe:SWEep:TIME:INTerval<wsp> <integer>[SEC]	
SWPM*	○	:SENSe:WAVelength:SRAnge<wsp> OFF ON 0 1	
SWPRM**.**	○	:CALCulate:PARameter[:CATegory]: SWPKrms:TH<wsp><NRf>[DB]	
SWRMS**.**	○	:CALCulate:PARameter[:CATegory]: RMS:TH<wsp><NRf>[DB]	
SWTHR**.**	○	:CALCulate:PARameter[:CATegory]: SWTHresh:TH<wsp><NRf>[DB]	
THRK**.**	○	:CALCulate:PARameter[:CATegory]: SWTHresh:K<wsp><NRf>	
THRTH**.**	○	:CALCulate:PARameter[:CATegory]: SWTHresh:TH<wsp><NRf>[DB]	
TIME?	○	-	
TLDAT*****.**; ***.**;***.**	×	:TRACe:TEMPlate:DATA<wsp> <template>,<wavelength>[M], <level>[DB]	
TLDATCLR	▲	:TRACe:TEMPlate:DATA:ADElete<wsp> <template> <template>=UPPer LOWer TARGET	An active template (UPPER/LOWER/TARGET)
TLDISP*	○	:TRACe:TEMPlate:DISPlay	
TLEXTRA*	▲	:TRACe:TEMPlate:EDIT:ETYPe	An active template (UPPER/LOWER/TARGET)
TLGONO*	○	:TRACe:TEMPlate:GONOgo	
TLSADR**	○	-	
TLSSYNC*	○	-	
TLLVSFT***.**	○	:TRACe:TEMPlate:WAVelength:SHIFT	
TLRESLT?	○	:TRACe:TEMPlate:RESult?	
TLTYPE*	○	:TRACe:TEMPlate:TTYPe	
TLWLSFT****.**	○	:TRACe:TEMPlate:WAVelength:SHIFT	
TRA?	▲	:TRACe:ATTRibute:TRA?	Diff.talker format 2: MAX HOLD / MIN HOLD

App

## List of the AQ6317-Compatible Commands

AQ6317 Series Control Command	Operates in AQ6317- Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
TRB?	▲	:TRACe:ATTRibute:TRB?	Diff. talker format 2: MAX HOLD / MIN HOLD
TRC?	×	:TRACe:ATTRibute:TRC?	
TRFMT*	○	-	
UCWRN*	○	:SYSTem:DISPlay:UNCal<wsp> OFF ON 0 1	
UHLD*	○	:DISPlay[:WINDOW]:SPLit<wsp>ON 1; :DISPlay[:WINDOW]:SPLit:HOLD: UPPer<wsp>OFF ON 0 1	
ULTRA*	○	:DISPlay[:WINDOW]:SPLit<wsp>ON 1; :DISPlay[:WINDOW]:SPLit:POsition<wsp> TRA, UP LOW 0 1	
ULTRB*	○	:DISPlay[:WINDOW]:SPLit<wsp>ON 1; :DISPlay[:WINDOW]:SPLit:POsition <wsp>TRB, UP LOW 0 1	
ULTRC*	○	:DISPlay[:WINDOW]:SPLit<wsp>ON 1; :DISPlay[:WINDOW]:SPLit:POsition <wsp>TRC, UP LOW 0 1	
WARN?	▲	:SYSTem:ERRor[:NEXT]?	
WCAL****.***	▲	:CALibration:WAveLength:EXTernal: SOURce<wsp>LASer 0; CALibration:WAveLength:EXTernal: WAveLength<wsp><NRf>[M]	Diff. parameter range
WCALG****.***	▲	:CALibration:WAveLength:EXTernal: SOURce<wsp>GASCell 1; CALibration:WAveLength:EXTernal: WAveLength<wsp><NRf>[M]	Diff. parameter range
WCALS	○	:CALibration:WAveLength:INTernal [:IMMediate]	
WCALT****;#.###	▲	:CALibration:WAveLength:OFFSet: TABLe<wsp><integer>,<NRf>[DB]	Diff. parameter range
WDMAN	○	:CALCulate:CATegory<wsp>WDM 10	
WDMCHAUT*	×	-	No parameter
WDMCHSW***;#	×	-	
WDMdif**.**	▲	:CALCulate:PARameter[:CATegory] :WDM:MDIFF<wsp><NRf>[DB]	Set only in WDM Analysis, not in NF Analysis
WDMDisp*	▲	:CALCulate:PARameter[:CATegory] :WDM:DTPe<wsp><display type> <display type>=ABSolute 0, RELative 1,MDRift 2,GDRift 3	Diff. parameter 0: ABSOLUTE 1: RELATIVE 3: DRIFT(MEAS) 4: DRIFT(GRID)
WDMSPMSK***	▲	:CALCulate:PARameter[:CATegory] :WDM:DMASK<wsp><NRf>[DB]	Diff. parameter range
WDMDual*	○	:CALCulate:PARameter[:CATegory] :WDM:DUAL<wsp>OFF ON 0 1	
WDMMax***	×	-	No parameter
WDMMR	○	:CALCulate:PARameter[:CATegory] :WDM:MMReset	

## List of the AQ6317-Compatible Commands

<b>AQ6317 Series Control Command</b>	<b>Operates in AQ6317-Comp Mode</b>	<b>AQ6370C/AQ6375/AQ6370D/AQ6373/AQ6373B Control Command Corresponding to AQ6317 Command</b>	<b>Remarks</b>
WDMNOI*	▲	[NOISE_ALGO is Auto Center] (NOISE POI=CTR) :CALCulate:PARameter[:CATEgory] :WDM:NALGo<wsp>ACEnter 2 [NOISE_ALGO is MANUAL Fix] (NOISE POI=CTR) :CALCulate:PARameter[:CATEgory] :WDM:NALGo<wsp>MFIX 1; :CALCulate:PARameter[:CATEgory] :WDM:FALGo<wsp>LINEar 0;	Diff. set value 0: AUTO-FIX 1: AUTO-CTR Set only in WDM Analysis, not in NF Analysis
WDMNOIBW****	○	:CALCulate:PARameter[:CATEgory]: WDM:NBW<wsp><NRf>[M HZ]	
WDMNOIP**.*	▲	:CALCulate:PARameter[:CATEgory]: WDM:FALGo<wsp>LINEar 0; :CALCulate:PARameter[:CATEgory]: WDM:NBW<wsp><NRf>[M]	Valid only when NOISE ALGO is set to MANUAL FIX
WDMOS*	○	:CALCulate:PARameter[:CATEgory]: WDM:RELation<wsp>OFFSet SPACing 0 1	
WDMREF*	×	-	
WDMREFDAT*	×	-	
WDMRH	○	:CALCulate:PARameter[:CATEgory] :WDM:RCH<wsp>0	
WDMRN***	○	:CALCulate:PARameter[:CATEgory] :WDM:RCH<wsp><integer>	
WDMSSLOPE*	○	:CALCulate:PARameter[:CATEgory] :WDM:OSlope<wsp>OFF ON 0 1	
WDMTCOPY	○	:HCOPY[:IMMEDIATE]:FUNCTION :CALCulate:LIST	
WDMTH**.*	▲	:CALCulate:PARameter[:CATEgory] :WDM:TH<wsp><NRf>[DB]	Set only in WDM Analysis, not in NF Analysis
WDMUNT*	×	:CALCulate:MARKer:UNIT<wsp> WAveLength FREQuency 0 1	
WLSFT**.***	○	:SENSe:CORRection:WAveLength: SHIFT<wsp><NRf>[M]	
WMKR****.***	▲	:CALCulate:MARKer:X<wsp>0,<NRf>[M]	Diff. parameter range
WNFAN	○	:CALCulate:CATEgory<wsp>NF 11	
WNFCVF*	▲	:CALCulate:PARameter[:CATEgory]: NF:FALGo<wsp><algorhytm> <algorhytm>=AFIX 0,MFIX 1, ACEnter 2,MCEnte 3	Valid only when ASE ALGO is set to MANUAL FIX or MANUAL CTR
WNFFA**.**	▲	:CALCulate:PARameter[:CATEgory]: NF:FARea<wsp><NRf>[M HZ]	Valid only when ASE ALGO is set to MANUAL FIX
WNFNPF**.**	▲	:CALCulate:PARameter[:CATEgory]: NF:MARea<wsp><NRf>[M HZ]	Valid only when all the following conditions are satisfied 1. ASE ALGO is set to MANUAL FIX or MANUAL CTR 2. FITTING ALGO is set besides LINEAR
WNFOFI**.**	○	:CALCulate:PARameter[:CATEgory]: NF:IOFFset<wsp><NRf>[DB]	
WNFOFO**.**	○	:CALCulate:PARameter[:CATEgory]: NF:OOffset<wsp><NRf>[DB]	
W NFSSE*	×	-	No parameter

App

## List of the AQ6317-Compatible Commands

AQ6317 Series Control Command	Operates in AQ6317- Comp Mode	AQ6370C/AQ6375/AQ6370D/AQ6373/ AQ6373B Control Command Corresponding to AQ6317 Command	Remarks
WR* '0000'	○	:MMEMory:STORe:TRACe<wsp> <trace name>,BIN CSV, <"file name">,EXTernal <trace name>=TRA TRB TRC	Saving to the external memory
WR3D* '0000'	×	-	
WRDT '0000'	○	:MMEMory:STORe:DATA<wsp> <"file name">,EXTernal	Saving to the external memory
WRGR'0000'	○	:MMEMory:STORe:GRAphics<wsp> B&W COLOR,BMP TIFF,<"file name">, EXTernal	Saving to the external memory
WRMEM** '0000'	○	:MMEMory:STORe:MEMory<wsp> <integer>,BIN CSV,<"file name">, EXTernal	Saving to the external memory
WRPRG** '0000'	○	:MMEMory:STORe:PROGram<wsp> <integer>,<"file name">,EXTernal	Saving to the external memory
WRSET'0000'	○	:MMEMory:STORe:SETTING<wsp> <"file name">,EXTernal	Saving to the external memory
WRTA	○	:TRACe:ATTRibute:TRA<wsp>WRITe 0	
WRTB	○	:TRACe:ATTRibute:TRB<wsp>WRITe 0	
WRTC	○	:TRACe:ATTRibute:TRC<wsp>WRITe 0	
WRTLTT'0000'	×	-	
XUNT*	○	:UNIT:X<wsp>WAveLength FREQuency   0 1	
ZSCL**	×	-	
ZSWPT**	○	:SENSe:SWEep:TIME:ONM<wsp> <integer>[SEC]	

# HIGH1, HIGH2, HIGH3 of Measurement Sensitivity

## For the AQ6370C, AQ6373, AQ6370D or AQ6373B

Even when the measurement sensitivity of the instrument is set to HIGH1 or HIGH2 or HIGH3, the chopper cannot operate unless the CHOP MODE setting of the SENS/MODE key is set to SWITCH. However, with AQ6317 series instruments, if the measurement sensitivity is set to HIGH1, HIGH2, or HIGH3, a chopper that removes monochrometer stray light is activated. The instrument includes the following AQ6317-compatible mode commands that allow you to edit the settings of the chopper operation.

AQ6317 command to use to set the chopper operation

Control command

CHOP\*

\*: 0 = Chopper OFF, 2 = SWITCH mode

Query command

CHOP?

A return value: Same as the above

## For the AQ6375

When the measurement sensitivity is set to HIGH1, HIGH2, or HIGH3, a chopper that removes monochrometer stray light is activated.

App

# Index

	Page
<b>A</b>	
ADVANCE .....	8-46
ANALYSIS .....	7-13, 8-36
ANALYSIS setting parameters .....	7-20
AQ6317-Compatible Commands.....	App-4
AQ6317-Compatible Mode.....	App-2
AQ6317 Status Byte.....	App-3
<b>B</b>	
Baud Rate.....	4-7
Buffer.....	1-3
<b>C</b>	
CALCulate Sub System Command .....	7-43
CENTER.....	7-4, 8-19
Chromaticity coordinates.....	7-101
COLOR.....	7-13, 7-99
Color analysis.....	7-48
Command Modes .....	App-1
Common Commands.....	7-37
Computer Name .....	3-6
Condition Judgement.....	8-52
COPY .....	7-19
<b>D</b>	
Data Inquiry .....	1-4
Device Clear .....	2-7
Device Trigger .....	1-4
DFB-LD.....	7-98
DISPLAY.....	7-7, 8-30
Displaying the OUTPUT WINDOW .....	8-11
Dominant wavelength.....	7-101
dominant wl .....	7-101
<b>E</b>	
EDFA-NF .....	7-99
Editing Parameters .....	8-6
ENVELOPE .....	7-98
Error Buffer .....	1-3
Error Numbers .....	8-13
Ethernet.....	3-1
Ethernet Interface Specifications.....	3-1
Executing a Program.....	8-9
External Control.....	8-53
<b>F</b>	
FEED .....	7-19
FIBER CORE SIZE.....	7-6, 8-25
FILE .....	7-14, 8-41
FILTER-BTM.....	7-99
FILTER-PK .....	7-99
Flow Control .....	4-7
FORMAT Sub System Command.....	7-76
FP-LD .....	7-98
Function Commands .....	8-5
<b>G</b>	
General Commands .....	8-49
GP-IB .....	2-1
GP-IB1 port.....	2-1
GP-IB2 port.....	2-1, 5-1
GP-IB address .....	2-5, 5-4
GP-IB Cable .....	2-1
GP-IB Interface Specifications.....	2-4
GTL.....	2-7
<b>H</b>	
HCOPY Sub System Command.....	7-76
HIGH1 to 3.....	App-17
<b>I</b>	
IFC.....	2-7
INITiate Sub System Command .....	7-77
Input Buffer .....	1-3
<b>L</b>	
LED.....	7-98
LEVEL .....	7-5, 8-22
Listener Function .....	2-3
List of Function Commands .....	8-18
Lists of Special Commands .....	8-49
Local .....	1-2, 2-3
Local Lockout .....	2-7
Loop Control .....	8-49
<b>M</b>	
MARKER .....	, 7-10
MEMORY .....	7-14, 8-40
MEMory Sub System Command .....	7-77
Merging a Copied Program .....	8-4
Message Terminators .....	1-3
MMEMory Sub System Command .....	7-78
Multiline Messages .....	2-8
<b>N</b>	
NOTCH .....	7-98
<b>O</b>	
Operation Condition Register .....	6-8
Operation Event Register .....	6-8
OSNR (WDM).....	7-13
Output Buffer .....	1-3
Output of Analysis Results .....	7-98
OUTPUT WINDOW .....	8-11
Overlappable Commands .....	7-1
Overlapping Commands .....	7-1

Index  
Index

## Index

	Page
<b>P</b>	
Parity Rate.....	4-7
PEAK SEARCH.....	7-12, 8-35
PK-RMS.....	7-98
PMD.....	7-98
POWER.....	7-98
Print Output.....	8-51
PROGRAM.....	7-15
PROGRAM EDIT.....	8-1
Program Editing Operations.....	8-5
program functions.....	8-1
PROGRAM NAME.....	8-2
PROGram Sub System Command.....	7-82
<b>Q</b>	Page
Questionable Condition Register.....	6-11
Questionable Event Enable Register.....	6-11
Questionable Event Register.....	6-11
<b>R</b>	Page
Remote.....	1-2, 2-3
Remote Commands.....	1-3
Remote Command Tree.....	7-29
REMOTE PORT NO.....	3-5
REN.....	2-7
RMS.....	7-98
RS-232.....	4-1
Rules of Syntax.....	7-1
<b>S</b>	Page
Sample Program.....	2-9, 3-8, 8-59
SDC.....	2-7
SENSe Sub System Command.....	7-83
Sequential Commands.....	7-1
Serial Poll Disable.....	2-7
Serial Poll Enable.....	2-7
Service Request Enable Register.....	6-4
SETUP.....	7-6, 8-24
SMOOTHING .....	7-6, 8-25
SMSR.....	7-98
SPAN.....	7-4, 8-20
Special Commands.....	8-5
Specifications.....	4-1, 5-2
SPEC WIDTH.....	7-20
Standard Event Status Enable Register.....	6-6
Standard Event Status Register.....	6-6
Status Byte Register.....	6-4
Status Register Overview Diagram .....	6-2
Status Registers.....	6-1
STATUs Sub System Command.....	7-86
Substitution of Measuring Conditions.....	8-55
SWEEP.....	7-4, 8-18
SYSTEM.....	7-16, 8-47
SYStem Sub System Command .....	7-87
<b>T</b>	Page
Talker Function .....	2-3
TCP/IP .....	3-4
THRESH.....	7-98
TRACE.....	7-8, 8-26
TRACe Sub System Command.....	7-91
TRIGger Sub System Command.....	7-95
Types of Commands.....	7-1
<b>U</b>	Page
UNIT Sub System Command .....	7-97
User I/O .....	8-56
<b>V</b>	Page
Variable Calculations.....	8-50
<b>W</b>	Page
WDM.....	7-98
WDM FIL-BTM.....	7-99
WDM FIL-PK .....	7-99
<b>X</b>	Page
x col .....	7-101
<b>Z</b>	Page
ZOOM.....	7-7, 8-28